

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024067.D
 Acq On : 17 Dec 2021 16:16
 Operator : SY/MD
 Sample : M5090-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	38002	38583	14.68%	1.721%
2	1.564	156	163	171	rBV	33092	36824	14.01%	1.642%
3	2.105	321	331	345	rVB	64687	91581	34.84%	4.084%
4	2.507	446	456	469	rVB3	4299	7009	2.67%	0.313%
5	3.908	883	892	925	rBV2	15146	62900	23.93%	2.805%
6	4.349	1014	1029	1054	rVB2	48486	121761	46.32%	5.430%
7	5.050	1230	1247	1267	rBV2	102365	255476	97.19%	11.394%
8	5.616	1412	1423	1448	rBV2	92980	196108	74.60%	8.746%
9	5.912	1504	1515	1529	rBV3	3155	6055	2.30%	0.270%
10	6.069	1552	1564	1584	rBV2	59694	122924	46.76%	5.482%
11	6.989	1840	1850	1870	rBV2	26838	50811	19.33%	2.266%
12	7.317	1939	1952	1968	rBV	118936	207617	78.98%	9.259%
13	7.625	2039	2048	2070	rBV3	15905	30342	11.54%	1.353%
14	8.091	2184	2193	2234	rBV	95555	228166	86.80%	10.176%
15	8.854	2418	2430	2452	rBV	157519	262870	100.00%	11.724%
16	10.217	2844	2854	2870	rBV2	42655	68538	26.07%	3.057%
17	10.381	2897	2905	2911	rBV5	2110	2962	1.13%	0.132%
18	11.249	3164	3175	3197	rBV	166554	254478	96.81%	11.349%
19	11.625	3278	3292	3313	rBV	120764	192329	73.17%	8.578%
20	12.249	3475	3486	3495	rBV2	3278	4914	1.87%	0.219%




Sum of corrected areas: 2242248

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024067.D
Acq On : 17 Dec 2021 16:16
Operator : SY/MD
Sample : M5090-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

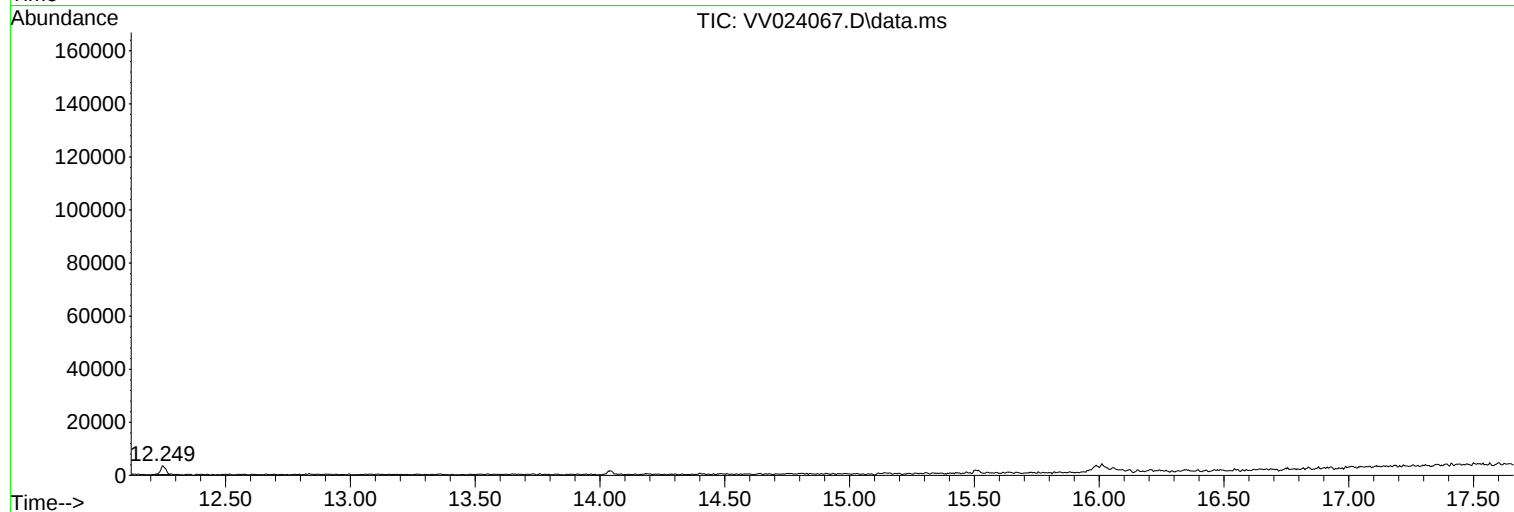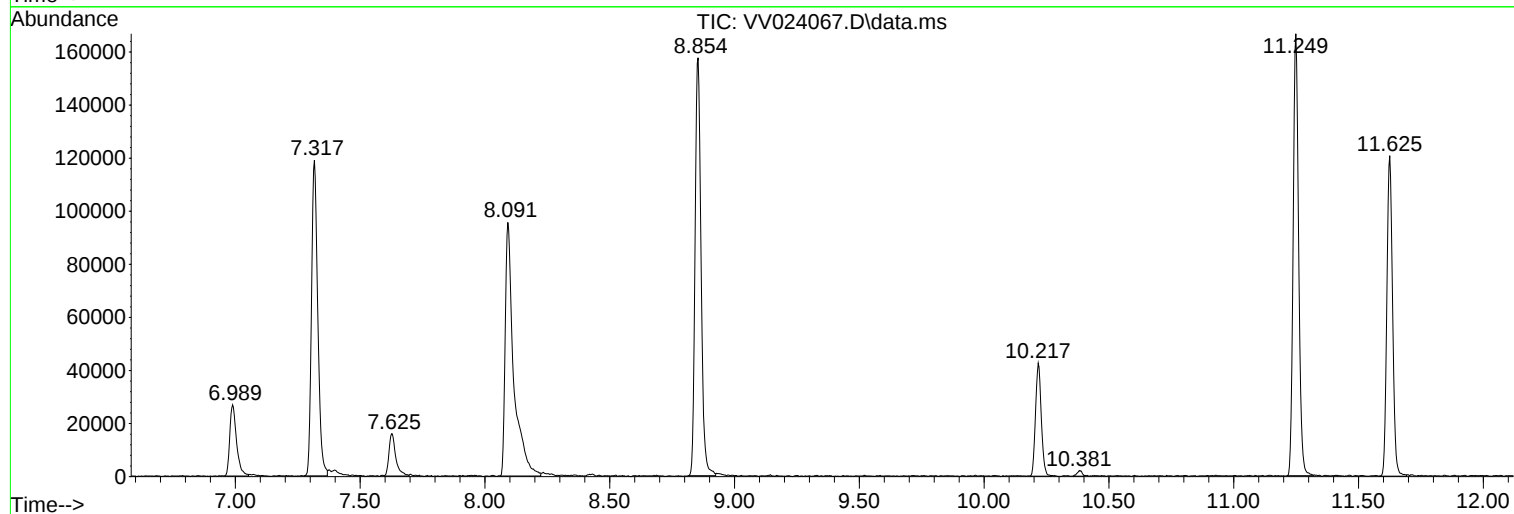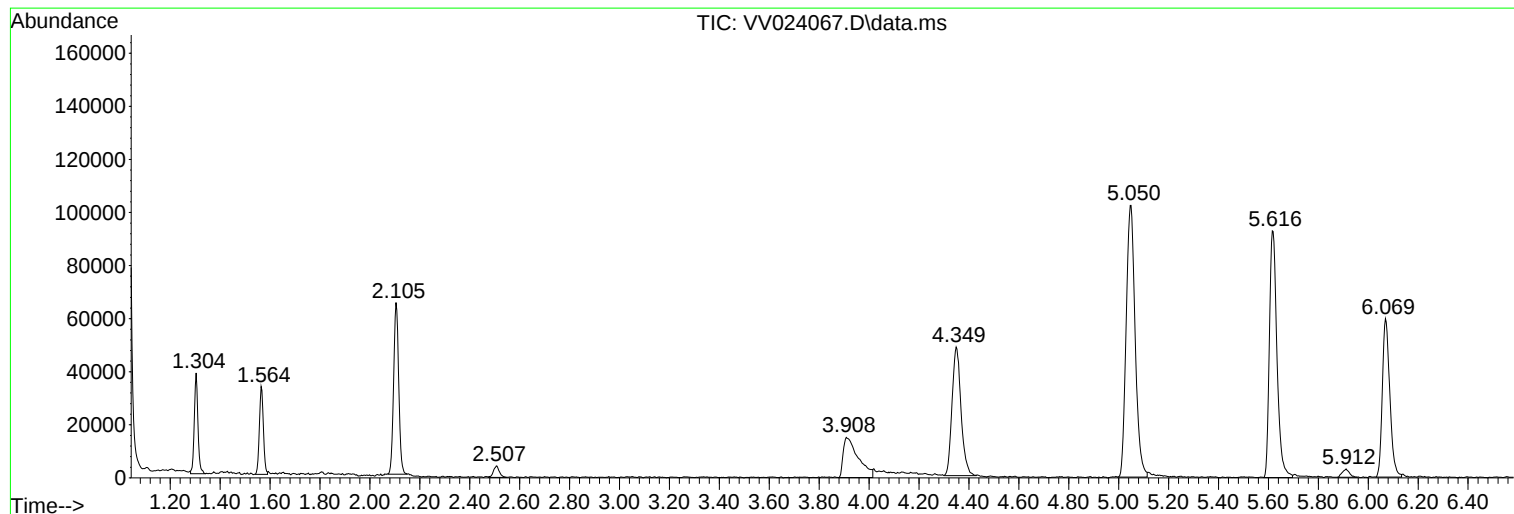

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024067.D
Acq On : 17 Dec 2021 16:16
Operator : SY/MD
Sample : M5090-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024067.D
Acq On : 17 Dec 2021 16:16
Operator : SY/MD
Sample : M5090-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc