

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024079.D
 Acq On : 17 Dec 2021 21:04
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK247

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	34106	37056	13.80%	1.640%
2	1.568	157	164	174	rBV	31461	35580	13.25%	1.575%
3	2.108	321	332	347	rBV	65392	95011	35.37%	4.206%
4	2.510	447	457	470	rVB3	10897	18742	6.98%	0.830%
5	3.902	879	890	923	rBV2	15506	64663	24.07%	2.862%
6	4.355	1015	1031	1052	rVB	46464	118182	44.00%	5.231%
7	5.047	1229	1246	1274	rBV3	99659	252900	94.16%	11.195%
8	5.616	1410	1423	1444	rBV	93988	196225	73.06%	8.686%
9	5.905	1503	1513	1528	rBV7	3424	7038	2.62%	0.312%
10	6.069	1552	1564	1583	rBV	60140	122300	45.53%	5.414%
11	6.989	1839	1850	1877	rBV	27739	52661	19.61%	2.331%
12	7.317	1941	1952	1971	rBV	117927	204454	76.12%	9.050%
13	7.625	2039	2048	2063	rBV2	15579	28546	10.63%	1.264%
14	8.092	2183	2193	2227	rBV	90971	226668	84.39%	10.034%
15	8.854	2418	2430	2454	rBV	160578	268595	100.00%	11.890%
16	10.217	2844	2854	2870	rBV2	42159	67920	25.29%	3.007%
17	10.384	2898	2906	2915	rBV3	3399	5280	1.97%	0.234%
18	11.249	3163	3175	3196	rBV	162483	255006	94.94%	11.288%
19	11.625	3277	3292	3310	rBV	117866	189158	70.42%	8.373%
20	12.252	3479	3487	3497	rVB2	3612	5325	1.98%	0.236%
21	14.040	4030	4043	4059	rBV	4305	7768	2.89%	0.344%




Sum of corrected areas: 2259078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024079.D
Acq On : 17 Dec 2021 21:04
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

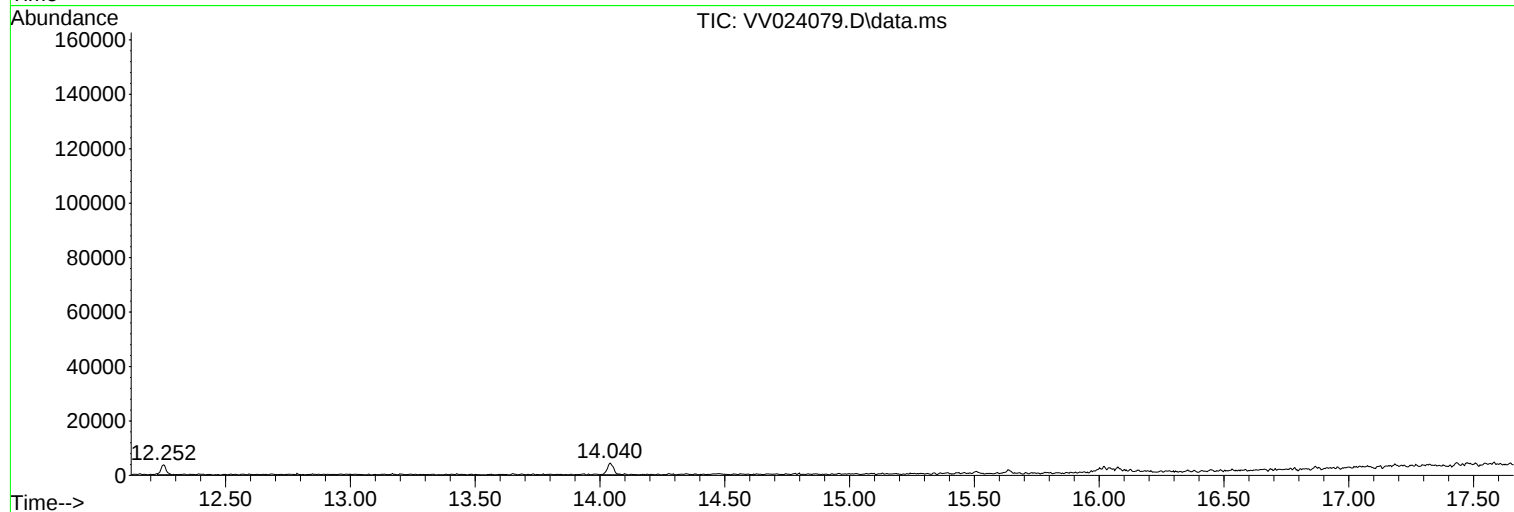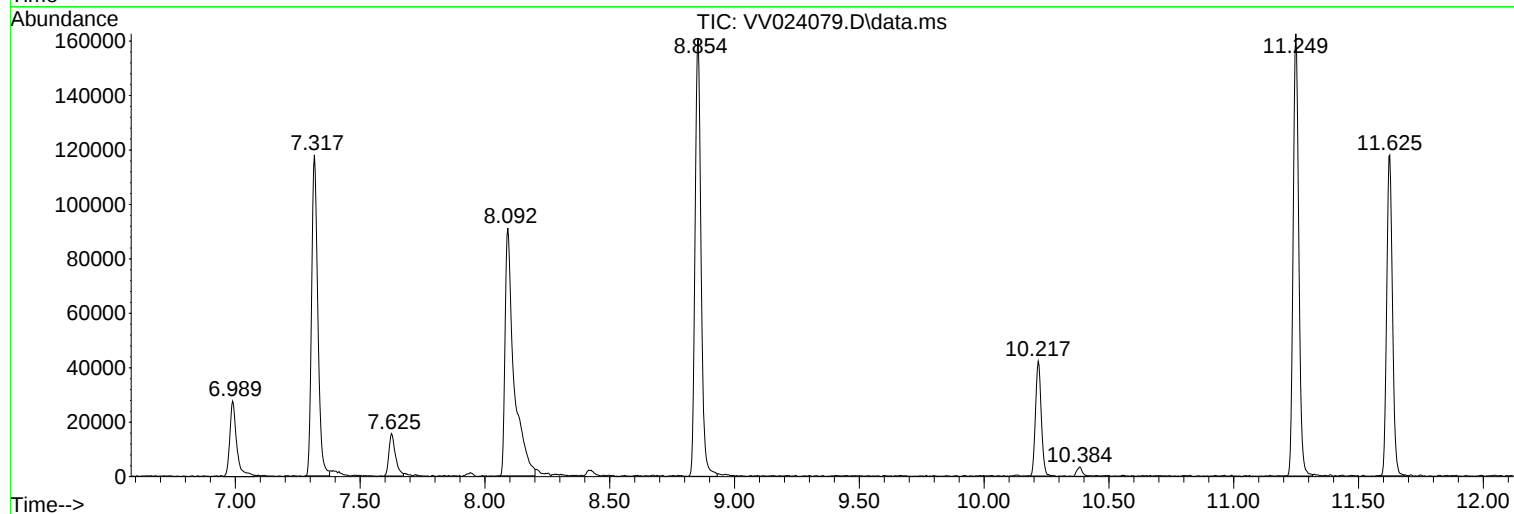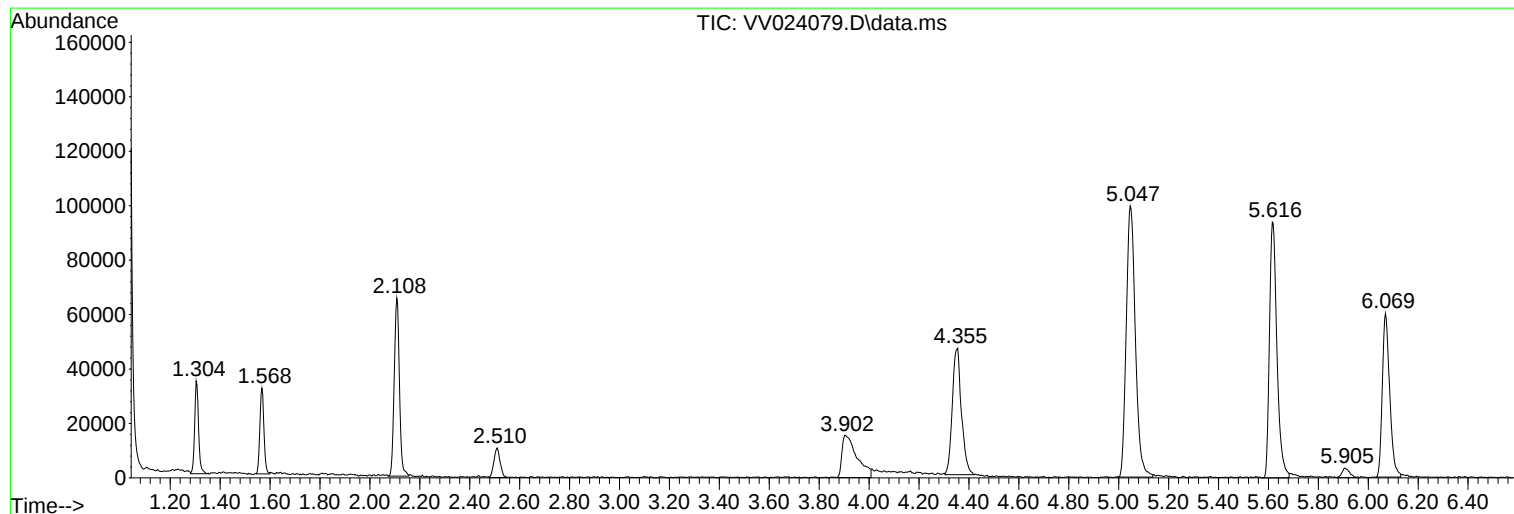

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024079.D
Acq On : 17 Dec 2021 21:04
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024079.D
Acq On : 17 Dec 2021 21:04
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
