
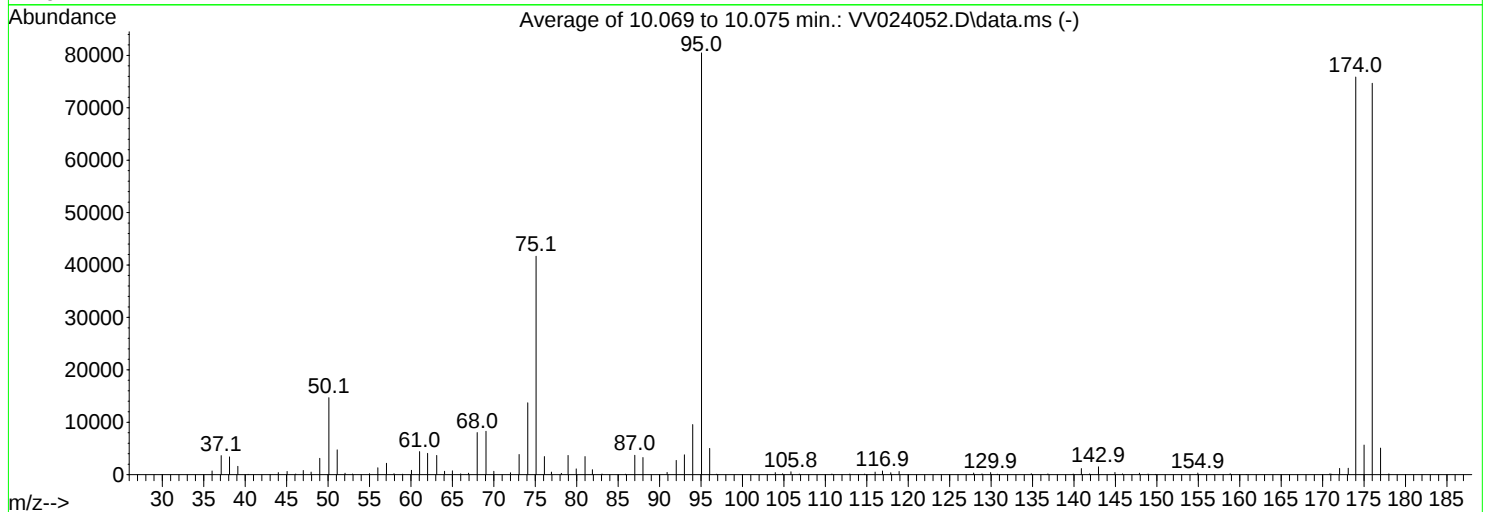


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024052.D
 Acq On : 17 Dec 2021 09:48
 Operator : SY/MD
 Sample : BFB254
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB254

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Dec 20 04:04:22 2021

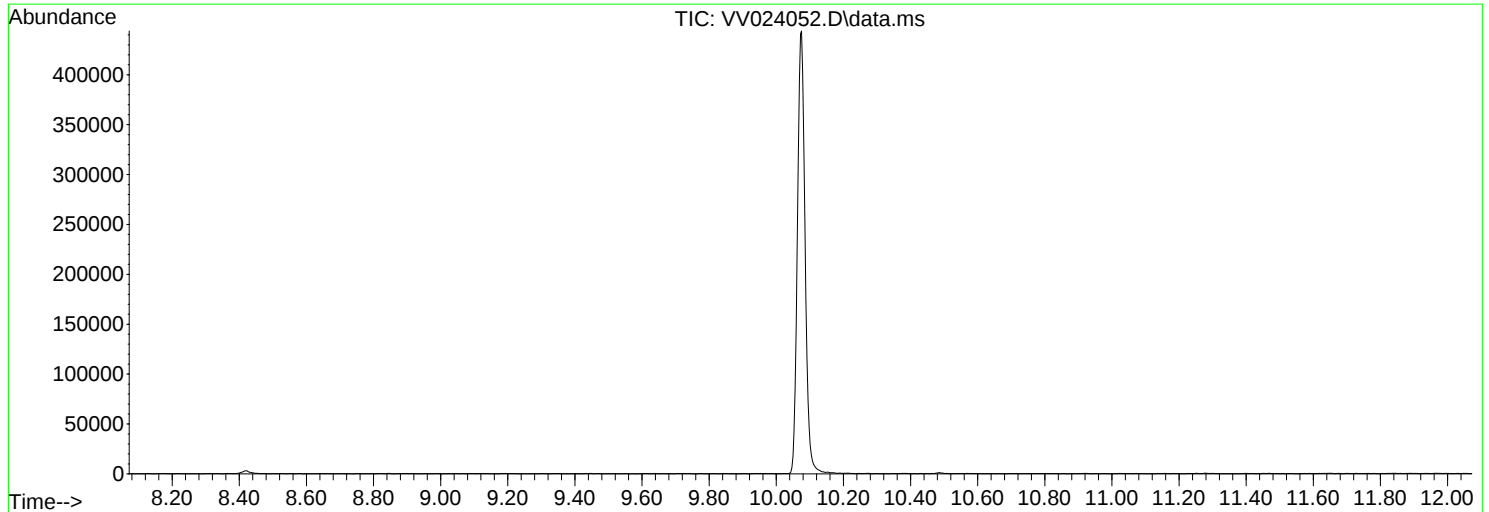

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	14677	PASS
75	95	30	80	51.8	41683	PASS
95	95	100	100	100.0	80488	PASS
96	95	5	9	6.2	5019	PASS
173	174	0.00	2	1.6	1215	PASS
174	95	50	120	94.3	75861	PASS
175	174	5	9	7.4	5647	PASS
176	174	95	105	98.5	74688	PASS
177	176	5	10	6.8	5079	PASS

Scan 2796 (10.030 min): VV024052.D\data.ms
BFB254

m/z	Abundance
39.80	146.0
44.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
36.00	631.0
37.10	3536.0
38.10	3022.0
39.10	1497.0
39.90	125.0
44.00	545.0
45.00	631.0
46.10	114.0
47.00	714.0
47.90	508.0
49.00	3017.0
50.10	13886.0
51.10	4484.0
52.10	210.0
53.00	111.0
55.00	189.0
56.00	1248.0
57.10	1959.0
57.90	153.0
59.00	128.0
60.10	752.0
61.00	4122.0
62.00	3841.0
63.10	3598.0
64.00	561.0
65.00	655.0
66.00	122.0
67.00	274.0
68.00	7606.0
69.10	7721.0
70.00	687.0
72.00	321.0
73.10	3459.0
74.10	13176.0
75.10	39440.0
76.10	3284.0
76.90	451.0
78.20	176.0
79.00	3546.0
80.00	1028.0
81.00	3243.0
81.90	850.0
83.00	115.0
87.00	3423.0
88.00	2937.0
90.90	412.0
92.00	2316.0
93.00	3399.0
94.00	8873.0
95.10	75536.0
96.00	4532.0
103.90	372.0
104.90	185.0
105.90	524.0
106.90	119.0
110.90	151.0
113.00	104.0
114.70	109.0
116.00	468.0
116.90	665.0
117.90	360.0
118.90	601.0
127.90	277.0
128.90	119.0
130.00	334.0
130.80	168.0
134.80	156.0
136.90	161.0
139.80	107.0
140.90	1203.0
141.90	136.0
143.00	1366.0
145.00	373.0
145.90	164.0
147.90	262.0
149.00	106.0
154.90	316.0
158.80	136.0
170.90	249.0
172.10	1064.0
173.10	1038.0
174.00	68624.0
175.00	5301.0
176.00	67960.0
177.00	4724.0
178.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
36.00	723.0
37.10	3807.0
38.10	3532.0
39.10	1680.0
39.90	116.0
40.40	115.0
43.00	103.0
44.10	549.0
45.10	607.0
46.10	128.0
47.00	778.0
47.90	503.0
49.00	3207.0
50.10	15133.0
51.10	4935.0
52.10	287.0
52.90	131.0
55.00	202.0
56.00	1352.0
57.10	2214.0
58.00	199.0
59.00	126.0
60.10	865.0
61.00	4593.0
62.00	4209.0
63.10	3830.0
64.00	652.0
65.00	776.0
66.00	146.0
66.90	287.0
68.00	8386.0
69.00	8600.0
70.00	652.0
72.00	378.0
73.10	3990.0
74.10	14158.0
75.10	43080.0
76.10	3594.0
76.90	504.0
78.10	274.0
79.00	3861.0
79.90	1153.0
81.00	3561.0
81.90	1005.0
83.00	137.0
85.90	107.0
87.00	3883.0
88.00	3352.0
90.90	456.0
92.00	2863.0
93.00	3873.0
94.00	9776.0
95.00	83136.0
96.00	5133.0
96.90	128.0
104.00	431.0
104.90	204.0
105.80	558.0
106.80	141.0
110.80	135.0
113.00	130.0
114.70	128.0
116.00	528.0
116.90	719.0
117.90	400.0
118.90	639.0
127.90	309.0
128.90	132.0
129.90	435.0
130.70	144.0
134.80	170.0
136.90	148.0
139.90	124.0
140.90	1194.0
141.90	141.0
143.00	1555.0
145.00	435.0
145.80	164.0
147.90	298.0
148.90	129.0
149.90	114.0
154.90	309.0
158.90	181.0
170.90	278.0
172.00	1257.0
173.10	1253.0
174.00	78160.0
175.00	5843.0
176.00	76848.0
177.00	5277.0
178.00	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
36.00	734.0
37.10	3585.0
38.10	3632.0
39.10	1617.0
39.90	111.0
40.30	117.0
44.10	514.0
45.10	561.0
46.10	106.0
47.00	874.0
48.00	445.0
49.00	3091.0
50.10	15011.0
51.10	4750.0
52.00	331.0
52.90	147.0
55.00	203.0
56.00	1319.0
57.00	2357.0
58.00	179.0
60.00	879.0
61.10	4516.0
62.00	4182.0
63.10	3562.0
64.10	688.0
65.00	798.0
66.00	164.0
66.90	267.0
68.00	8131.0
69.00	8544.0
70.00	624.0
72.00	392.0
73.00	4072.0
74.10	13793.0
75.10	42528.0
76.10	3520.0
77.00	481.0
78.10	328.0
78.90	3609.0
79.90	1141.0
81.00	3577.0
81.90	966.0
83.10	117.0
85.90	133.0
87.00	3793.0
88.00	3502.0
90.90	408.0
92.00	3017.0
93.00	4123.0
94.00	9991.0
95.00	82792.0
96.10	5392.0
96.90	149.0
104.00	417.0
104.80	198.0
105.80	555.0
106.80	132.0
110.70	107.0
112.90	116.0
114.80	128.0
116.00	473.0
116.90	692.0
117.90	371.0
118.90	583.0
127.90	344.0
128.90	172.0
129.90	477.0
134.90	189.0
136.80	138.0
140.00	155.0
140.90	1085.0
141.90	150.0
142.90	1557.0
144.90	467.0
145.80	141.0
147.90	269.0
148.90	135.0
149.80	124.0
155.00	290.0
156.90	111.0
158.80	208.0
160.80	109.0
171.10	239.0
172.00	1258.0
173.10	1353.0
174.00	80800.0
175.00	5797.0
176.00	79256.0
177.00	5235.0
178.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254