


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121818\
 Data File : VV009009.D
 Acq On : 18 Dec 2018 09:30
 Operator : SY/MD
 Sample : BFB98
 Misc : 5.00 G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB98

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
 Title : VOC Analysis
 Last Update : Fri Dec 21 01:30:11 2018

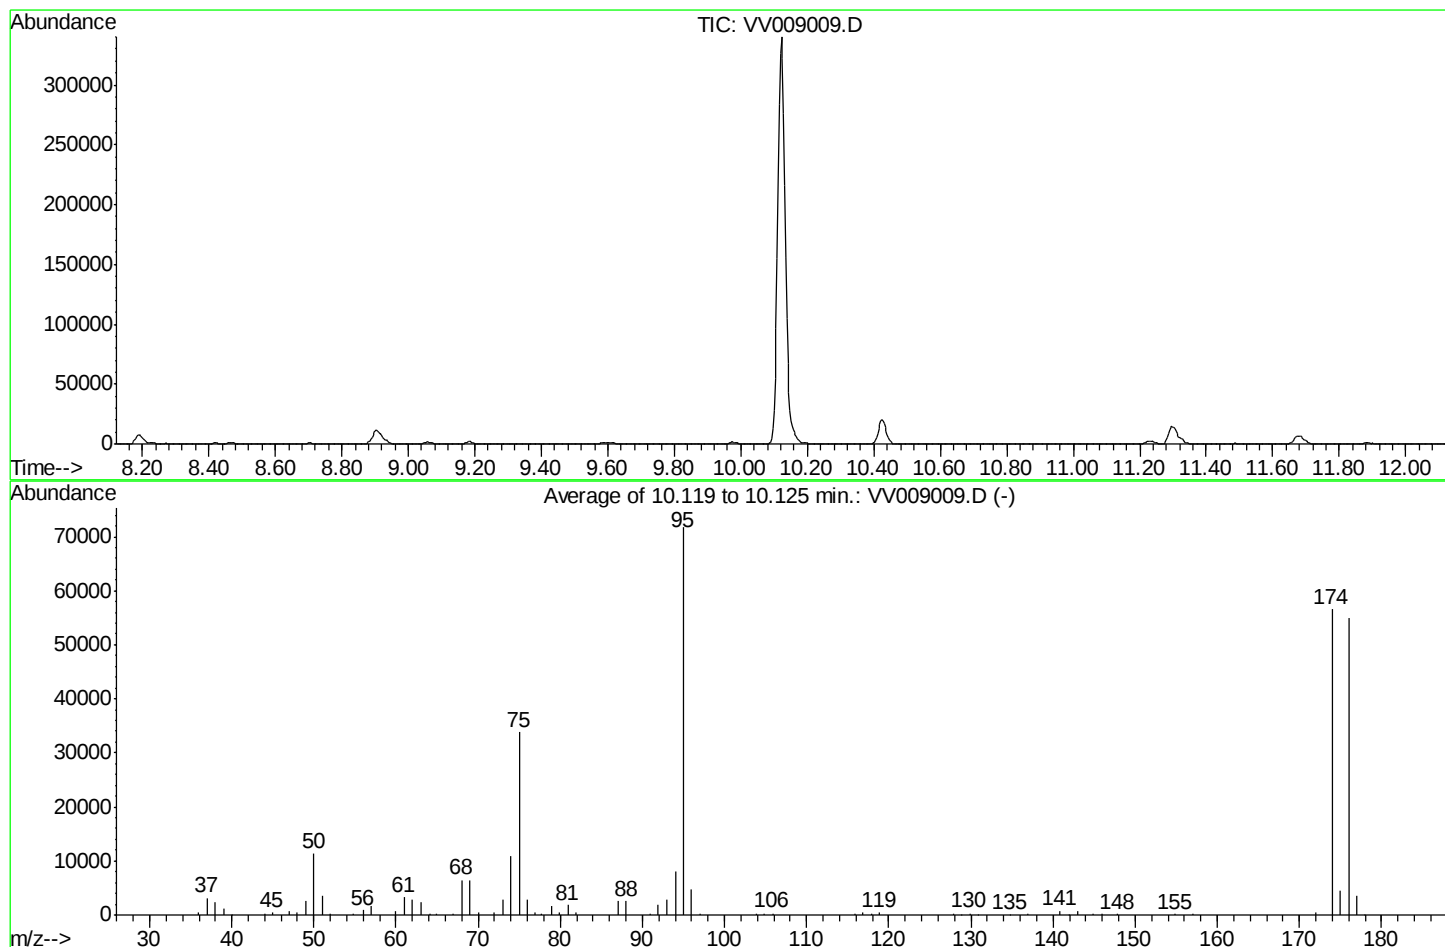

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	11357	PASS
75	95	30	80	47.2	33864	PASS
95	95	100	100	100.0	71738	PASS
96	95	5	9	6.6	4743	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.9	56570	PASS
175	174	5	9	7.8	4432	PASS
176	174	95	101	97.4	55077	PASS
177	176	5	9	6.5	3607	PASS

m/z	Abundance
36.00	508.0
37.00	2990.0
38.00	2504.0
39.00	1052.0
40.00	148.0
44.00	511.0
44.90	476.0
47.00	697.0
48.00	443.0
49.00	2368.0
50.00	11330.0
51.00	3429.0
52.00	154.0
54.80	167.0
56.00	978.0
57.00	1655.0
60.00	630.0
61.00	3320.0
62.00	3078.0
63.00	2442.0
64.10	233.0
65.00	316.0
67.00	168.0
68.00	6488.0
69.00	6489.0
70.00	483.0
71.90	399.0
73.00	2857.0
74.00	11072.0
75.00	33888.0
76.00	2912.0
76.90	346.0
77.70	207.0
78.90	1713.0
79.90	511.0
80.90	1966.0
81.90	460.0
87.00	2769.0
88.10	2371.0
91.00	246.0
92.00	1787.0
93.00	2806.0
94.00	8303.0
95.00	71392.0
96.00	4833.0
97.00	175.0
104.00	282.0
104.90	138.0
105.90	313.0
115.90	312.0
116.90	394.0
117.90	290.0
118.90	372.0
127.90	291.0
129.90	275.0
134.80	118.0
136.90	130.0
140.90	783.0
142.10	121.0
143.00	661.0
144.90	144.0
145.90	125.0
147.90	173.0
154.90	181.0
157.00	140.0
172.10	548.0
174.00	54696.0
175.00	4370.0
176.00	53912.0
177.00	3609.0
177.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
35.90	502.0
37.00	3049.0
38.00	2304.0
39.10	1127.0
40.10	120.0
44.00	461.0
44.90	369.0
47.00	600.0
48.00	315.0
49.00	2591.0
50.00	10994.0
51.00	3439.0
52.00	142.0
54.80	185.0
56.00	874.0
57.00	1526.0
59.90	608.0
61.00	3078.0
62.00	2747.0
63.00	2142.0
64.10	207.0
64.90	319.0
66.90	120.0
67.00	119.0
68.00	6260.0
69.00	6138.0
70.00	577.0
71.90	352.0
73.00	2834.0
74.00	10632.0
75.00	32736.0
76.00	2815.0
77.00	365.0
77.80	257.0
78.90	1759.0
79.90	473.0
80.90	1737.0
81.90	427.0
87.00	2180.0
88.00	2598.0
91.00	266.0
91.90	1876.0
93.00	2650.0
94.00	7396.0
95.00	69552.0
96.00	4484.0
96.90	156.0
103.80	270.0
104.80	121.0
105.80	315.0
115.80	224.0
116.80	352.0
117.90	273.0
118.90	376.0
127.90	263.0
128.80	100.0
129.90	313.0
130.80	108.0
137.00	146.0
140.90	821.0
141.90	122.0
142.90	868.0
144.90	131.0
145.90	175.0
147.90	163.0
154.90	172.0
157.10	115.0
172.00	561.0
174.00	56576.0
175.00	4363.0
176.00	54704.0
177.00	3479.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

Scan 2796 (10.080 min): VV009009.D
BFB98

m/z	Abundance
39.90	122.0
44.00	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	524.0
37.00	3215.0
38.00	2522.0
39.00	1127.0
40.00	126.0
44.00	472.0
44.90	435.0
47.00	678.0
48.00	376.0
49.00	2632.0
50.00	11749.0
51.00	3620.0
52.00	159.0
54.80	199.0
56.00	985.0
57.00	1637.0
60.00	633.0
61.00	3420.0
62.00	3075.0
63.00	2387.0
64.10	226.0
64.90	352.0
67.00	155.0
68.00	6688.0
69.00	6589.0
70.00	537.0
71.90	401.0
73.10	2998.0
74.00	11344.0
75.00	34968.0
76.00	3034.0
77.00	381.0
77.70	250.0
78.90	1864.0
79.90	497.0
80.90	1899.0
81.90	480.0
87.00	2614.0
88.00	2643.0
91.00	259.0
92.00	1894.0
93.00	2872.0
94.00	8300.0
95.00	74272.0
96.00	4912.0
97.00	173.0
104.00	234.0
104.80	140.0
105.80	325.0
115.80	267.0
116.90	389.0
117.90	287.0
118.90	395.0
127.90	278.0
129.90	300.0
130.90	103.0
134.80	108.0
137.00	139.0
140.90	872.0
141.90	121.0
142.90	790.0
144.90	139.0
145.90	166.0
147.90	199.0
154.90	194.0
157.10	138.0
172.00	593.0
174.00	58440.0
175.00	4563.0
176.00	56616.0
177.00	3733.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98