
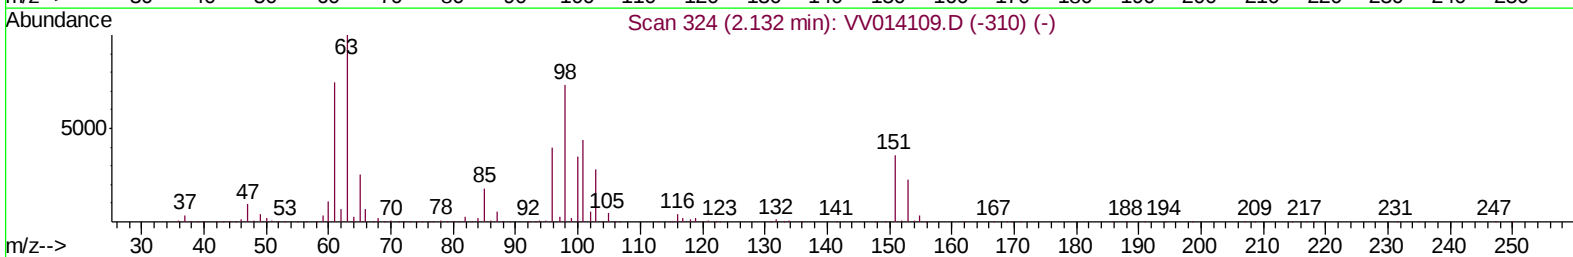
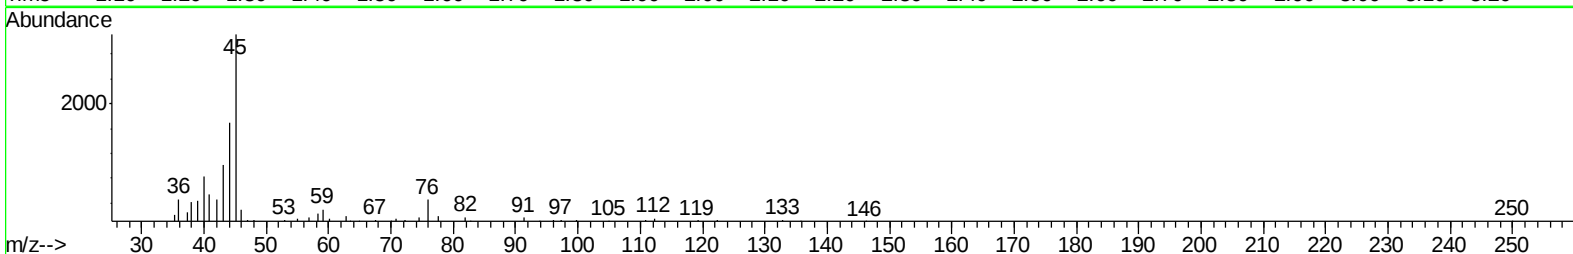


Data File : VV014119.D
Acq On : 18 Dec 2019 14:10
Operator : SY/MD
Sample : K6356-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 07:09:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 19 07:06:05 2019
Response via : Initial Calibration

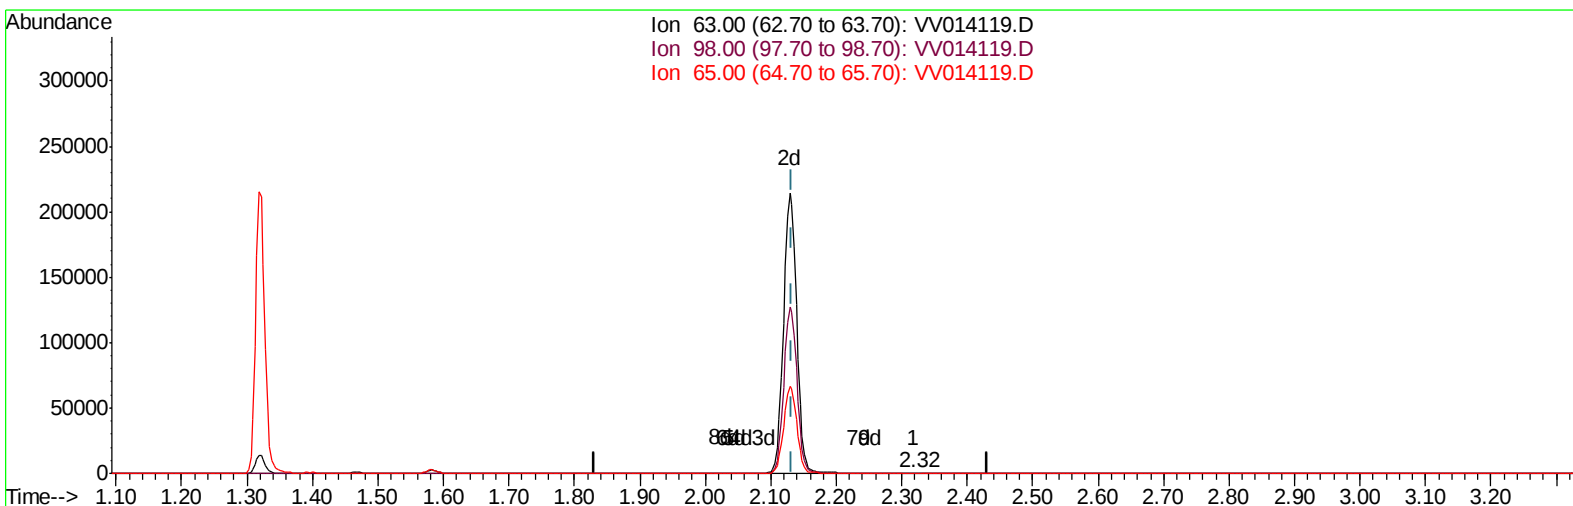

TIC: VV014119.D

(11) 1,1-Dichloroethene-d2 (S)

2.319min (+0.186) 0.03ug/L

response 281

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	55.87
65.00	23.60	22.78
0.00	0.00	0.00