

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014112.D
 Acq On : 18 Dec 2019 11:24
 Operator : SY/MD
 Sample : K6276-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Dec 19 07:38:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 19 07:06:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	745831	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	731264	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	325201	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	230074	53.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.68%
7) Chloroethane-d5	1.58	69	213929	47.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.02%
11) 1,1-Dichloroethene-d2	2.13	63	313556	32.87	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.74%
21) 2-Butanone-d5	3.92	46	301943	99.45	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.45%
24) Chloroform-d	4.40	84	442283	48.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.64%
26) 1,2-Dichloroethane-d4	5.08	65	278440	48.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.02%
32) Benzene-d6	5.10	84	874449	46.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.30%
36) 1,2-Dichloropropane-d6	6.11	67	278449	48.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.90%
41) Toluene-d8	7.36	98	719941	41.68	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.36%
43) trans-1,3-Dichloropropene-	7.66	79	112723	40.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.46%
47) 2-Hexanone-d5	8.13	63	196938	92.73	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.73%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	368671	44.76	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.52%
64) 1,2-Dichlorobenzene-d4	11.67	152	312476	48.92	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.84%


Target Compounds					Ovalue
13) Acetone	2.19	43	5080	1.142 ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\
Data File : VV014112.D
Acq On : 18 Dec 2019 11:24
Operator : SY/MD
Sample : K6276-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Dec 19 07:38:36 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 19 07:06:05 2019
Response via : Initial Calibration

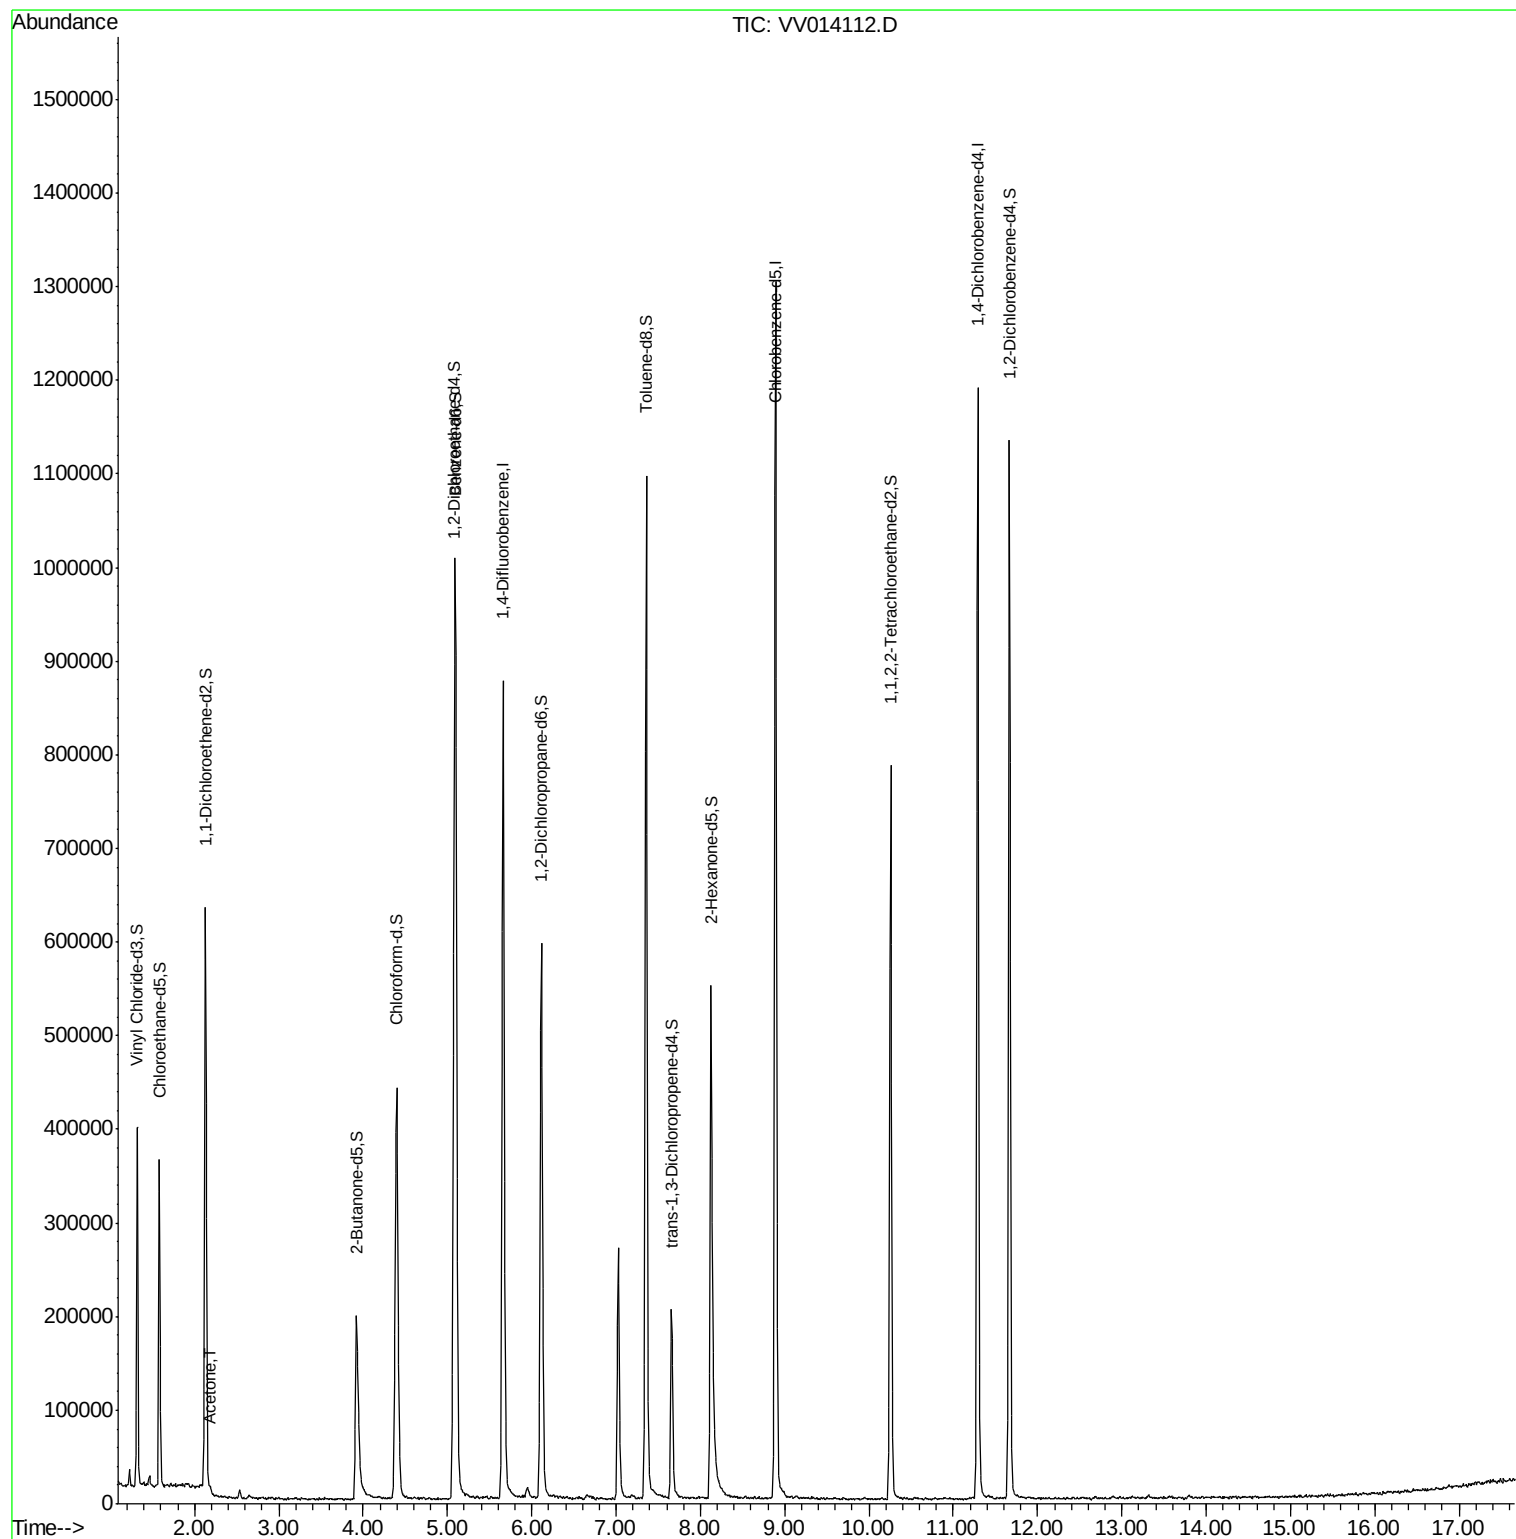

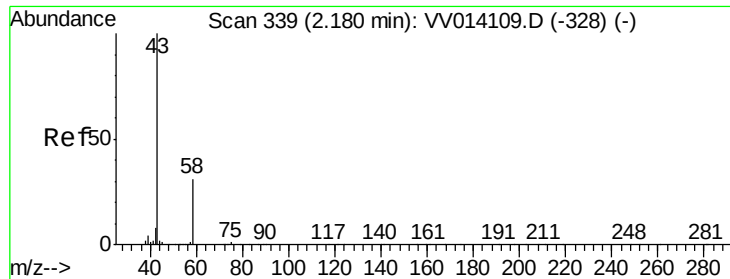

#13

Acetone

Concen: 1.142 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.01 min

Lab File: VV014112.D

Acq: 18 Dec 2019 11:24

Instrument :

MSVOA_V

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 5080

Ion Ratio Lower Upper

43 100

58 44.9 0.0 60.8

