

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\  
 Data File : VV014114.D  
 Acq On : 18 Dec 2019 12:11  
 Operator : SY/MD  
 Sample : K6314-11  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BFF14

Quant Time: Dec 19 07:44:14 2019  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM120219WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Dec 19 07:06:05 2019  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Difluorobenzene     | 5.66  | 114  | 684522   | 50.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 8.89  | 117  | 652976   | 50.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.29 | 152  | 284624   | 50.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |         |       |          |          |      |         |
|--------------------------------|---------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.32    | 65    | 205514   | 51.91    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 60 - 135 | Recovery | =    | 103.82% |
| 7) Chloroethane-d5             | 1.58    | 69    | 194051   | 46.96    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 130 | Recovery | =    | 93.92%  |
| 11) 1,1-Dichloroethene-d2      | 2.13    | 63    | 280253   | 32.01    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 60 - 125 | Recovery | =    | 64.02%  |
| 21) 2-Butanone-d5              | 3.92    | 46    | 300671   | 107.90   | ug/L | 0.00    |
| Spiked Amount                  | 100.000 | Range | 40 - 130 | Recovery | =    | 107.90% |
| 24) Chloroform-d               | 4.40    | 84    | 409309   | 49.23    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 125 | Recovery | =    | 98.46%  |
| 26) 1,2-Dichloroethane-d4      | 5.08    | 65    | 258743   | 49.11    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 125 | Recovery | =    | 98.22%  |
| 32) Benzene-d6                 | 5.10    | 84    | 810119   | 47.88    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 125 | Recovery | =    | 95.76%  |
| 36) 1,2-Dichloropropane-d6     | 6.11    | 67    | 261271   | 51.44    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 120 | Recovery | =    | 102.88% |
| 41) Toluene-d8                 | 7.36    | 98    | 688648   | 44.64    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 80 - 120 | Recovery | =    | 89.28%  |
| 43) trans-1,3-Dichloropropene- | 7.66    | 79    | 109131   | 44.16    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 60 - 125 | Recovery | =    | 88.32%  |
| 47) 2-Hexanone-d5              | 8.13    | 63    | 185259   | 97.69    | ug/L | 0.00    |
| Spiked Amount                  | 100.000 | Range | 45 - 130 | Recovery | =    | 97.69%  |
| 57) 1,1,2,2-Tetrachloroethane- | 10.25   | 84    | 351955   | 47.86    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 65 - 120 | Recovery | =    | 95.72%  |
| 64) 1,2-Dichlorobenzene-d4     | 11.67   | 152   | 277690   | 49.68    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 80 - 120 | Recovery | =    | 99.36%  |


| Target Compounds |      |    |      |            | Ovalue |
|------------------|------|----|------|------------|--------|
| 13) Acetone      | 2.18 | 43 | 4425 | 1.084 ug/L | 91     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\  
Data File : VV014114.D  
Acq On : 18 Dec 2019 12:11  
Operator : SY/MD  
Sample : K6314-11  
Misc : 5.0mL/MSVOA V/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFF14

Quant Time: Dec 19 07:44:14 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM120219WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Dec 19 07:06:05 2019  
Response via : Initial Calibration

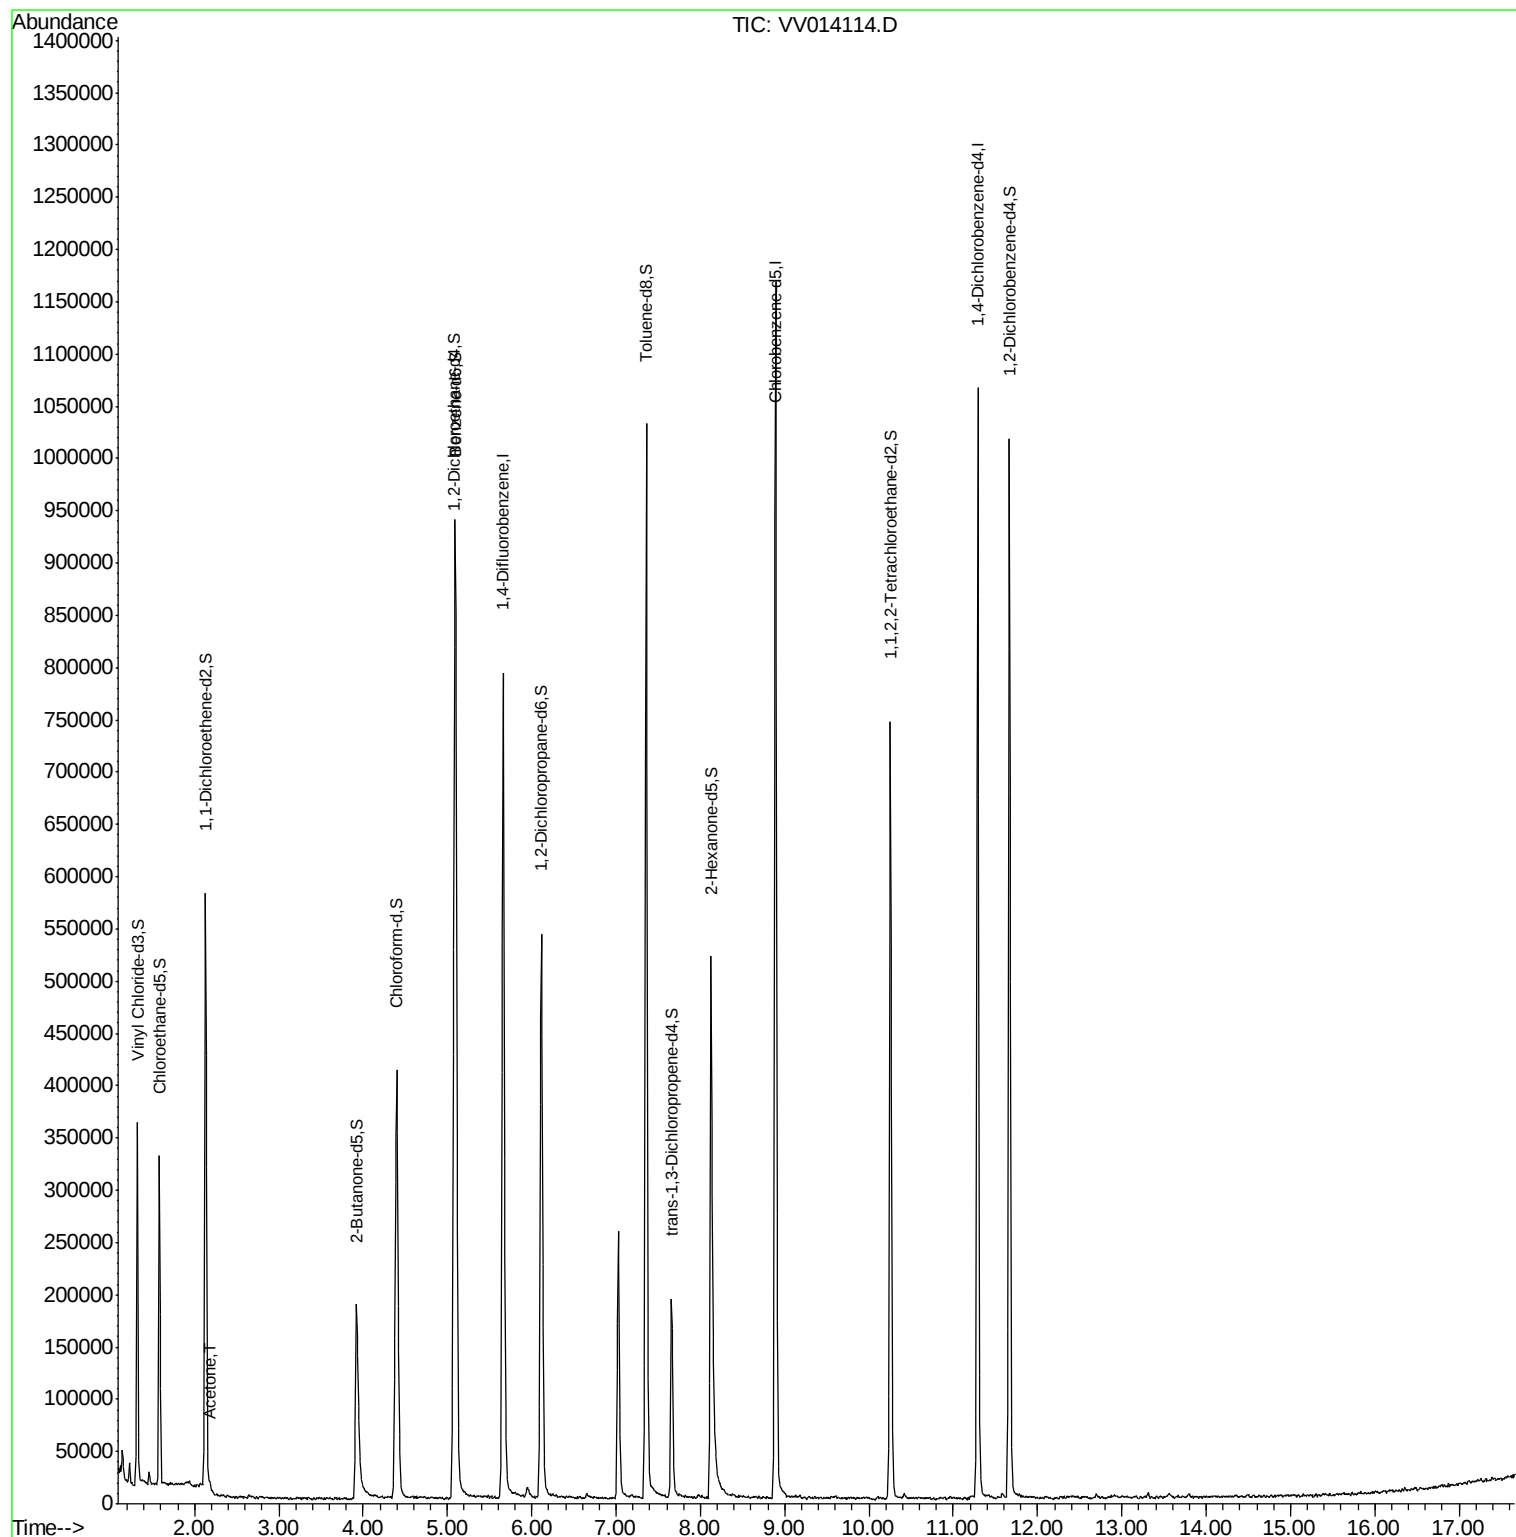

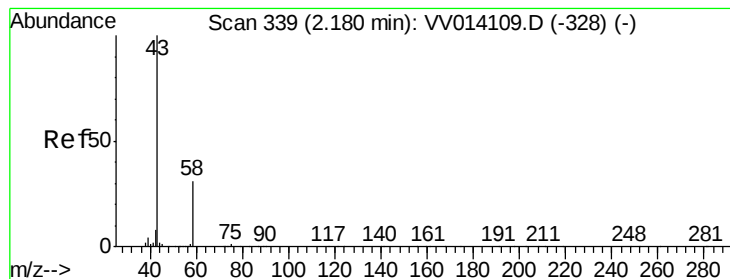

#13

Acetone

Concen: 1.084 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV014114.D

Acq: 18 Dec 2019 12:11

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFF14

Tot Ion: 43 Resp: 4425

Ion Ratio Lower Upper

43 100

58 35.1 0.0 60.8

