

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014112.D
 Acq On : 18 Dec 2019 11:24
 Operator : SY/MD
 Sample : K6276-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	82	rVB	380039	383428	14.96%	1.953%
2	1.582	146	153	171	rVB	350266	391859	15.29%	1.996%
3	2.129	315	323	338	rVB	618548	881363	34.39%	4.488%
4	2.582	461	464	466	rBV4	1680	900	0.04%	0.005%
5	2.762	517	520	523	rBV4	2094	1660	0.06%	0.008%
6	2.869	547	553	554	rBV4	1532	1375	0.05%	0.007%
7	2.907	562	565	567	rBV4	1844	1098	0.04%	0.006%
8	3.071	613	616	619	rBV5	1457	939	0.04%	0.005%
9	3.094	621	623	625	rVV3	1236	569	0.02%	0.003%
10	3.113	625	629	631	rVB4	1692	1084	0.04%	0.006%
11	3.238	663	668	671	rBV7	1927	1891	0.07%	0.010%
12	3.261	671	675	676	rBV4	1271	904	0.04%	0.005%
13	3.479	739	743	745	rBV4	2457	1685	0.07%	0.009%
14	3.495	745	748	750	rVV2	1664	808	0.03%	0.004%
15	3.521	750	756	759	rVB7	1468	1843	0.07%	0.009%
16	3.541	759	762	765	rBV5	2827	1959	0.08%	0.010%
17	3.598	778	780	781	rBV2	1815	719	0.03%	0.004%
18	3.624	786	788	789	rVV2	1734	713	0.03%	0.004%
19	3.634	789	791	794	rVB4	1055	553	0.02%	0.003%
20	3.685	805	807	809	rVB3	1603	590	0.02%	0.003%
21	3.695	809	810	814	rBV3	1064	763	0.03%	0.004%
22	3.772	833	834	837	rBV2	918	559	0.02%	0.003%
23	3.788	837	839	841	rVV3	1557	994	0.04%	0.005%
24	3.814	845	847	850	rBV4	1625	966	0.04%	0.005%
25	3.872	863	865	867	rBV3	1125	615	0.02%	0.003%
26	3.923	870	881	907	rBV	194891	510082	19.90%	2.598%
27	4.315	999	1003	1004	rVB3	1335	733	0.03%	0.004%
28	4.325	1004	1006	1008	rBV3	1201	555	0.02%	0.003%
29	4.396	1013	1028	1054	rVV	438133	1048744	40.92%	5.341%
30	4.676	1112	1115	1117	rBV4	1726	1054	0.04%	0.005%
31	4.714	1124	1127	1129	rBV4	2101	1340	0.05%	0.007%
32	4.749	1136	1138	1140	rBV3	1130	735	0.03%	0.004%
33	4.888	1177	1181	1183	rBV4	1555	1127	0.04%	0.006%
34	4.936	1192	1196	1198	rBV3	1129	836	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014112.D
 Acq On : 18 Dec 2019 11:24
 Operator : SY/MD
 Sample : K6276-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.016	1219	1221	1226	rBV6	1444	1418	0.06%	0.007%
36	5.093	1226	1245	1273	rBV2	1005336	2563195	100.00%	13.053%
37	5.338	1317	1321	1324	rBV5	2146	2129	0.08%	0.011%
38	5.425	1345	1348	1349	rBV3	2408	1304	0.05%	0.007%
39	5.659	1408	1421	1440	rBV	872511	1707664	66.62%	8.696%
40	6.113	1550	1562	1584	rBV	589203	1148870	44.82%	5.851%
41	6.486	1676	1678	1679	rBV2	1757	519	0.02%	0.003%
42	6.499	1679	1682	1686	rVB4	1505	975	0.04%	0.005%
43	6.611	1715	1717	1719	rBV3	1525	622	0.02%	0.003%
44	6.769	1763	1766	1770	rBV5	2774	2022	0.08%	0.010%
45	6.888	1802	1803	1806	rVB2	1342	565	0.02%	0.003%
46	6.904	1806	1808	1810	rBV3	1412	734	0.03%	0.004%
47	6.952	1821	1823	1824	rBV2	1446	563	0.02%	0.003%
48	7.026	1834	1846	1868	rBV	268888	490258	19.13%	2.497%
49	7.283	1922	1926	1929	rBV5	1381	1397	0.05%	0.007%
50	7.357	1936	1949	1969	rBV	1090779	1875583	73.17%	9.551%
51	7.659	2031	2043	2057	rBV	202409	349597	13.64%	1.780%
52	7.881	2107	2112	2114	rBV6	2284	2131	0.08%	0.011%
53	8.126	2176	2188	2225	rBV	547416	1193632	46.57%	6.079%
54	8.476	2294	2297	2298	rBV2	1952	902	0.04%	0.005%
55	8.682	2359	2361	2363	rVB3	1612	641	0.03%	0.003%
56	8.698	2363	2366	2369	rBV5	2764	2127	0.08%	0.011%
57	8.891	2414	2426	2445	rBV	1298507	2096971	81.81%	10.679%
58	9.277	2544	2546	2547	rBV2	1598	609	0.02%	0.003%
59	9.315	2556	2558	2560	rBV3	2194	932	0.04%	0.005%
60	9.380	2576	2578	2582	rVB5	2401	1337	0.05%	0.007%
61	9.399	2582	2584	2590	rVB5	1861	1909	0.07%	0.010%
62	9.434	2590	2595	2596	rBV4	2330	1559	0.06%	0.008%
63	9.460	2601	2603	2604	rBV2	1519	558	0.02%	0.003%
64	9.486	2609	2611	2613	rBV2	1043	610	0.02%	0.003%
65	9.588	2639	2643	2644	rBV3	1532	933	0.04%	0.005%
66	9.740	2687	2690	2692	rBV4	1183	545	0.02%	0.003%
67	9.756	2692	2695	2697	rBV4	1032	583	0.02%	0.003%
68	9.775	2699	2701	2709	rVV9	1140	1382	0.05%	0.007%
69	9.926	2747	2748	2751	rBV3	1083	526	0.02%	0.003%
70	10.061	2787	2790	2792	rBV3	1025	841	0.03%	0.004%
71	10.087	2795	2798	2800	rVB3	1058	605	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014112.D
 Acq On : 18 Dec 2019 11:24
 Operator : SY/MD
 Sample : K6276-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.106	2800	2804	2810	rBV10	1747	2062	0.08%	0.011%
73	10.190	2826	2830	2831	rBV3	1973	1238	0.05%	0.006%
74	10.257	2837	2851	2870	rBV	784234	1252388	48.86%	6.378%
75	10.373	2884	2887	2890	rBV3	2089	1428	0.06%	0.007%
76	10.412	2897	2899	2900	rBV2	1593	687	0.03%	0.003%
77	10.450	2909	2911	2918	rVB7	2475	2310	0.09%	0.012%
78	10.508	2927	2929	2931	rBV3	1217	559	0.02%	0.003%
79	10.531	2933	2936	2937	rBV3	2066	1118	0.04%	0.006%
80	10.630	2964	2967	2970	rVB5	1586	976	0.04%	0.005%
81	10.717	2992	2994	2998	rVB3	1579	830	0.03%	0.004%
82	10.762	3004	3008	3009	rBV2	1597	1184	0.05%	0.006%
83	11.064	3100	3102	3104	rBV2	1550	873	0.03%	0.004%
84	11.129	3120	3122	3124	rBV3	1115	584	0.02%	0.003%
85	11.219	3146	3150	3152	rBV5	1931	1635	0.06%	0.008%
86	11.289	3160	3172	3196	rBV	1185722	1852638	72.28%	9.435%
87	11.595	3266	3267	3271	rBV4	1274	769	0.03%	0.004%
88	11.666	3277	3289	3310	rBV	1128466	1798005	70.15%	9.156%
89	11.858	3347	3349	3350	rBV2	1789	781	0.03%	0.004%
90	12.045	3404	3407	3409	rBV4	1857	1329	0.05%	0.007%
91	12.096	3421	3423	3425	rBV3	1660	571	0.02%	0.003%
92	12.344	3497	3500	3502	rBV4	1816	1086	0.04%	0.006%
93	12.463	3536	3537	3544	rBV7	1923	1406	0.05%	0.007%
94	12.656	3590	3597	3599	rBV8	2470	3162	0.12%	0.016%
95	12.794	3637	3640	3642	rBV2	2020	1232	0.05%	0.006%
96	12.868	3660	3663	3664	rBV3	1732	891	0.03%	0.005%
97	13.051	3717	3720	3723	rBV4	1734	1174	0.05%	0.006%
98	13.370	3817	3819	3824	rVB5	2022	1523	0.06%	0.008%
99	13.399	3824	3828	3830	rBV4	2254	1605	0.06%	0.008%
100	14.196	4075	4076	4080	rVB4	1710	954	0.04%	0.005%


Sum of corrected areas: 19636789

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\
Data File : VV014112.D
Acq On : 18 Dec 2019 11:24
Operator : SY/MD
Sample : K6276-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

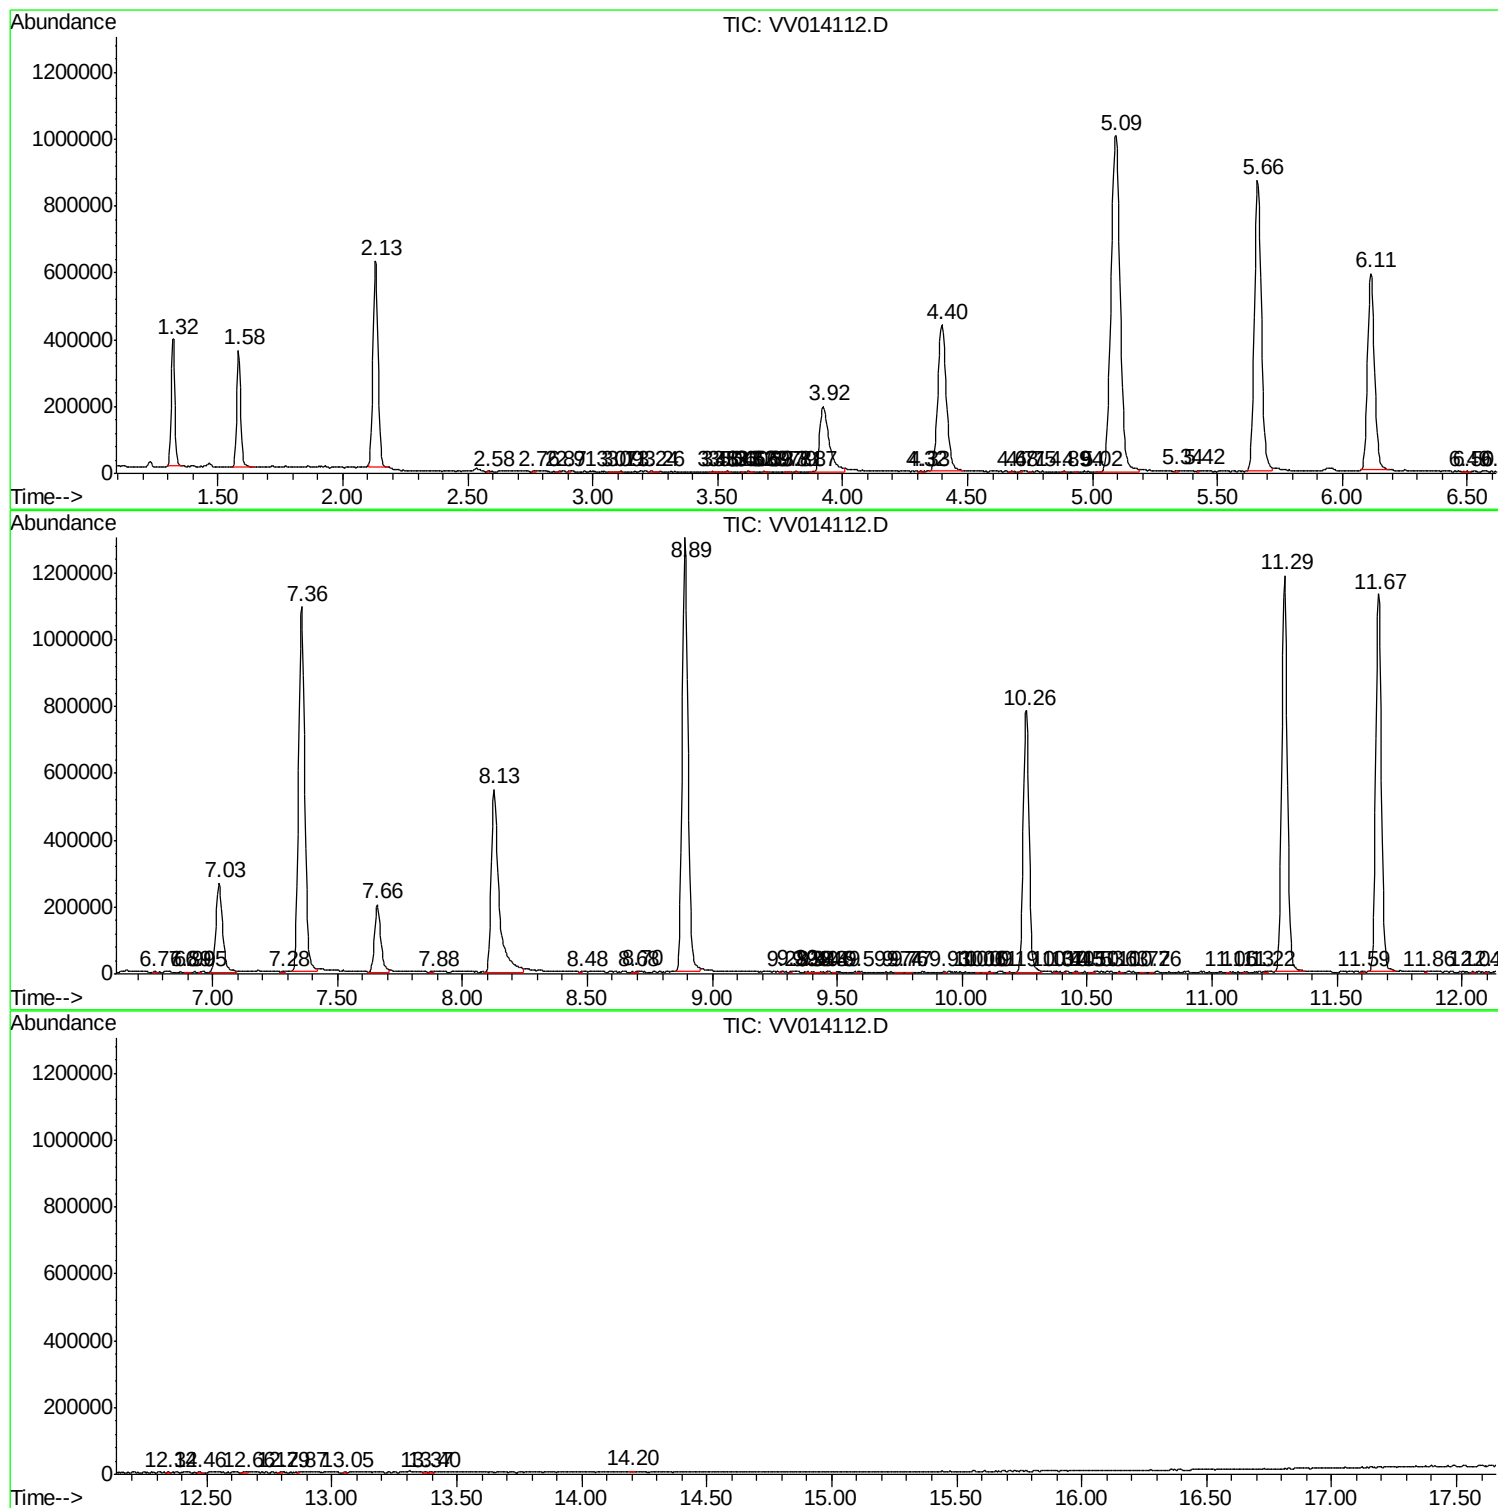

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014112.D
Acq On : 18 Dec 2019 11:24
Operator : SY/MD
Sample : K6276-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121819\
Data File : VV014112.D
Acq On : 18 Dec 2019 11:24
Operator : SY/MD
Sample : K6276-14
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc