

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014114.D
 Acq On : 18 Dec 2019 12:11
 Operator : SY/MD
 Sample : K6314-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	87	rVB	343550	343443	14.40%	1.900%
2	1.582	147	153	163	rVB	312480	345864	14.50%	1.913%
3	2.132	315	324	345	rVB	572082	819774	34.37%	4.535%
4	2.630	476	479	480	rBV3	2551	1436	0.06%	0.008%
5	2.971	582	585	586	rBV2	678	425	0.02%	0.002%
6	3.126	630	633	635	rBV3	1451	898	0.04%	0.005%
7	3.142	635	638	642	rVB4	1424	1148	0.05%	0.006%
8	3.257	672	674	678	rVB5	1614	989	0.04%	0.005%
9	3.277	678	680	681	rBV2	600	232	0.01%	0.001%
10	3.286	681	683	687	rBV4	1460	712	0.03%	0.004%
11	3.302	687	688	690	rBV2	1061	325	0.01%	0.002%
12	3.347	700	702	704	rBV3	1900	1142	0.05%	0.006%
13	3.415	721	723	726	rBV4	1460	857	0.04%	0.005%
14	3.447	730	733	737	rBV3	2514	2133	0.09%	0.012%
15	3.560	766	768	770	rBV3	1503	940	0.04%	0.005%
16	3.618	785	786	787	rBV	956	326	0.01%	0.002%
17	3.650	793	796	797	rBV3	1005	644	0.03%	0.004%
18	3.698	809	811	812	rBV2	1030	392	0.02%	0.002%
19	3.730	820	821	825	rBV4	1226	716	0.03%	0.004%
20	3.798	840	842	844	rVB2	2040	772	0.03%	0.004%
21	3.814	844	847	849	rVB3	1207	755	0.03%	0.004%
22	3.830	849	852	855	rBV4	1573	866	0.04%	0.005%
23	3.846	855	857	861	rVB5	1574	1205	0.05%	0.007%
24	3.875	861	866	869	rBV6	2464	2766	0.12%	0.015%
25	3.923	870	881	908	rBV	185615	489340	20.52%	2.707%
26	4.396	1011	1028	1053	rBV	410000	982480	41.19%	5.435%
27	4.611	1093	1095	1099	rBV4	1954	1395	0.06%	0.008%
28	4.981	1207	1210	1211	rBV2	939	479	0.02%	0.003%
29	5.023	1220	1223	1224	rBV2	1399	838	0.04%	0.005%
30	5.093	1227	1245	1276	rVV2	936754	2385140	100.00%	13.195%
31	5.659	1409	1421	1443	rBV	787210	1552575	65.09%	8.589%
32	6.113	1550	1562	1588	rBV	536339	1075890	45.11%	5.952%
33	6.408	1651	1654	1660	rBV8	2287	2610	0.11%	0.014%
34	6.598	1711	1713	1717	rBV4	1441	1091	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014114.D
 Acq On : 18 Dec 2019 12:11
 Operator : SY/MD
 Sample : K6314-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.859	1791	1794	1796	rBV4	1729	1245	0.05%	0.007%
36	7.026	1833	1846	1870	rBV	256305	474250	19.88%	2.624%
37	7.302	1931	1932	1935	rBV3	1010	392	0.02%	0.002%
38	7.357	1936	1949	1965	rBV	1027738	1781750	74.70%	9.857%
39	7.659	2034	2043	2061	rBV	188308	319103	13.38%	1.765%
40	7.900	2116	2118	2120	rVB3	2173	931	0.04%	0.005%
41	8.084	2172	2175	2177	rVB3	2090	1136	0.05%	0.006%
42	8.129	2178	2189	2219	rBV	518236	1111324	46.59%	6.148%
43	8.791	2392	2395	2401	rVB7	2582	2400	0.10%	0.013%
44	8.820	2401	2404	2406	rBV3	1457	924	0.04%	0.005%
45	8.891	2414	2426	2446	rBV	1164270	1893560	79.39%	10.475%
46	9.270	2541	2544	2545	rBV3	2398	1292	0.05%	0.007%
47	9.357	2568	2571	2576	rVB6	2887	2439	0.10%	0.013%
48	9.386	2576	2580	2582	rBV5	1462	1192	0.05%	0.007%
49	9.418	2588	2590	2592	rBV2	1430	772	0.03%	0.004%
50	9.543	2626	2629	2632	rBV5	2094	1225	0.05%	0.007%
51	9.672	2667	2669	2671	rVB3	1098	435	0.02%	0.002%
52	9.746	2689	2692	2694	rBV4	2646	1723	0.07%	0.010%
53	9.826	2715	2717	2722	rVB5	2295	1882	0.08%	0.010%
54	9.849	2722	2724	2725	rBV2	1919	834	0.03%	0.005%
55	9.955	2756	2757	2758	rBV	1047	347	0.01%	0.002%
56	10.048	2784	2786	2790	rVB3	1495	648	0.03%	0.004%
57	10.067	2790	2792	2793	rVB2	762	242	0.01%	0.001%
58	10.122	2808	2809	2811	rBV2	1255	500	0.02%	0.003%
59	10.164	2820	2822	2826	rVB4	1781	1018	0.04%	0.006%
60	10.183	2826	2828	2829	rVB2	806	283	0.01%	0.002%
61	10.199	2829	2833	2835	rBV5	1403	1185	0.05%	0.007%
62	10.254	2835	2850	2871	rBV	744302	1188386	49.82%	6.574%
63	10.553	2940	2943	2947	rBV5	1468	1226	0.05%	0.007%
64	10.579	2947	2951	2954	rBV5	2219	2238	0.09%	0.012%
65	10.643	2969	2971	2972	rBV	1019	395	0.02%	0.002%
66	10.682	2981	2983	2987	rBV4	1722	1213	0.05%	0.007%
67	10.743	3000	3002	3004	rBV3	1168	728	0.03%	0.004%
68	10.781	3013	3014	3016	rBV	1075	347	0.01%	0.002%
69	10.794	3016	3018	3020	rVV3	1222	470	0.02%	0.003%
70	10.923	3057	3058	3061	rBV3	797	513	0.02%	0.003%
71	10.945	3061	3065	3067	rVV4	1943	1441	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014114.D
 Acq On : 18 Dec 2019 12:11
 Operator : SY/MD
 Sample : K6314-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.955	3067	3068	3072	rVV4	2003	1153	0.05%	0.006%
73	11.029	3089	3091	3092	rBV2	1147	632	0.03%	0.003%
74	11.058	3098	3100	3104	rBV3	1701	1142	0.05%	0.006%
75	11.116	3117	3118	3119	rBV2	1121	418	0.02%	0.002%
76	11.177	3132	3137	3141	rBV6	2233	2509	0.11%	0.014%
77	11.206	3141	3146	3147	rBV3	3154	2598	0.11%	0.014%
78	11.289	3160	3172	3192	rBV	1061720	1645187	68.98%	9.101%
79	11.665	3278	3289	3306	rBV	1010496	1595077	66.88%	8.824%
80	11.858	3347	3349	3353	rBV4	1855	1201	0.05%	0.007%
81	12.013	3395	3397	3400	rBV3	1240	907	0.04%	0.005%
82	12.196	3451	3454	3455	rBV3	1425	818	0.03%	0.005%
83	12.247	3469	3470	3471	rBV	861	180	0.01%	0.001%
84	12.257	3471	3473	3474	rBV2	1713	788	0.03%	0.004%
85	12.315	3488	3491	3493	rBV5	2095	1235	0.05%	0.007%
86	12.521	3552	3555	3557	rBV4	2489	1254	0.05%	0.007%
87	12.662	3596	3599	3600	rBV3	1536	855	0.04%	0.005%


Sum of corrected areas: 18076541

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\
Data File : VV014114.D
Acq On : 18 Dec 2019 12:11
Operator : SY/MD
Sample : K6314-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF14

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

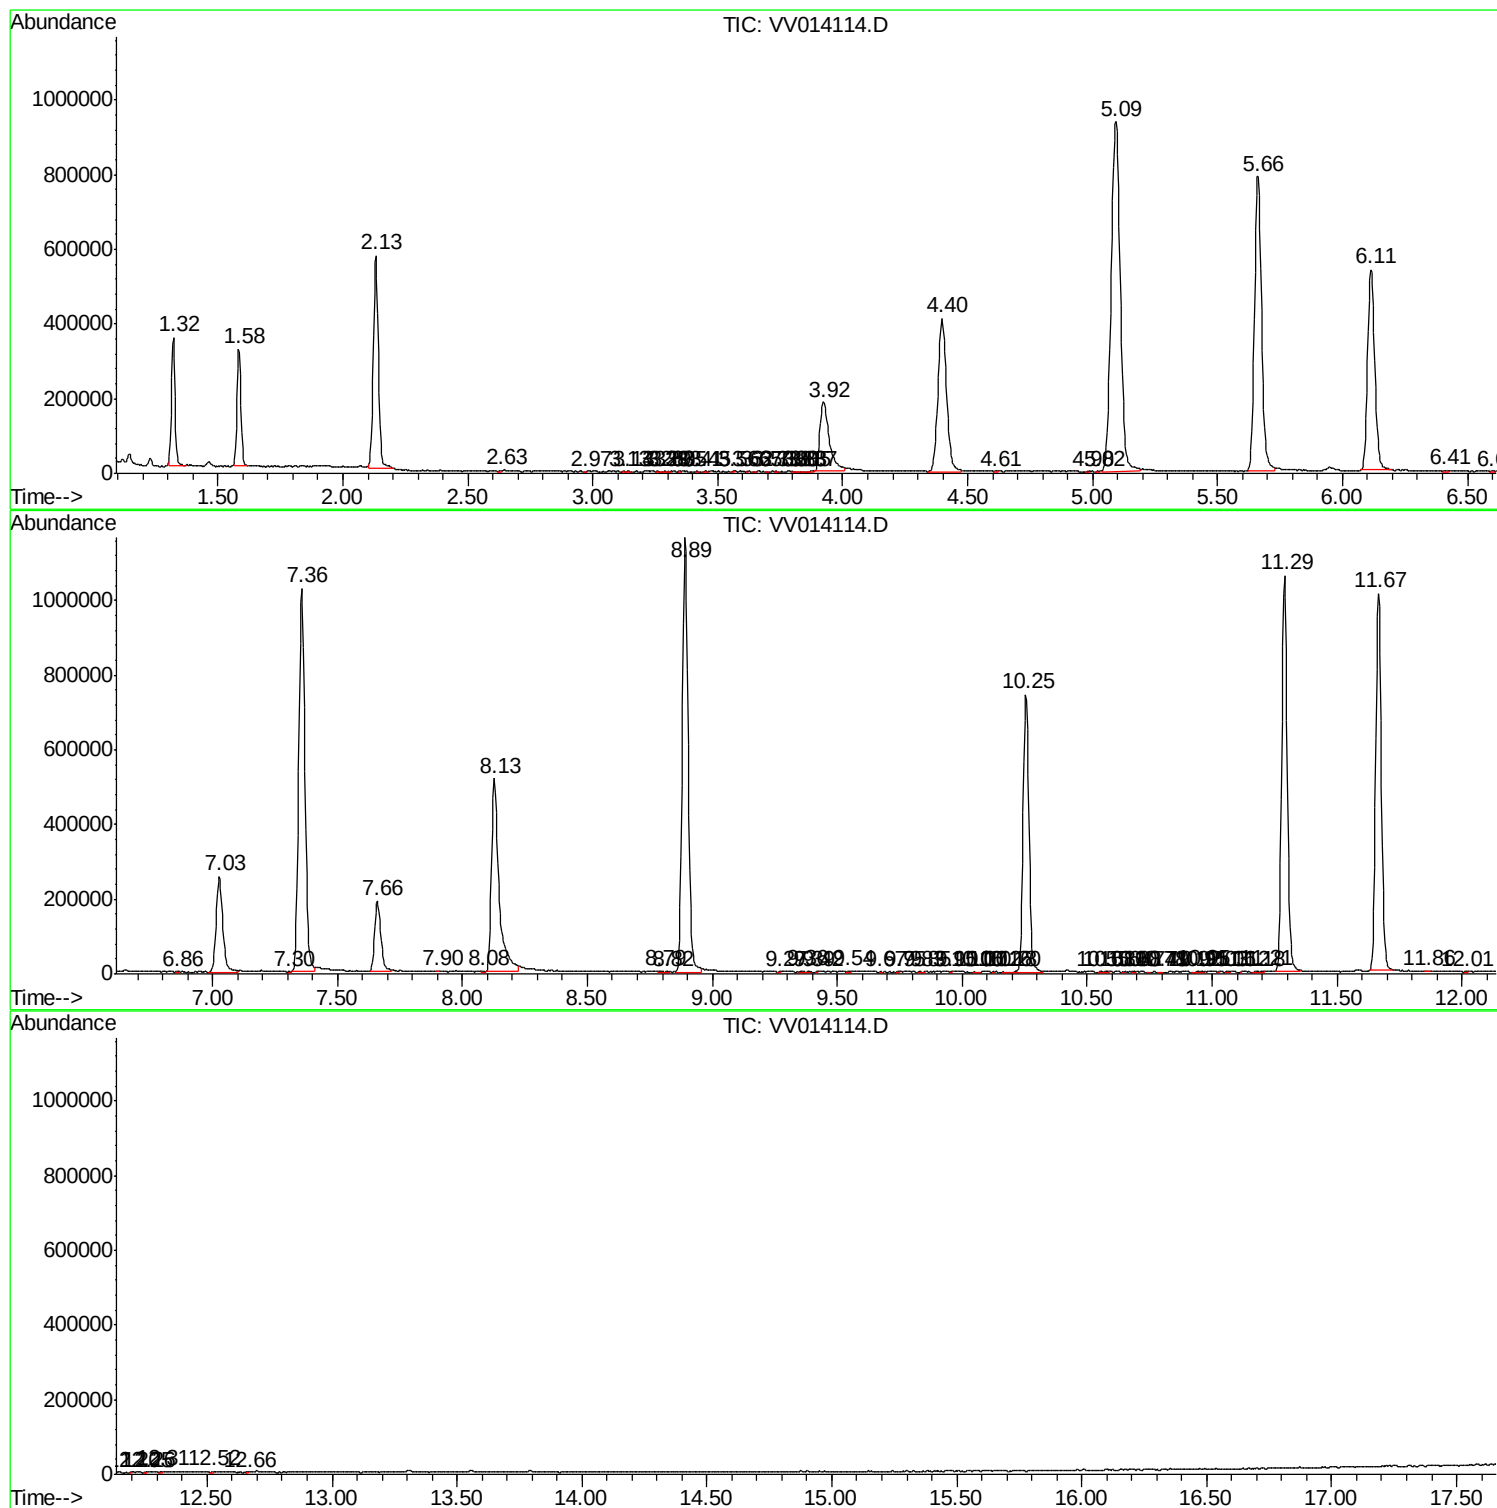

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014114.D
Acq On : 18 Dec 2019 12:11
Operator : SY/MD
Sample : K6314-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF14

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121819\
Data File : VV014114.D
Acq On : 18 Dec 2019 12:11
Operator : SY/MD
Sample : K6314-11
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFF14

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc