

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014115.D
 Acq On : 18 Dec 2019 12:35
 Operator : SY/MD
 Sample : K6314-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	84	rBV	363041	362333	14.79%	1.898%
2	1.582	146	153	166	rVB	329567	364417	14.88%	1.909%
3	2.129	314	323	340	rVB	589752	848224	34.62%	4.442%
4	2.364	394	396	401	rVB5	2202	1701	0.07%	0.009%
5	2.447	415	422	423	rBV5	2520	2787	0.11%	0.015%
6	2.573	456	461	463	rBV4	1823	1334	0.05%	0.007%
7	2.795	520	530	535	rBV4	2612	4747	0.19%	0.025%
8	3.077	616	618	629	rVB10	2431	3049	0.12%	0.016%
9	3.129	629	634	635	rBV5	1561	1161	0.05%	0.006%
10	3.238	665	668	672	rVV5	1406	1182	0.05%	0.006%
11	3.322	691	694	698	rBV5	1327	1150	0.05%	0.006%
12	3.364	704	707	712	rBV6	1762	1400	0.06%	0.007%
13	3.386	712	714	720	rVB7	1672	1619	0.07%	0.008%
14	3.450	732	734	737	rBV4	2043	1292	0.05%	0.007%
15	3.512	750	753	758	rBV8	1386	1307	0.05%	0.007%
16	3.540	758	762	766	rVB5	1291	1218	0.05%	0.006%
17	3.631	784	790	795	rBV9	2437	3504	0.14%	0.018%
18	3.740	819	824	826	rBV5	1613	1512	0.06%	0.008%
19	3.852	854	859	862	rBV6	1438	1484	0.06%	0.008%
20	3.920	869	880	902	rBV	186266	480098	19.60%	2.514%
21	4.248	980	982	986	rVB4	1656	1177	0.05%	0.006%
22	4.325	1002	1006	1009	rVV5	2126	2042	0.08%	0.011%
23	4.396	1012	1028	1054	rVV	428753	1026178	41.89%	5.374%
24	4.534	1068	1071	1074	rBV4	1479	1224	0.05%	0.006%
25	4.614	1094	1096	1099	rBV4	2239	1384	0.06%	0.007%
26	5.093	1225	1245	1269	rBV2	964288	2449807	100.00%	12.830%
27	5.421	1344	1347	1349	rBV4	1856	1095	0.04%	0.006%
28	5.460	1357	1359	1362	rVB4	1909	1223	0.05%	0.006%
29	5.540	1382	1384	1388	rVB5	2365	1244	0.05%	0.007%
30	5.659	1405	1421	1449	rBV	841867	1677605	68.48%	8.786%
31	5.939	1505	1508	1509	rBV3	5347	2818	0.12%	0.015%
32	6.113	1548	1562	1582	rVV	552357	1118614	45.66%	5.858%
33	6.341	1631	1633	1636	rBV3	1650	1152	0.05%	0.006%
34	6.646	1723	1728	1729	rBV5	3866	2920	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014115.D
 Acq On : 18 Dec 2019 12:35
 Operator : SY/MD
 Sample : K6314-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.753	1757	1761	1762	rBV4	2002	1259	0.05%	0.007%
36	6.814	1777	1780	1785	rBV7	1200	1239	0.05%	0.006%
37	6.946	1817	1821	1823	rBV4	1836	1323	0.05%	0.007%
38	7.026	1832	1846	1870	rBV	263855	486631	19.86%	2.549%
39	7.167	1886	1890	1892	rBV4	2645	1966	0.08%	0.010%
40	7.257	1916	1918	1925	rVB7	2024	2024	0.08%	0.011%
41	7.357	1936	1949	1965	rBV	1082236	1865224	76.14%	9.768%
42	7.659	2032	2043	2060	rBV	194841	331506	13.53%	1.736%
43	7.923	2121	2125	2128	rVB6	1483	1221	0.05%	0.006%
44	8.126	2177	2188	2229	rBV	526855	1136497	46.39%	5.952%
45	8.572	2325	2327	2332	rVB5	2332	1372	0.06%	0.007%
46	8.634	2343	2346	2347	rBV2	2368	1402	0.06%	0.007%
47	8.685	2359	2362	2367	rBV7	2460	2048	0.08%	0.011%
48	8.781	2388	2392	2394	rBV5	1603	1408	0.06%	0.007%
49	8.891	2413	2426	2458	rBV	1274005	2057241	83.98%	10.774%
50	9.261	2538	2541	2545	rVB6	2066	1557	0.06%	0.008%
51	9.370	2570	2575	2577	rBV4	1957	1862	0.08%	0.010%
52	9.386	2577	2580	2583	rVV5	1830	1223	0.05%	0.006%
53	9.531	2622	2625	2627	rVB3	2118	1232	0.05%	0.006%
54	9.598	2637	2646	2655	rBV9	7953	16072	0.66%	0.084%
55	9.785	2701	2704	2708	rVB6	2578	1687	0.07%	0.009%
56	9.859	2719	2727	2729	rBV9	2945	3746	0.15%	0.020%
57	9.920	2743	2746	2748	rBV3	1570	1178	0.05%	0.006%
58	9.933	2748	2750	2755	rVV6	2072	2408	0.10%	0.013%
59	9.968	2759	2761	2767	rVB6	3138	2502	0.10%	0.013%
60	10.254	2837	2850	2873	rBV	750105	1203106	49.11%	6.301%
61	10.412	2896	2899	2900	rBV3	2822	1135	0.05%	0.006%
62	10.482	2917	2921	2923	rBV5	1956	1366	0.06%	0.007%
63	10.543	2937	2940	2943	rVB3	2088	1404	0.06%	0.007%
64	10.637	2967	2969	2972	rVB4	2083	1121	0.05%	0.006%
65	10.723	2994	2996	3001	rVB4	1968	1567	0.06%	0.008%
66	10.900	3047	3051	3056	rVB9	3495	3398	0.14%	0.018%
67	10.971	3067	3073	3074	rBV6	3680	3214	0.13%	0.017%
68	11.103	3110	3114	3119	rVB7	1637	1894	0.08%	0.010%
69	11.135	3119	3124	3126	rBV6	2070	1833	0.07%	0.010%
70	11.209	3139	3147	3149	rBV8	4447	5695	0.23%	0.030%
71	11.289	3160	3172	3190	rBV	1146971	1815669	74.11%	9.509%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014115.D
 Acq On : 18 Dec 2019 12:35
 Operator : SY/MD
 Sample : K6314-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.386	3200	3202	3206	rBV5	1788	1175	0.05%	0.006%
73	11.666	3277	3289	3312	rBV	1090030	1691263	69.04%	8.857%
74	12.293	3481	3484	3489	rBV7	1894	1571	0.06%	0.008%
75	12.395	3511	3516	3524	rVV10	5571	8748	0.36%	0.046%
76	12.508	3548	3551	3553	rBV4	1592	1135	0.05%	0.006%
77	12.694	3603	3609	3617	rVB9	3583	4827	0.20%	0.025%
78	12.794	3637	3640	3647	rVB9	2851	2144	0.09%	0.011%
79	12.942	3682	3686	3689	rVB6	1732	1304	0.05%	0.007%
80	13.231	3772	3776	3780	rBV6	1601	1349	0.06%	0.007%
81	13.309	3792	3800	3811	rVB6	3710	8520	0.35%	0.045%
82	13.357	3811	3815	3818	rVB5	1510	1253	0.05%	0.007%
83	13.383	3818	3823	3826	rBV7	2403	2472	0.10%	0.013%
84	13.399	3826	3828	3830	rBV3	2462	1352	0.06%	0.007%
85	13.440	3838	3841	3842	rBV3	1790	1223	0.05%	0.006%
86	13.556	3875	3877	3884	rVB6	3221	2746	0.11%	0.014%
87	13.585	3884	3886	3891	rVB6	2496	2123	0.09%	0.011%
88	13.775	3940	3945	3947	rBV6	1799	1675	0.07%	0.009%
89	13.794	3947	3951	3954	rBV4	3515	3305	0.13%	0.017%
90	13.907	3985	3986	3990	rVB4	2366	1417	0.06%	0.007%
91	13.964	4001	4004	4006	rBV3	2393	1153	0.05%	0.006%
92	14.032	4022	4025	4027	rBV5	1757	1438	0.06%	0.008%
93	14.122	4050	4053	4057	rVB4	1868	1287	0.05%	0.007%
94	14.225	4083	4085	4088	rBV4	1444	1130	0.05%	0.006%
95	14.257	4093	4095	4100	rBV4	1370	1214	0.05%	0.006%
96	14.321	4110	4115	4116	rBV5	2462	1702	0.07%	0.009%
97	14.646	4211	4216	4218	rBV5	2369	1611	0.07%	0.008%
98	14.714	4235	4237	4241	rBV4	1856	1495	0.06%	0.008%
99	14.894	4291	4293	4297	rVB5	2061	1271	0.05%	0.007%
100	15.903	4605	4607	4610	rBV3	2442	1218	0.05%	0.006%


Sum of corrected areas: 19094353

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\
Data File : VV014115.D
Acq On : 18 Dec 2019 12:35
Operator : SY/MD
Sample : K6314-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

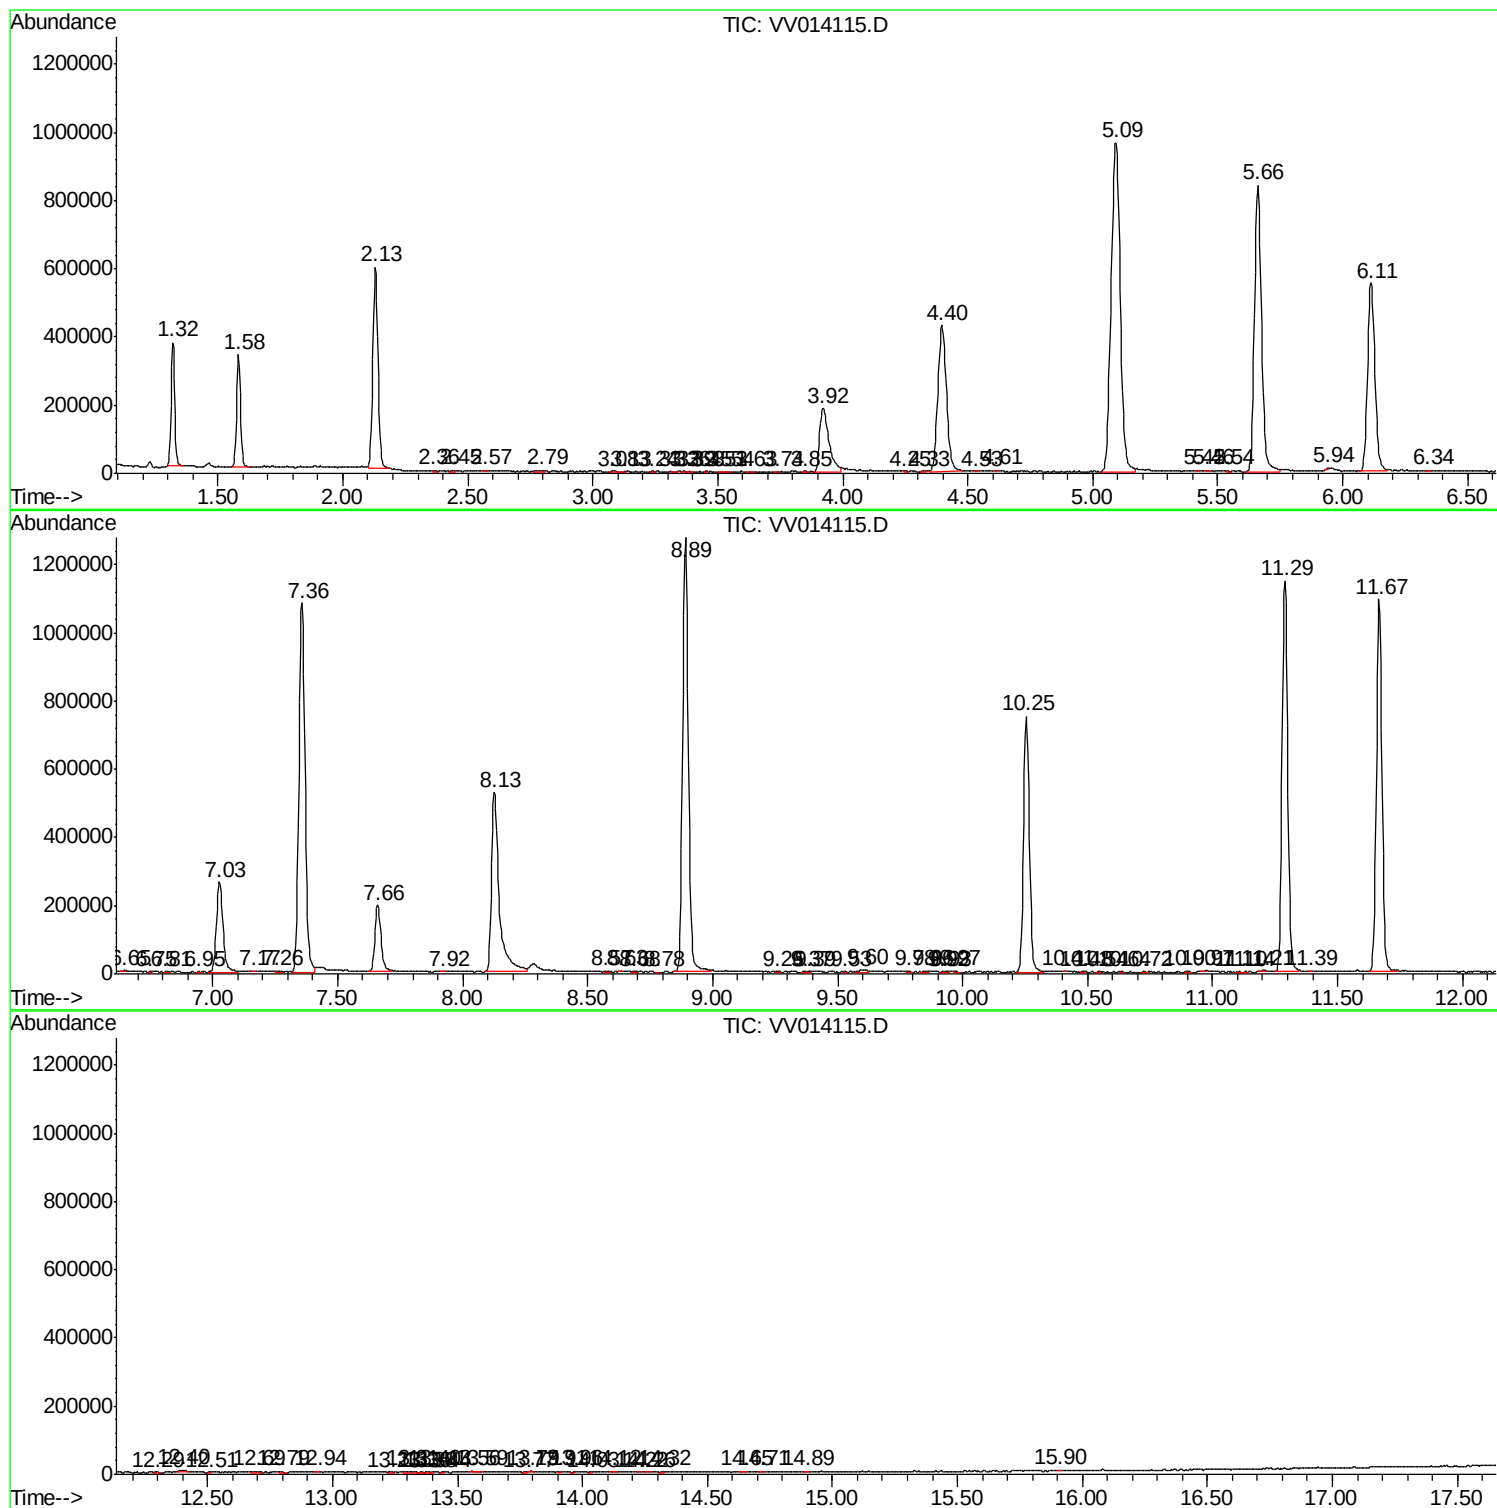

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014115.D
Acq On : 18 Dec 2019 12:35
Operator : SY/MD
Sample : K6314-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121819\
Data File : VV014115.D
Acq On : 18 Dec 2019 12:35
Operator : SY/MD
Sample : K6314-12
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFF47

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
