

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014119.D
 Acq On : 18 Dec 2019 14:10
 Operator : SY/MD
 Sample : K6356-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	80	rVB	347675	341956	13.82%	1.771%
2	1.582	146	153	166	rVB	322139	358823	14.50%	1.859%
3	2.129	315	323	336	rVB	571571	797491	32.23%	4.131%
4	2.524	442	446	447	rBV4	1786	1166	0.05%	0.006%
5	2.762	517	520	522	rBV3	3125	1866	0.08%	0.010%
6	2.859	544	550	553	rBV8	1947	2134	0.09%	0.011%
7	2.968	581	584	585	rBV4	1349	896	0.04%	0.005%
8	3.087	620	621	624	rBV3	1439	646	0.03%	0.003%
9	3.116	627	630	632	rBV4	1775	1205	0.05%	0.006%
10	3.142	636	638	642	rVB5	2042	1401	0.06%	0.007%
11	3.161	642	644	645	rBV2	961	337	0.01%	0.002%
12	3.280	674	681	685	rBV7	2013	2741	0.11%	0.014%
13	3.338	693	699	700	rBV5	1603	1085	0.04%	0.006%
14	3.447	731	733	737	rBV5	1810	1008	0.04%	0.005%
15	3.483	740	744	746	rBV4	1949	1381	0.06%	0.007%
16	3.499	747	749	750	rBV2	1262	435	0.02%	0.002%
17	3.566	765	770	772	rBV4	1294	1080	0.04%	0.006%
18	3.579	772	774	778	rVB3	1615	1098	0.04%	0.006%
19	3.605	778	782	783	rBV5	1392	965	0.04%	0.005%
20	3.614	783	785	789	rVV5	1200	629	0.03%	0.003%
21	3.630	789	790	792	rVB2	1432	493	0.02%	0.003%
22	3.653	795	797	799	rBV2	1089	494	0.02%	0.003%
23	3.688	806	808	810	rBV3	1614	788	0.03%	0.004%
24	3.743	822	825	826	rBV2	1210	602	0.02%	0.003%
25	3.801	841	843	847	rVB4	2018	1206	0.05%	0.006%
26	3.827	847	851	852	rBV4	1059	623	0.03%	0.003%
27	3.878	865	867	868	rBV2	1172	529	0.02%	0.003%
28	3.926	870	882	913	rVV2	230578	700454	28.31%	3.629%
29	4.399	1014	1029	1054	rBV2	437274	1126798	45.54%	5.837%
30	4.737	1131	1134	1139	rBV6	2057	1787	0.07%	0.009%
31	4.968	1203	1206	1207	rBV4	2003	1015	0.04%	0.005%
32	5.003	1215	1217	1220	rBV3	853	525	0.02%	0.003%
33	5.090	1226	1244	1266	rBV2	983769	2474570	100.00%	12.819%
34	5.425	1345	1348	1350	rBV4	2276	1664	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014119.D
 Acq On : 18 Dec 2019 14:10
 Operator : SY/MD
 Sample : K6356-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.659	1408	1421	1446	rBV	865064	1700652	68.73%	8.810%
36	6.113	1546	1562	1581	rBV	567442	1136096	45.91%	5.885%
37	6.614	1716	1718	1721	rBV4	2045	990	0.04%	0.005%
38	6.656	1724	1731	1735	rBV9	4572	6798	0.27%	0.035%
39	6.839	1786	1788	1789	rBV2	1625	680	0.03%	0.004%
40	7.026	1834	1846	1865	rBV	270206	484233	19.57%	2.509%
41	7.357	1936	1949	1972	rBV	1036944	1833017	74.07%	9.496%
42	7.659	2034	2043	2060	rBV	194396	321974	13.01%	1.668%
43	8.058	2165	2167	2168	rBV2	2029	800	0.03%	0.004%
44	8.129	2177	2189	2217	rBV	579843	1180059	47.69%	6.113%
45	8.444	2283	2287	2288	rBV4	2496	1621	0.07%	0.008%
46	8.736	2375	2378	2384	rVB6	3455	3691	0.15%	0.019%
47	8.775	2384	2390	2392	rBV7	2176	2299	0.09%	0.012%
48	8.891	2414	2426	2446	rBV	1264770	2066132	83.49%	10.704%
49	9.248	2534	2537	2539	rBV3	2016	1182	0.05%	0.006%
50	9.309	2552	2556	2559	rBV6	1824	1709	0.07%	0.009%
51	9.392	2579	2582	2589	rVB9	2138	2295	0.09%	0.012%
52	9.489	2605	2612	2613	rBV7	2686	2930	0.12%	0.015%
53	9.550	2628	2631	2632	rBV3	842	562	0.02%	0.003%
54	9.572	2636	2638	2639	rBV3	1357	518	0.02%	0.003%
55	9.733	2684	2688	2691	rBV5	2261	1789	0.07%	0.009%
56	9.775	2699	2701	2706	rVB4	2431	1612	0.07%	0.008%
57	9.797	2706	2708	2710	rBV4	1130	563	0.02%	0.003%
58	9.868	2728	2730	2735	rBV4	1374	825	0.03%	0.004%
59	9.942	2750	2753	2754	rBV4	1814	1006	0.04%	0.005%
60	9.952	2754	2756	2757	rBV2	1478	561	0.02%	0.003%
61	10.067	2789	2792	2796	rVB5	2687	1674	0.07%	0.009%
62	10.093	2796	2800	2801	rBV3	1322	841	0.03%	0.004%
63	10.103	2801	2803	2805	rVB3	1221	494	0.02%	0.003%
64	10.113	2805	2806	2808	rBV3	1333	737	0.03%	0.004%
65	10.167	2819	2823	2825	rBV4	1063	874	0.04%	0.005%
66	10.254	2838	2850	2873	rBV	733345	1175715	47.51%	6.091%
67	10.402	2894	2896	2897	rBV2	1680	742	0.03%	0.004%
68	10.511	2927	2930	2933	rBV4	1421	1058	0.04%	0.005%
69	10.643	2966	2971	2973	rBV6	1757	1168	0.05%	0.006%
70	10.656	2973	2975	2976	rVB2	1024	300	0.01%	0.002%
71	10.669	2976	2979	2981	rBV3	1668	1084	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014119.D
 Acq On : 18 Dec 2019 14:10
 Operator : SY/MD
 Sample : K6356-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.720	2991	2995	2997	rBV4	1124	850	0.03%	0.004%
73	10.756	3004	3006	3007	rBV2	1053	412	0.02%	0.002%
74	10.804	3016	3021	3027	rBV9	2004	2317	0.09%	0.012%
75	10.865	3038	3040	3041	rBV3	1571	685	0.03%	0.004%
76	11.039	3092	3094	3097	rVB3	1004	495	0.02%	0.003%
77	11.103	3110	3114	3116	rBV3	3149	2032	0.08%	0.011%
78	11.180	3135	3138	3139	rBV2	1227	737	0.03%	0.004%
79	11.289	3159	3172	3188	rBV	1195768	1822359	73.64%	9.441%
80	11.666	3278	3289	3309	rBV	1078167	1692067	68.38%	8.766%
81	11.977	3382	3386	3389	rBV6	1743	1377	0.06%	0.007%
82	12.100	3422	3424	3425	rBV2	1898	803	0.03%	0.004%
83	12.225	3461	3463	3465	rVB3	1408	510	0.02%	0.003%
84	12.241	3465	3468	3471	rVB5	1807	910	0.04%	0.005%
85	12.408	3516	3520	3522	rBV5	2116	1399	0.06%	0.007%
86	12.453	3530	3534	3536	rBV4	1594	1117	0.05%	0.006%
87	12.685	3601	3606	3607	rBV4	2632	1998	0.08%	0.010%
88	13.170	3755	3757	3760	rBV4	1535	960	0.04%	0.005%
89	13.839	3962	3965	3969	rBV5	2409	2134	0.09%	0.011%
90	13.948	3996	3999	4000	rBV3	1700	985	0.04%	0.005%


Sum of corrected areas: 19303319

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\
Data File : VV014119.D
Acq On : 18 Dec 2019 14:10
Operator : SY/MD
Sample : K6356-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D36

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

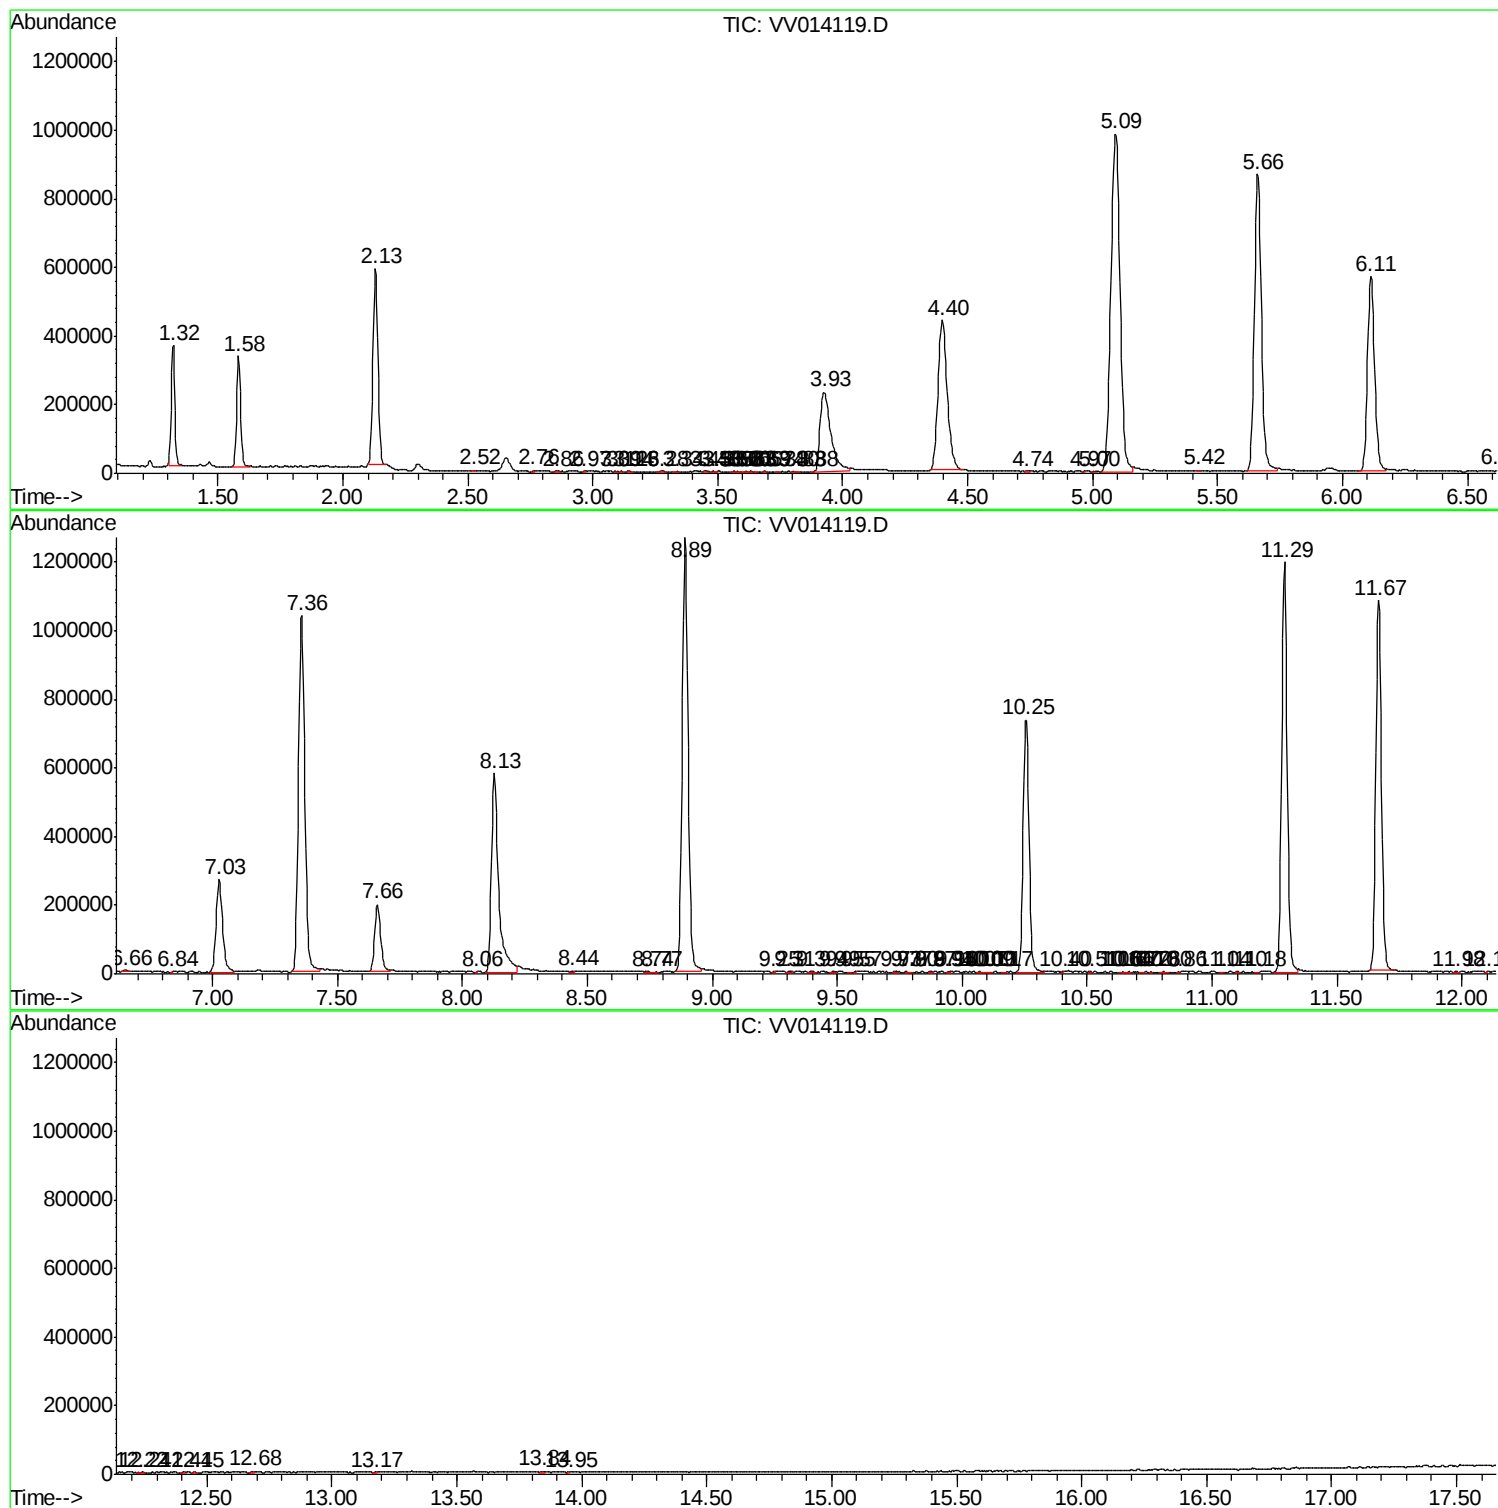

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014119.D
Acq On : 18 Dec 2019 14:10
Operator : SY/MD
Sample : K6356-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D36

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014119.D
Acq On : 18 Dec 2019 14:10
Operator : SY/MD
Sample : K6356-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D36

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc