

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014120.D
 Acq On : 18 Dec 2019 14:33
 Operator : SY/MD
 Sample : K6356-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	82	rVB	356449	350198	13.93%	1.768%
2	1.582	146	153	164	rVB	322846	354558	14.10%	1.790%
3	2.129	315	323	335	rBV	571412	786177	31.26%	3.968%
4	2.753	514	517	519	rBV4	1097	700	0.03%	0.004%
5	2.859	548	550	555	rVB6	2383	1617	0.06%	0.008%
6	2.981	585	588	592	rBV5	1523	1194	0.05%	0.006%
7	3.000	592	594	597	rBV4	1585	866	0.03%	0.004%
8	3.061	611	613	616	rVB4	2076	991	0.04%	0.005%
9	3.081	616	619	620	rBV3	1431	849	0.03%	0.004%
10	3.161	640	644	647	rBV5	1776	1715	0.07%	0.009%
11	3.200	652	656	660	rBV6	1734	1939	0.08%	0.010%
12	3.428	725	727	731	rBV4	1469	1073	0.04%	0.005%
13	3.454	731	735	737	rBV5	2168	1606	0.06%	0.008%
14	3.534	755	760	763	rBV7	1770	1574	0.06%	0.008%
15	3.589	772	777	778	rBV4	1450	1285	0.05%	0.006%
16	3.624	786	788	795	rVB8	1923	1958	0.08%	0.010%
17	3.669	800	802	804	rBV3	1537	841	0.03%	0.004%
18	3.701	807	812	815	rBV6	2002	1728	0.07%	0.009%
19	3.769	831	833	836	rVB3	1697	987	0.04%	0.005%
20	3.794	836	841	842	rBV5	2186	1521	0.06%	0.008%
21	3.823	848	850	856	rBV7	1743	1335	0.05%	0.007%
22	3.923	870	881	916	rBV2	223689	679708	27.03%	3.431%
23	4.280	990	992	995	rBV4	2020	1350	0.05%	0.007%
24	4.396	1015	1028	1053	rVB	435517	1062765	42.26%	5.364%
25	4.585	1085	1087	1089	rBV2	1837	783	0.03%	0.004%
26	4.650	1105	1107	1110	rBV3	1332	919	0.04%	0.005%
27	4.788	1148	1150	1154	rBV5	1143	789	0.03%	0.004%
28	4.897	1181	1184	1187	rBV5	1536	1052	0.04%	0.005%
29	4.955	1198	1202	1205	rBV5	1776	1634	0.06%	0.008%
30	5.007	1214	1218	1221	rBV5	2057	1164	0.05%	0.006%
31	5.023	1221	1223	1226	rBV4	1572	1169	0.05%	0.006%
32	5.093	1226	1245	1283	rBV2	984568	2514607	100.00%	12.692%
33	5.402	1337	1341	1342	rBV3	1683	1325	0.05%	0.007%
34	5.508	1370	1374	1377	rBV5	2625	2161	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014120.D
 Acq On : 18 Dec 2019 14:33
 Operator : SY/MD
 Sample : K6356-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.605	1402	1404	1407	rBV4	1735	1176	0.05%	0.006%
36	5.659	1407	1421	1445	rBV	860646	1692298	67.30%	8.541%
37	6.048	1540	1542	1544	rBV3	1491	798	0.03%	0.004%
38	6.113	1549	1562	1586	rVV	563927	1138518	45.28%	5.746%
39	6.437	1659	1663	1665	rBV4	1416	1020	0.04%	0.005%
40	6.560	1697	1701	1702	rBV3	1945	1271	0.05%	0.006%
41	6.637	1722	1725	1726	rBV3	3174	1673	0.07%	0.008%
42	6.788	1768	1772	1775	rBV5	1940	2045	0.08%	0.010%
43	6.945	1819	1821	1826	rBV5	1515	964	0.04%	0.005%
44	7.026	1833	1846	1862	rBV	267946	483409	19.22%	2.440%
45	7.357	1937	1949	1968	rBV	1047875	1811659	72.05%	9.144%
46	7.621	2028	2031	2032	rBV3	2142	1107	0.04%	0.006%
47	7.659	2033	2043	2061	rVV	199998	338732	13.47%	1.710%
48	7.868	2106	2108	2111	rBV3	1715	1078	0.04%	0.005%
49	8.129	2175	2189	2222	rBV	540583	1141191	45.38%	5.760%
50	8.489	2299	2301	2306	rVB4	1536	1056	0.04%	0.005%
51	8.688	2360	2363	2368	rBV7	2840	2309	0.09%	0.012%
52	8.727	2373	2375	2377	rVB3	2172	850	0.03%	0.004%
53	8.756	2381	2384	2386	rVB4	1637	996	0.04%	0.005%
54	8.778	2389	2391	2393	rBV3	1476	1022	0.04%	0.005%
55	8.839	2405	2410	2413	rBV6	2568	2159	0.09%	0.011%
56	8.891	2413	2426	2453	rBV	1286571	2171500	86.36%	10.960%
57	9.331	2560	2563	2564	rBV2	1968	1168	0.05%	0.006%
58	9.370	2573	2575	2577	rBV3	1174	746	0.03%	0.004%
59	9.598	2644	2646	2649	rBV4	1232	862	0.03%	0.004%
60	9.662	2662	2666	2668	rBV5	2066	1330	0.05%	0.007%
61	9.775	2699	2701	2704	rBV3	1654	838	0.03%	0.004%
62	9.833	2715	2719	2721	rBV4	1651	1100	0.04%	0.006%
63	9.939	2748	2752	2756	rBV6	2206	2129	0.08%	0.011%
64	9.974	2760	2763	2765	rBV3	1063	705	0.03%	0.004%
65	10.016	2771	2776	2779	rBV7	827	885	0.04%	0.004%
66	10.080	2793	2796	2798	rBV4	1437	1140	0.05%	0.006%
67	10.254	2837	2850	2874	rBV	741681	1188780	47.27%	6.000%
68	10.543	2937	2940	2944	rBV5	2036	1730	0.07%	0.009%
69	10.714	2991	2993	2996	rBV5	1255	792	0.03%	0.004%
70	10.749	3002	3004	3009	rVB4	1735	982	0.04%	0.005%
71	10.842	3030	3033	3035	rBV3	2257	1207	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014120.D
 Acq On : 18 Dec 2019 14:33
 Operator : SY/MD
 Sample : K6356-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.858	3035	3038	3040	rVB4	2053	1180	0.05%	0.006%
73	10.894	3040	3049	3054	rBV10	3403	4976	0.20%	0.025%
74	10.936	3060	3062	3068	rBV6	2028	1781	0.07%	0.009%
75	11.061	3097	3101	3104	rVB6	1390	890	0.04%	0.004%
76	11.109	3114	3116	3119	rBV4	1040	711	0.03%	0.004%
77	11.154	3126	3130	3133	rVB5	1905	1331	0.05%	0.007%
78	11.196	3140	3143	3144	rBV3	2304	1357	0.05%	0.007%
79	11.225	3144	3152	3160	rVV7	5686	9520	0.38%	0.048%
80	11.289	3160	3172	3193	rBV	1204654	1858129	73.89%	9.378%
81	11.665	3278	3289	3314	rBV2	1140402	2096514	83.37%	10.582%
82	11.900	3360	3362	3364	rBV3	1652	987	0.04%	0.005%
83	12.145	3433	3438	3441	rBV7	2103	1795	0.07%	0.009%
84	12.206	3454	3457	3461	rBV6	1419	1318	0.05%	0.007%
85	12.325	3492	3494	3497	rVB4	1909	1218	0.05%	0.006%
86	12.354	3497	3503	3505	rBV7	2590	2326	0.09%	0.012%
87	12.392	3513	3515	3518	rVB3	1506	802	0.03%	0.004%
88	12.411	3518	3521	3522	rBV3	1689	774	0.03%	0.004%
89	12.566	3566	3569	3572	rBV4	2332	1873	0.07%	0.009%
90	12.646	3592	3594	3596	rBV3	1554	963	0.04%	0.005%
91	12.862	3658	3661	3665	rBV5	1374	1334	0.05%	0.007%
92	13.077	3726	3728	3730	rBV3	1245	723	0.03%	0.004%
93	13.090	3730	3732	3734	rVV3	1845	834	0.03%	0.004%
94	13.244	3777	3780	3782	rBV4	2342	1745	0.07%	0.009%
95	13.463	3847	3848	3853	rVB4	1818	812	0.03%	0.004%
96	13.485	3853	3855	3857	rBV3	1743	673	0.03%	0.003%
97	13.791	3943	3950	3961	rVB2	17184	29205	1.16%	0.147%
98	14.016	4016	4020	4021	rBV4	1785	1374	0.05%	0.007%
99	14.054	4030	4032	4033	rBV2	1442	728	0.03%	0.004%
100	15.315	4423	4424	4428	rBV3	2387	1479	0.06%	0.007%


Sum of corrected areas: 19812715

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\
Data File : VV014120.D
Acq On : 18 Dec 2019 14:33
Operator : SY/MD
Sample : K6356-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

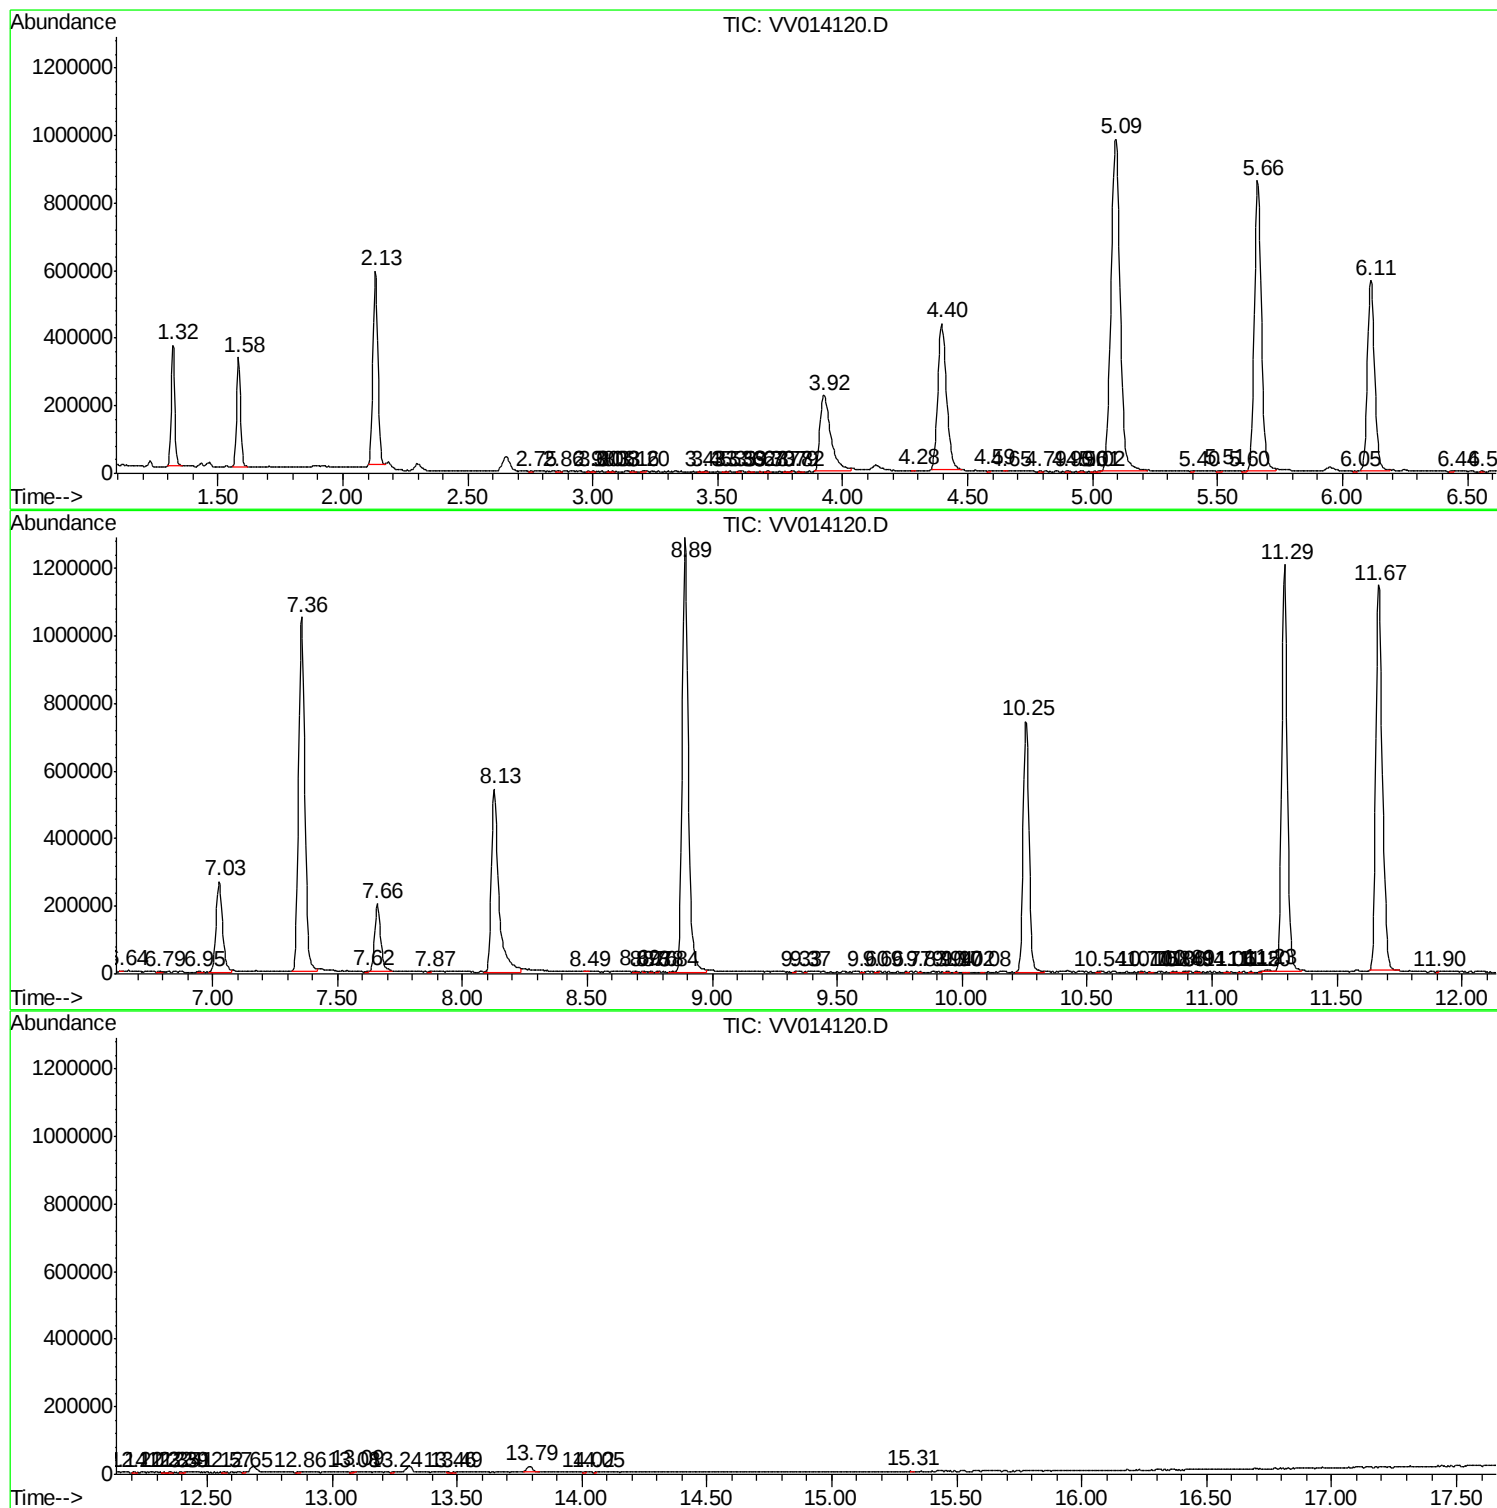

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014120.D
Acq On : 18 Dec 2019 14:33
Operator : SY/MD
Sample : K6356-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014120.D
Acq On : 18 Dec 2019 14:33
Operator : SY/MD
Sample : K6356-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D37

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc