

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121819\
 Data File : VV014121.D
 Acq On : 18 Dec 2019 14:57
 Operator : SY/MD
 Sample : K6356-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	81	rVB	354783	349264	10.40%	1.562%
2	1.582	146	153	165	rVB	321800	352631	10.51%	1.577%
3	2.129	315	323	333	rBV	573063	782952	23.33%	3.502%
4	2.611	471	473	474	rBV2	2189	1141	0.03%	0.005%
5	2.923	566	570	574	rBV7	2259	2169	0.06%	0.010%
6	3.074	615	617	622	rBV6	1469	1050	0.03%	0.005%
7	3.097	622	624	627	rVB4	1998	1047	0.03%	0.005%
8	3.135	632	636	637	rBV4	1577	1193	0.04%	0.005%
9	3.164	643	645	649	rBV4	1066	816	0.02%	0.004%
10	3.225	662	664	666	rBV3	1001	528	0.02%	0.002%
11	3.293	682	685	687	rVB3	1770	900	0.03%	0.004%
12	3.312	687	691	693	rBV4	2649	1832	0.05%	0.008%
13	3.399	716	718	721	rVB4	2499	1260	0.04%	0.006%
14	3.521	754	756	759	rVB3	1916	1088	0.03%	0.005%
15	3.544	761	763	769	rVV7	2625	2186	0.07%	0.010%
16	3.608	781	783	785	rVB3	1414	500	0.01%	0.002%
17	3.634	785	791	794	rBV8	2214	2382	0.07%	0.011%
18	3.859	859	861	864	rVB4	1077	554	0.02%	0.002%
19	3.926	864	882	916	rBV2	228920	723927	21.57%	3.238%
20	4.392	1016	1027	1053	rVB	413943	1005589	29.96%	4.498%
21	4.630	1099	1101	1104	rVB4	2301	1103	0.03%	0.005%
22	4.791	1147	1151	1154	rBV5	1782	1447	0.04%	0.006%
23	4.852	1167	1170	1173	rVB4	2532	1443	0.04%	0.006%
24	4.884	1178	1180	1182	rBV3	1608	855	0.03%	0.004%
25	4.962	1201	1204	1206	rBV3	1463	1105	0.03%	0.005%
26	5.010	1217	1219	1221	rVB3	1928	752	0.02%	0.003%
27	5.023	1221	1223	1225	rBV3	1555	863	0.03%	0.004%
28	5.090	1228	1244	1272	rVV2	947615	2428856	72.36%	10.864%
29	5.659	1408	1421	1444	rBV	859539	1698541	50.60%	7.597%
30	6.113	1550	1562	1592	rVB	548806	1098014	32.71%	4.911%
31	6.627	1720	1722	1725	rBV4	2337	1809	0.05%	0.008%
32	6.798	1771	1775	1777	rBV5	2102	1244	0.04%	0.006%
33	6.955	1819	1824	1827	rBV6	2367	2264	0.07%	0.010%
34	7.026	1834	1846	1865	rBV	274059	492170	14.66%	2.201%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121819\
 Data File : VV014121.D
 Acq On : 18 Dec 2019 14:57
 Operator : SY/MD
 Sample : K6356-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	7.357	1937	1949	1970	rBV	1081592	1856213	55.30%	8.303%
36	7.659	2033	2043	2067	rBV	198908	341149	10.16%	1.526%
37	7.961	2134	2137	2138	rBV3	1901	1078	0.03%	0.005%
38	8.125	2178	2188	2219	rBV	553272	1151361	34.30%	5.150%
39	8.624	2342	2343	2345	rBV2	1756	839	0.02%	0.004%
40	8.810	2399	2401	2404	rBV4	1705	958	0.03%	0.004%
41	8.891	2411	2426	2449	rBV	1322818	2251588	67.08%	10.071%
42	9.505	2615	2617	2619	rBV2	1199	538	0.02%	0.002%
43	9.527	2622	2624	2629	rVB4	2336	1323	0.04%	0.006%
44	9.550	2629	2631	2634	rBV4	1904	1400	0.04%	0.006%
45	9.772	2697	2700	2703	rVB4	1527	1128	0.03%	0.005%
46	9.807	2709	2711	2712	rBV2	1170	407	0.01%	0.002%
47	10.132	2806	2812	2815	rVB8	2727	2905	0.09%	0.013%
48	10.148	2815	2817	2819	rBV3	1690	980	0.03%	0.004%
49	10.254	2838	2850	2870	rBV	738230	1166654	34.76%	5.218%
50	10.492	2921	2924	2926	rBV3	2205	726	0.02%	0.003%
51	10.524	2932	2934	2937	rBV3	835	539	0.02%	0.002%
52	10.566	2946	2947	2948	rBV	894	237	0.01%	0.001%
53	10.608	2958	2960	2962	rBV3	1151	448	0.01%	0.002%
54	10.666	2975	2978	2980	rBV4	1574	889	0.03%	0.004%
55	10.707	2988	2991	2992	rBV2	1667	1105	0.03%	0.005%
56	10.945	3061	3065	3067	rBV4	1203	1040	0.03%	0.005%
57	10.958	3067	3069	3072	rVV3	1673	721	0.02%	0.003%
58	11.087	3106	3109	3111	rBV4	1112	647	0.02%	0.003%
59	11.132	3118	3123	3125	rVB5	1724	1597	0.05%	0.007%
60	11.148	3125	3128	3130	rVB3	1231	451	0.01%	0.002%
61	11.161	3130	3132	3133	rBV2	1003	391	0.01%	0.002%
62	11.289	3161	3172	3194	rBV2	1228007	2104908	62.71%	9.415%
63	11.675	3277	3292	3312	rBV3	1426162	3356700	100.00%	15.014%
64	12.190	3450	3452	3456	rVB5	2402	1304	0.04%	0.006%
65	12.373	3504	3509	3511	rBV5	1750	1778	0.05%	0.008%
66	12.405	3517	3519	3522	rBV4	1930	1018	0.03%	0.005%
67	12.678	3596	3604	3618	rVB	104571	167691	5.00%	0.750%
68	12.955	3687	3690	3692	rBV3	1964	1452	0.04%	0.006%
69	13.305	3789	3799	3815	rVB	293658	461839	13.76%	2.066%
70	13.450	3842	3844	3845	rBV2	1648	795	0.02%	0.004%
71	13.788	3938	3949	3966	rBV	298990	468120	13.95%	2.094%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121819\
Data File : VV014121.D
Acq On : 18 Dec 2019 14:57
Operator : SY/MD
Sample : K6356-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

72	14.196	4069	4076	4090	rVB3	23996	40813	1.22%	0.183%
----	--------	------	------	------	------	-------	-------	-------	--------


Sum of corrected areas: 22357205

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121819\
Data File : VV014121.D
Acq On : 18 Dec 2019 14:57
Operator : SY/MD
Sample : K6356-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

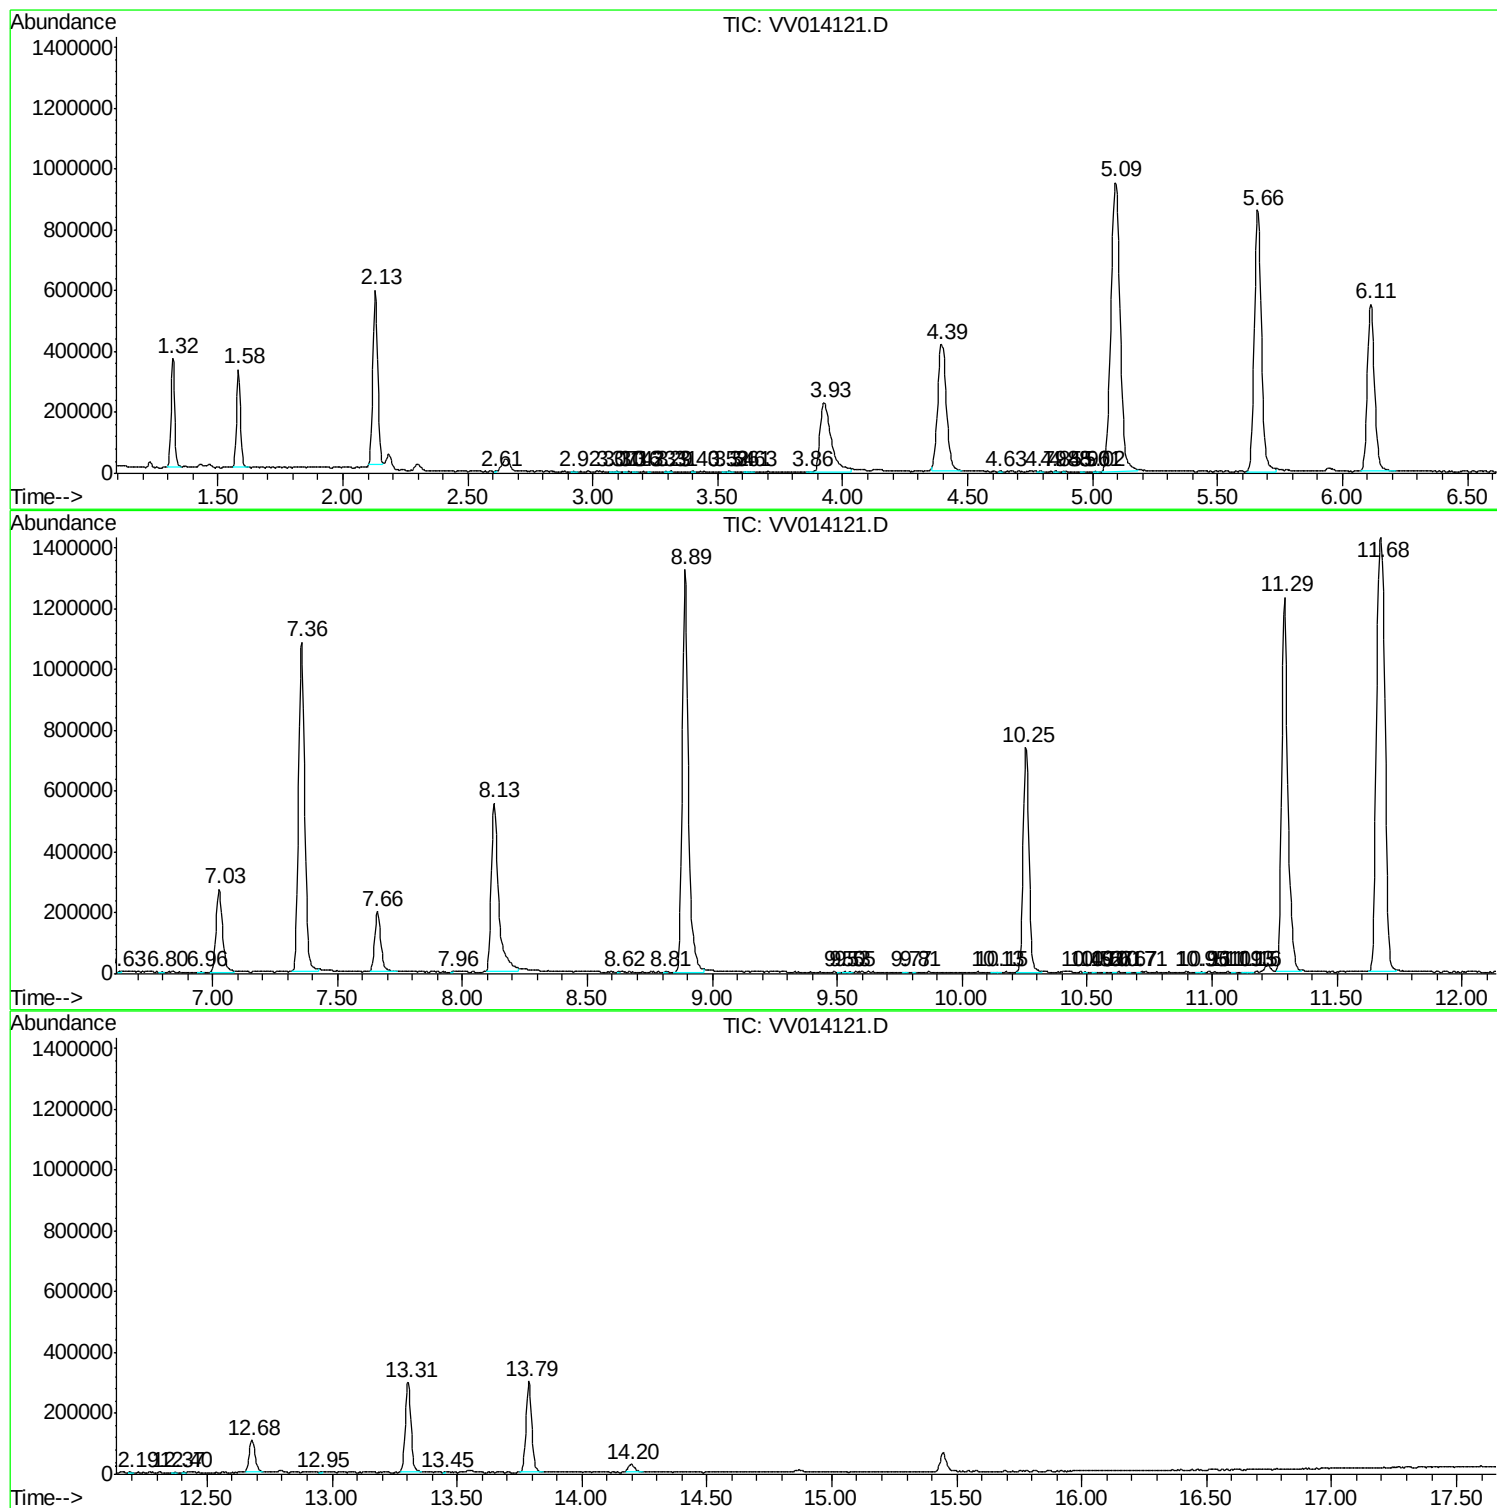

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121819\
Data File : VV014121.D
Acq On : 18 Dec 2019 14:57
Operator : SY/MD
Sample : K6356-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121819\
Data File : VV014121.D
Acq On : 18 Dec 2019 14:57
Operator : SY/MD
Sample : K6356-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc