

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014122.D
 Acq On : 18 Dec 2019 15:21
 Operator : SY/MD
 Sample : K6356-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	84	rVB	357402	353326	12.30%	1.609%
2	1.582	147	153	163	rVB	328267	356899	12.42%	1.625%
3	2.132	315	324	336	rVB	572472	806316	28.06%	3.671%
4	2.344	388	390	393	rBV4	2705	1058	0.04%	0.005%
5	2.614	470	474	475	rBV4	1635	1203	0.04%	0.005%
6	2.868	551	553	554	rBV2	1512	808	0.03%	0.004%
7	2.971	583	585	589	rBV4	1204	791	0.03%	0.004%
8	3.315	690	692	694	rBV3	1716	917	0.03%	0.004%
9	3.328	694	696	700	rVV4	1341	805	0.03%	0.004%
10	3.483	739	744	746	rBV5	1908	1142	0.04%	0.005%
11	3.502	746	750	752	rBV5	1335	866	0.03%	0.004%
12	3.518	753	755	758	rBV4	1326	887	0.03%	0.004%
13	3.585	774	776	778	rBV3	1424	647	0.02%	0.003%
14	3.682	802	806	808	rBV4	1484	864	0.03%	0.004%
15	3.698	809	811	814	rVB3	1850	926	0.03%	0.004%
16	3.746	824	826	830	rBV5	1117	643	0.02%	0.003%
17	3.801	840	843	844	rBV3	1710	803	0.03%	0.004%
18	3.839	853	855	856	rBV2	1098	514	0.02%	0.002%
19	3.855	856	860	861	rBV3	1009	719	0.03%	0.003%
20	3.920	870	880	905	rBV	194720	514512	17.91%	2.343%
21	4.315	1000	1003	1008	rBV7	1641	1888	0.07%	0.009%
22	4.392	1014	1027	1059	rVB	422291	1017182	35.40%	4.631%
23	4.553	1073	1077	1080	rBV4	1653	1430	0.05%	0.007%
24	4.621	1094	1098	1101	rBV7	2577	2083	0.07%	0.009%
25	4.711	1120	1126	1129	rBV7	2175	2265	0.08%	0.010%
26	4.852	1167	1170	1172	rBV3	1444	1019	0.04%	0.005%
27	4.920	1189	1191	1193	rBV3	1108	480	0.02%	0.002%
28	4.968	1204	1206	1208	rVB3	1913	689	0.02%	0.003%
29	4.997	1212	1215	1219	rBV4	2117	1495	0.05%	0.007%
30	5.093	1228	1245	1257	rBV2	986088	2521046	87.74%	11.478%
31	5.499	1369	1371	1373	rBV2	2034	1027	0.04%	0.005%
32	5.659	1408	1421	1439	rBV	882562	1740149	60.56%	7.923%
33	6.113	1550	1562	1588	rVB	558215	1132039	39.40%	5.154%
34	6.531	1689	1692	1694	rBV4	1301	894	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014122.D
 Acq On : 18 Dec 2019 15:21
 Operator : SY/MD
 Sample : K6356-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.595	1710	1712	1720	rVB8	2299	1854	0.06%	0.008%
36	6.765	1763	1765	1767	rBV3	1833	560	0.02%	0.003%
37	6.810	1774	1779	1782	rBV7	1846	2114	0.07%	0.010%
38	6.878	1793	1800	1803	rBV7	1807	2789	0.10%	0.013%
39	6.942	1818	1820	1822	rBV3	1040	571	0.02%	0.003%
40	6.978	1829	1831	1833	rBV3	2464	1121	0.04%	0.005%
41	7.026	1835	1846	1865	rVV	264577	474217	16.50%	2.159%
42	7.357	1935	1949	1971	rBV	1049477	1848885	64.34%	8.418%
43	7.659	2033	2043	2062	rBV	201349	338139	11.77%	1.540%
44	7.926	2124	2126	2129	rVB3	2392	1198	0.04%	0.005%
45	7.945	2129	2132	2133	rBV2	2310	1164	0.04%	0.005%
46	8.084	2172	2175	2177	rBV4	1831	1195	0.04%	0.005%
47	8.125	2178	2188	2223	rVV2	563020	1164351	40.52%	5.301%
48	8.572	2325	2327	2328	rBV2	1916	757	0.03%	0.003%
49	8.604	2335	2337	2340	rVB4	1993	816	0.03%	0.004%
50	8.624	2340	2343	2345	rBV3	1513	837	0.03%	0.004%
51	8.707	2366	2369	2373	rBV4	1789	1461	0.05%	0.007%
52	8.762	2383	2386	2387	rBV3	1780	861	0.03%	0.004%
53	8.891	2414	2426	2432	rBV	1399915	2372981	82.58%	10.804%
54	9.270	2540	2544	2545	rBV4	3833	2368	0.08%	0.011%
55	9.344	2565	2567	2568	rBV2	1822	635	0.02%	0.003%
56	9.402	2582	2585	2588	rBV4	1367	1193	0.04%	0.005%
57	9.440	2594	2597	2603	rBV8	2098	2626	0.09%	0.012%
58	9.611	2646	2650	2652	rBV5	1660	1376	0.05%	0.006%
59	9.646	2659	2661	2664	rBV3	2088	1418	0.05%	0.006%
60	9.698	2674	2677	2678	rBV3	1624	973	0.03%	0.004%
61	9.817	2712	2714	2717	rBV4	967	548	0.02%	0.002%
62	9.900	2738	2740	2746	rVB6	2035	2021	0.07%	0.009%
63	9.932	2746	2750	2754	rBV5	2903	1892	0.07%	0.009%
64	10.035	2780	2782	2785	rBV4	1131	522	0.02%	0.002%
65	10.051	2785	2787	2788	rBV2	1279	608	0.02%	0.003%
66	10.157	2816	2820	2823	rBV4	2274	1283	0.04%	0.006%
67	10.209	2831	2836	2837	rBV5	1425	866	0.03%	0.004%
68	10.254	2837	2850	2872	rVV	776726	1242519	43.24%	5.657%
69	10.511	2926	2930	2933	rBV6	2182	1359	0.05%	0.006%
70	10.563	2944	2946	2950	rBV6	1446	889	0.03%	0.004%
71	10.592	2954	2955	2959	rVB3	2670	1162	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121819\
 Data File : VV014122.D
 Acq On : 18 Dec 2019 15:21
 Operator : SY/MD
 Sample : K6356-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.617	2959	2963	2965	rBV5	2104	1537	0.05%	0.007%
73	10.662	2975	2977	2980	rVB3	1840	734	0.03%	0.003%
74	10.714	2991	2993	2996	rVB4	1980	763	0.03%	0.003%
75	10.784	3013	3015	3016	rBV2	1181	609	0.02%	0.003%
76	10.833	3027	3030	3033	rBV3	1555	1343	0.05%	0.006%
77	11.013	3084	3086	3087	rBV2	1277	519	0.02%	0.002%
78	11.055	3094	3099	3106	rBV10	2498	2918	0.10%	0.013%
79	11.093	3106	3111	3116	rBV8	1771	1913	0.07%	0.009%
80	11.154	3128	3130	3132	rBV3	1392	494	0.02%	0.002%
81	11.170	3132	3135	3139	rBV6	1393	1275	0.04%	0.006%
82	11.222	3144	3151	3161	rVV3	54098	85092	2.96%	0.387%
83	11.289	3161	3172	3198	rVB2	1307835	2738931	95.32%	12.471%
84	11.669	3277	3290	3315	rBV3	1292488	2873440	100.00%	13.083%
85	11.948	3375	3377	3381	rVB5	2705	1651	0.06%	0.008%
86	11.971	3381	3384	3385	rBV3	1782	1006	0.04%	0.005%
87	12.026	3399	3401	3403	rBV3	1126	577	0.02%	0.003%
88	12.061	3410	3412	3415	rBV4	2512	1568	0.05%	0.007%
89	12.251	3469	3471	3473	rBV3	1044	606	0.02%	0.003%
90	12.325	3492	3494	3498	rBV3	1461	1115	0.04%	0.005%
91	12.350	3498	3502	3504	rBV5	1513	1120	0.04%	0.005%
92	12.399	3513	3517	3520	rBV5	1972	1512	0.05%	0.007%
93	12.495	3545	3547	3551	rBV4	1603	915	0.03%	0.004%
94	12.688	3599	3607	3615	rBV6	10152	17644	0.61%	0.080%
95	12.817	3645	3647	3650	rBV4	1478	688	0.02%	0.003%
96	12.871	3658	3664	3667	rBV7	2129	2679	0.09%	0.012%
97	13.305	3787	3799	3818	rBV	119698	196017	6.82%	0.892%
98	13.408	3829	3831	3837	rBV7	2112	1856	0.06%	0.008%
99	13.788	3942	3949	3965	rVB2	45162	75206	2.62%	0.342%
100	13.910	3984	3987	3988	rBV3	2280	1044	0.04%	0.005%


Sum of corrected areas: 21963233

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121819\
Data File : VV014122.D
Acq On : 18 Dec 2019 15:21
Operator : SY/MD
Sample : K6356-05DL 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D40DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

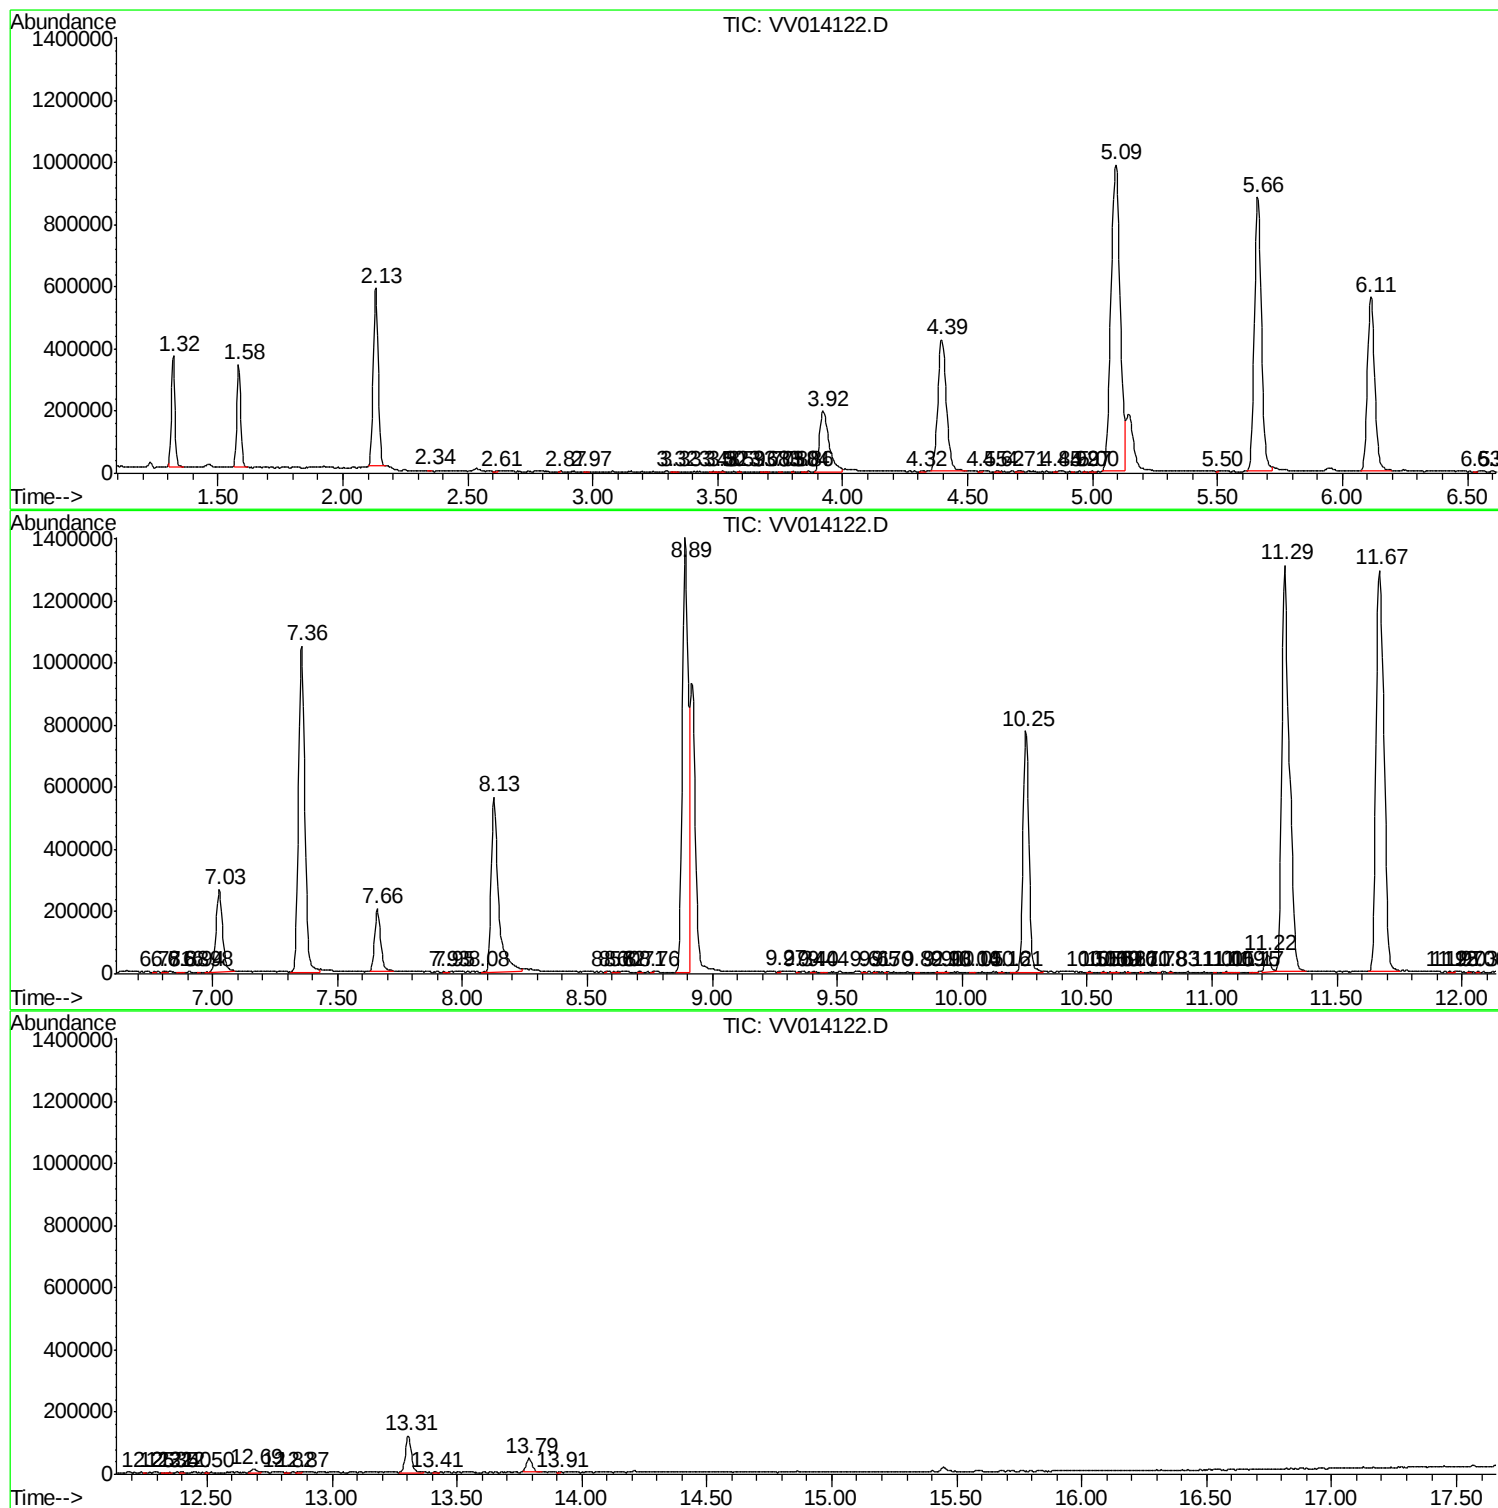

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121819\
Data File : VV014122.D
Acq On : 18 Dec 2019 15:21
Operator : SY/MD
Sample : K6356-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D40DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121819\
Data File : VV014122.D
Acq On : 18 Dec 2019 15:21
Operator : SY/MD
Sample : K6356-05DL 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0D40DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc