


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121819\
 Data File : VV014108.D
 Acq On : 18 Dec 2019 09:02
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis
 Last Update : Thu Dec 19 07:06:05 2019

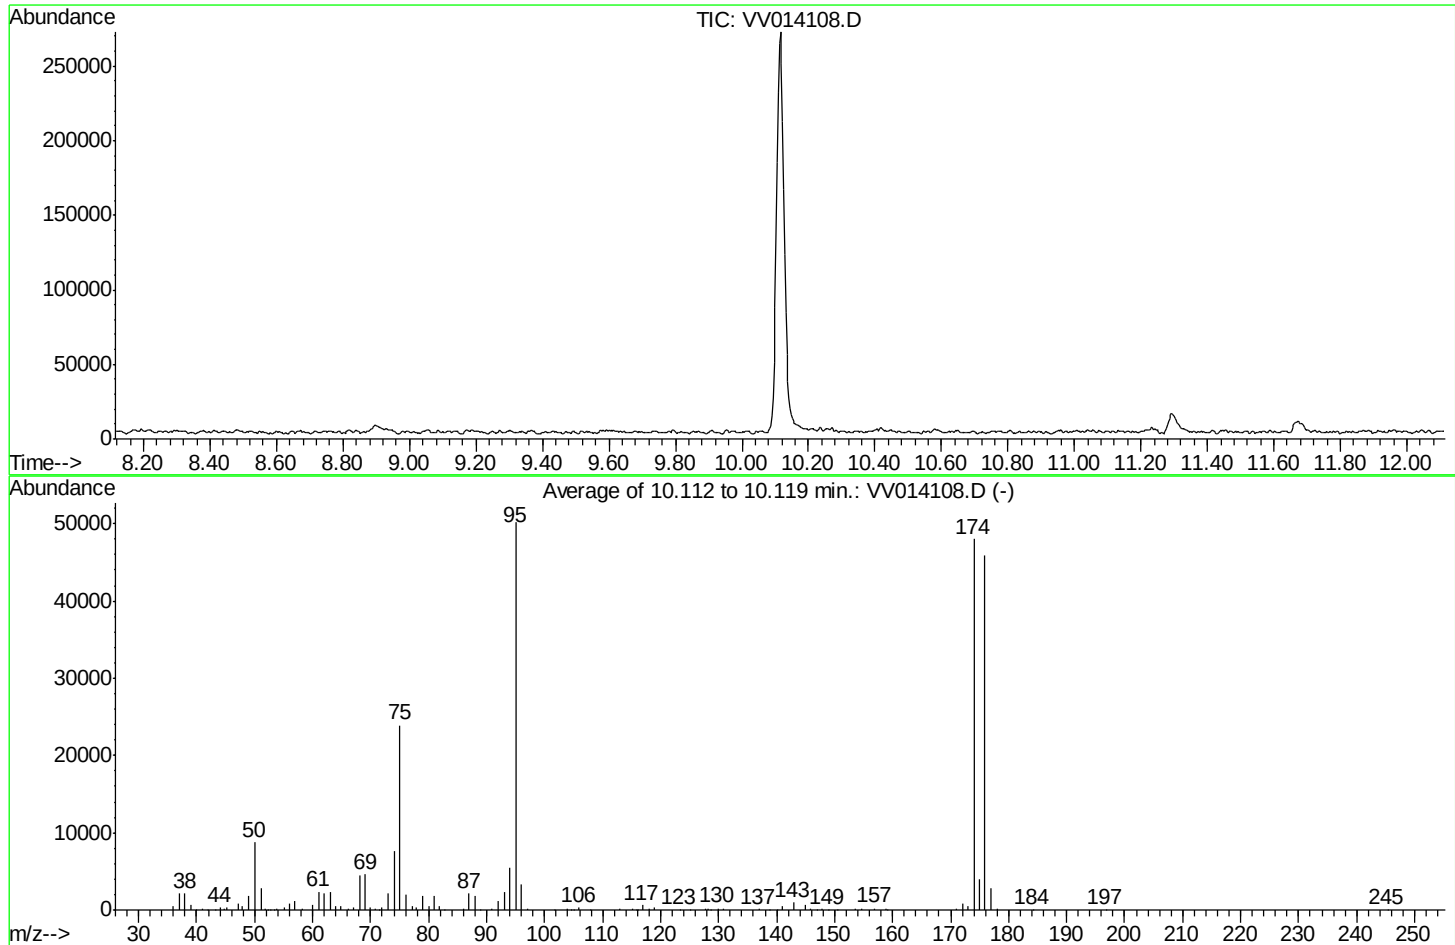

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	8753	PASS
75	95	30	80	47.6	23882	PASS
95	95	100	100	100.0	50173	PASS
96	95	5	9	6.6	3334	PASS
173	174	0.00	2	1.1	540	PASS
174	95	50	120	95.6	47986	PASS
175	174	5	9	8.3	3986	PASS
176	174	95	101	95.5	45824	PASS
177	176	5	9	6.2	2837	PASS

m/z	Abundance
36.00	634.0
37.00	2350.0
38.00	2070.0
39.10	951.0
40.10	646.0
42.60	102.0
43.30	208.0
44.00	983.0
44.80	336.0
45.20	427.0
45.80	139.0
47.10	977.0
47.90	591.0
49.00	2046.0
50.00	8691.0
51.10	3000.0
52.20	214.0
52.70	169.0
53.20	118.0
53.80	112.0
54.30	141.0
55.10	234.0
56.10	885.0
56.90	1308.0
60.00	606.0
61.00	2568.0
62.00	2197.0
63.00	2393.0
64.10	613.0
64.90	452.0
66.10	172.0
67.00	372.0
68.00	4525.0
69.10	4719.0
70.00	447.0
70.90	206.0
72.00	286.0
73.00	2094.0
74.00	7994.0
75.00	24152.0
76.10	2110.0
77.00	495.0
77.90	234.0
78.90	1774.0
80.10	462.0
81.00	1811.0
81.90	477.0
82.60	129.0
85.90	143.0
87.00	2127.0
88.00	2051.0
88.80	142.0
90.90	259.0
91.90	1102.0
93.00	2065.0
94.00	5517.0
95.00	51192.0
96.00	3416.0
97.00	170.0
103.90	212.0
105.10	128.0
105.90	315.0
107.90	110.0
112.90	106.0
115.20	152.0
116.90	654.0
117.90	241.0
118.90	373.0
125.00	103.0
127.60	245.0
128.10	189.0
129.90	232.0
130.90	194.0
136.90	110.0
138.80	136.0
141.00	472.0
142.90	955.0
144.90	580.0
145.90	182.0
147.80	249.0
148.90	141.0
153.60	158.0
154.70	179.0
156.90	256.0
159.10	117.0
170.90	282.0
172.10	945.0
174.00	47880.0
175.00	3897.0
175.90	45456.0
176.90	2890.0
177.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

184.20104.0

245.30108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	723.0
37.00	2356.0
38.00	2199.0
39.10	945.0
40.00	677.0
41.00	163.0
41.80	103.0
42.70	104.0
43.40	201.0
44.00	910.0
44.80	352.0
45.20	457.0
47.10	938.0
47.90	543.0
49.10	1877.0
50.00	9218.0
51.10	2924.0
51.90	226.0
53.90	117.0
54.30	138.0
55.10	264.0
56.10	938.0
57.00	1256.0
58.20	123.0
60.00	649.0
61.00	2522.0
62.00	2305.0
63.00	2502.0
64.10	582.0
64.90	515.0
66.00	156.0
67.10	281.0
68.00	4605.0
69.10	4677.0
70.00	575.0
70.80	207.0
72.00	298.0
73.00	2179.0
74.00	7869.0
75.00	24800.0
76.10	2122.0
77.10	459.0
78.00	312.0
78.90	1886.0
80.00	510.0
81.00	1848.0
81.90	455.0
82.70	103.0
86.00	185.0
87.00	2203.0
88.00	1906.0
88.90	109.0
90.90	241.0
91.90	1136.0
93.00	2403.0
94.00	5541.0
95.00	51864.0
96.10	3462.0
97.00	157.0
103.90	193.0
104.60	101.0
105.90	255.0
107.90	102.0
113.00	127.0
115.00	102.0
115.80	124.0
116.90	649.0
117.90	251.0
119.00	372.0
123.30	109.0
125.00	102.0
127.70	206.0
128.10	202.0
129.80	222.0
130.90	174.0
136.90	121.0
138.80	114.0
140.90	478.0
142.90	1009.0
145.00	669.0
145.80	166.0
147.00	107.0
147.80	234.0
148.90	122.0
153.70	123.0
154.70	160.0
156.90	226.0
158.80	139.0
170.90	193.0
172.00	937.0
172.90	811.0
174.00	49640.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

174.90	4146.0
175.90	47592.0
177.00	2999.0
178.00	128.0
196.70	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.10	718.0
37.00	2149.0
38.00	2185.0
39.10	930.0
40.00	761.0
41.00	196.0
41.80	133.0
43.40	154.0
44.00	883.0
45.20	423.0
47.10	732.0
48.00	436.0
49.10	1638.0
50.10	8352.0
51.10	2641.0
51.90	196.0
53.30	128.0
54.00	142.0
55.20	268.0
56.00	836.0
57.00	1017.0
58.10	154.0
60.10	601.0
61.00	2073.0
62.00	2217.0
63.00	2150.0
64.10	521.0
64.90	557.0
66.00	121.0
67.10	212.0
68.10	4418.0
69.10	4357.0
70.00	573.0
70.90	182.0
71.40	174.0
72.00	291.0
73.00	2023.0
74.00	6943.0
75.10	22696.0
76.00	1996.0
77.20	451.0
78.00	338.0
78.90	1788.0
80.00	470.0
80.90	1736.0
81.90	410.0
86.00	218.0
87.00	2107.0
88.00	1712.0
90.90	191.0
91.90	1124.0
93.00	2405.0
94.00	5246.0
95.00	47464.0
96.10	3125.0
97.00	111.0
101.70	105.0
103.90	157.0
105.90	202.0
113.00	157.0
114.90	111.0
115.70	133.0
116.10	126.0
116.90	567.0
118.00	225.0
119.00	340.0
128.10	228.0
128.70	142.0
129.80	246.0
130.90	124.0
137.00	123.0
140.00	108.0
140.90	422.0
143.00	922.0
145.00	707.0
145.70	147.0
147.80	138.0
150.40	114.0
156.90	180.0
158.80	165.0
172.10	843.0
172.90	809.0
174.00	46440.0
174.90	3917.0
175.90	44424.0
177.00	2932.0
178.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.10	159.0
35.90	219.0
37.20	167.0
38.90	154.0
39.30	173.0
40.00	630.0
42.10	114.0
42.70	166.0
43.30	140.0
44.00	616.0
45.20	103.0
45.90	142.0
47.50	210.0
48.80	111.0
54.50	114.0
55.70	115.0
60.60	126.0
62.20	105.0
63.90	142.0
70.20	129.0
98.00	118.0
129.30	128.0
176.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84