

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019692.D
 Acq On : 18 Dec 2020 12:09
 Operator : SY/MD
 Sample : L5062-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	275983	270922	13.62%	1.851%
2	1.570	142	149	164	rBV	232463	261459	13.14%	1.786%
3	2.110	308	317	348	rVB	382829	602576	30.29%	4.116%
4	3.110	625	628	631	rBV	356	235	0.01%	0.002%
5	3.164	643	645	646	rBV3	313	128	0.01%	0.001%
6	3.196	653	655	657	rBV	396	195	0.01%	0.001%
7	3.315	690	692	695	rBV2	448	296	0.01%	0.002%
8	3.425	721	726	730	rVB5	548	593	0.03%	0.004%
9	3.450	730	734	736	rBV3	583	494	0.02%	0.003%
10	3.470	738	740	745	rVB2	490	276	0.01%	0.002%
11	3.495	745	748	750	rBV3	534	351	0.02%	0.002%
12	3.614	779	785	790	rVB3	521	551	0.03%	0.004%
13	3.640	790	793	794	rBV2	359	205	0.01%	0.001%
14	3.676	803	804	805	rBV2	92	30	0.00%	0.000%
15	3.698	805	811	814	rBV3	611	611	0.03%	0.004%
16	3.733	819	822	825	rBV3	447	347	0.02%	0.002%
17	3.756	825	829	831	rBV2	429	305	0.02%	0.002%
18	3.836	852	854	856	rBV2	289	142	0.01%	0.001%
19	3.888	857	870	917	rBV	163127	513313	25.80%	3.507%
20	4.351	997	1014	1040	rBV	322158	801018	40.26%	5.472%
21	4.766	1138	1143	1145	rBV3	611	605	0.03%	0.004%
22	4.785	1148	1149	1151	rVB2	413	130	0.01%	0.001%
23	4.817	1155	1159	1160	rBV	540	414	0.02%	0.003%
24	4.872	1171	1176	1180	rBV5	557	536	0.03%	0.004%
25	4.930	1191	1194	1196	rBV2	325	235	0.01%	0.002%
26	4.981	1208	1210	1211	rBV	347	154	0.01%	0.001%
27	5.048	1213	1231	1262	rVV2	767401	1989552	100.00%	13.591%
28	5.383	1333	1335	1337	rBV3	611	261	0.01%	0.002%
29	5.560	1387	1390	1391	rBV	565	297	0.01%	0.002%
30	5.618	1395	1408	1436	rBV	589474	1191386	59.88%	8.139%
31	5.865	1484	1485	1486	rBV	443	122	0.01%	0.001%
32	5.910	1486	1499	1517	rVV2	15294	34507	1.73%	0.236%
33	6.071	1536	1549	1575	rBV	458988	938574	47.18%	6.412%
34	6.373	1641	1643	1650	rVB3	756	765	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019692.D
 Acq On : 18 Dec 2020 12:09
 Operator : SY/MD
 Sample : L5062-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.412	1650	1655	1659	rBV4	588	448	0.02%	0.003%
36	6.428	1659	1660	1663	rBV	314	132	0.01%	0.001%
37	6.444	1663	1665	1670	rBV2	358	327	0.02%	0.002%
38	6.489	1677	1679	1680	rBV	320	89	0.00%	0.001%
39	6.544	1694	1696	1699	rVB2	626	203	0.01%	0.001%
40	6.560	1699	1701	1702	rBV	431	201	0.01%	0.001%
41	6.592	1709	1711	1715	rBV3	346	199	0.01%	0.001%
42	6.634	1721	1724	1725	rBV	515	273	0.01%	0.002%
43	6.749	1757	1760	1762	rBV2	573	391	0.02%	0.003%
44	6.785	1769	1771	1776	rVB3	778	556	0.03%	0.004%
45	6.820	1776	1782	1785	rBV3	343	413	0.02%	0.003%
46	6.862	1791	1795	1799	rBV3	365	348	0.02%	0.002%
47	6.891	1802	1804	1809	rVB3	357	171	0.01%	0.001%
48	6.946	1820	1821	1823	rBV2	452	214	0.01%	0.001%
49	6.987	1823	1834	1857	rVV	232396	417531	20.99%	2.852%
50	7.238	1908	1912	1916	rBV6	730	812	0.04%	0.006%
51	7.318	1925	1937	1957	rBV	759118	1326984	66.70%	9.065%
52	7.624	2021	2032	2055	rBV	164134	291127	14.63%	1.989%
53	7.942	2120	2131	2139	rBV3	7607	12654	0.64%	0.086%
54	8.010	2150	2152	2156	rVB2	609	310	0.02%	0.002%
55	8.029	2156	2158	2161	rBV4	708	340	0.02%	0.002%
56	8.090	2166	2177	2213	rBV	581793	1064322	53.50%	7.271%
57	8.502	2302	2305	2310	rBV4	722	711	0.04%	0.005%
58	8.733	2375	2377	2383	rBV3	764	695	0.03%	0.005%
59	8.855	2403	2415	2441	rBV	875948	1398546	70.29%	9.554%
60	9.122	2496	2498	2500	rBV2	570	286	0.01%	0.002%
61	9.367	2572	2574	2578	rVB	431	188	0.01%	0.001%
62	9.463	2602	2604	2606	rBV2	209	114	0.01%	0.001%
63	9.476	2606	2608	2611	rBV3	274	212	0.01%	0.001%
64	9.518	2616	2621	2623	rBV2	508	463	0.02%	0.003%
65	9.543	2626	2629	2630	rVV2	503	266	0.01%	0.002%
66	9.560	2630	2634	2640	rVB4	1018	1119	0.06%	0.008%
67	9.585	2640	2642	2643	rBV	404	137	0.01%	0.001%
68	9.733	2686	2688	2689	rBV2	587	265	0.01%	0.002%
69	9.788	2702	2705	2708	rBV3	531	346	0.02%	0.002%
70	9.836	2717	2720	2722	rBV3	435	287	0.01%	0.002%
71	9.907	2740	2742	2743	rBV	308	101	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019692.D
 Acq On : 18 Dec 2020 12:09
 Operator : SY/MD
 Sample : L5062-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	9.945	2752	2754	2757	rBV3	468	231	0.01%	0.002%
73	10.103	2801	2803	2807	rVB2	598	370	0.02%	0.003%
74	10.161	2817	2821	2827	rBV4	618	525	0.03%	0.004%
75	10.222	2827	2840	2863	rBV	611920	957744	48.14%	6.543%
76	10.463	2913	2915	2918	rVB2	355	186	0.01%	0.001%
77	10.479	2918	2920	2921	rBV2	273	107	0.01%	0.001%
78	10.550	2937	2942	2946	rBV2	1054	859	0.04%	0.006%
79	10.656	2972	2975	2978	rBV3	473	340	0.02%	0.002%
80	10.675	2979	2981	2983	rVV	411	167	0.01%	0.001%
81	10.756	3003	3006	3008	rBV2	408	327	0.02%	0.002%
82	10.788	3013	3016	3019	rBV4	464	336	0.02%	0.002%
83	11.055	3098	3099	3100	rBV4	280	55	0.00%	0.000%
84	11.135	3121	3124	3127	rBV2	440	340	0.02%	0.002%
85	11.212	3147	3148	3150	rBV	487	199	0.01%	0.001%
86	11.254	3150	3161	3180	rBV	843222	1287596	64.72%	8.796%
87	11.508	3238	3240	3242	rBV3	568	319	0.02%	0.002%
88	11.630	3265	3278	3298	rBV	805972	1251901	62.92%	8.552%
89	11.887	3353	3358	3362	rBV3	723	725	0.04%	0.005%
90	12.190	3450	3452	3453	rBV	585	247	0.01%	0.002%
91	12.852	3655	3658	3661	rBV2	835	761	0.04%	0.005%
92	12.932	3678	3683	3686	rBV3	989	961	0.05%	0.007%
93	13.138	3745	3747	3750	rBV2	717	404	0.02%	0.003%
94	13.614	3893	3895	3900	rBV3	710	455	0.02%	0.003%


Sum of corrected areas: 14638521

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121820\
Data File : VV019692.D
Acq On : 18 Dec 2020 12:09
Operator : SY/MD
Sample : L5062-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B30

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

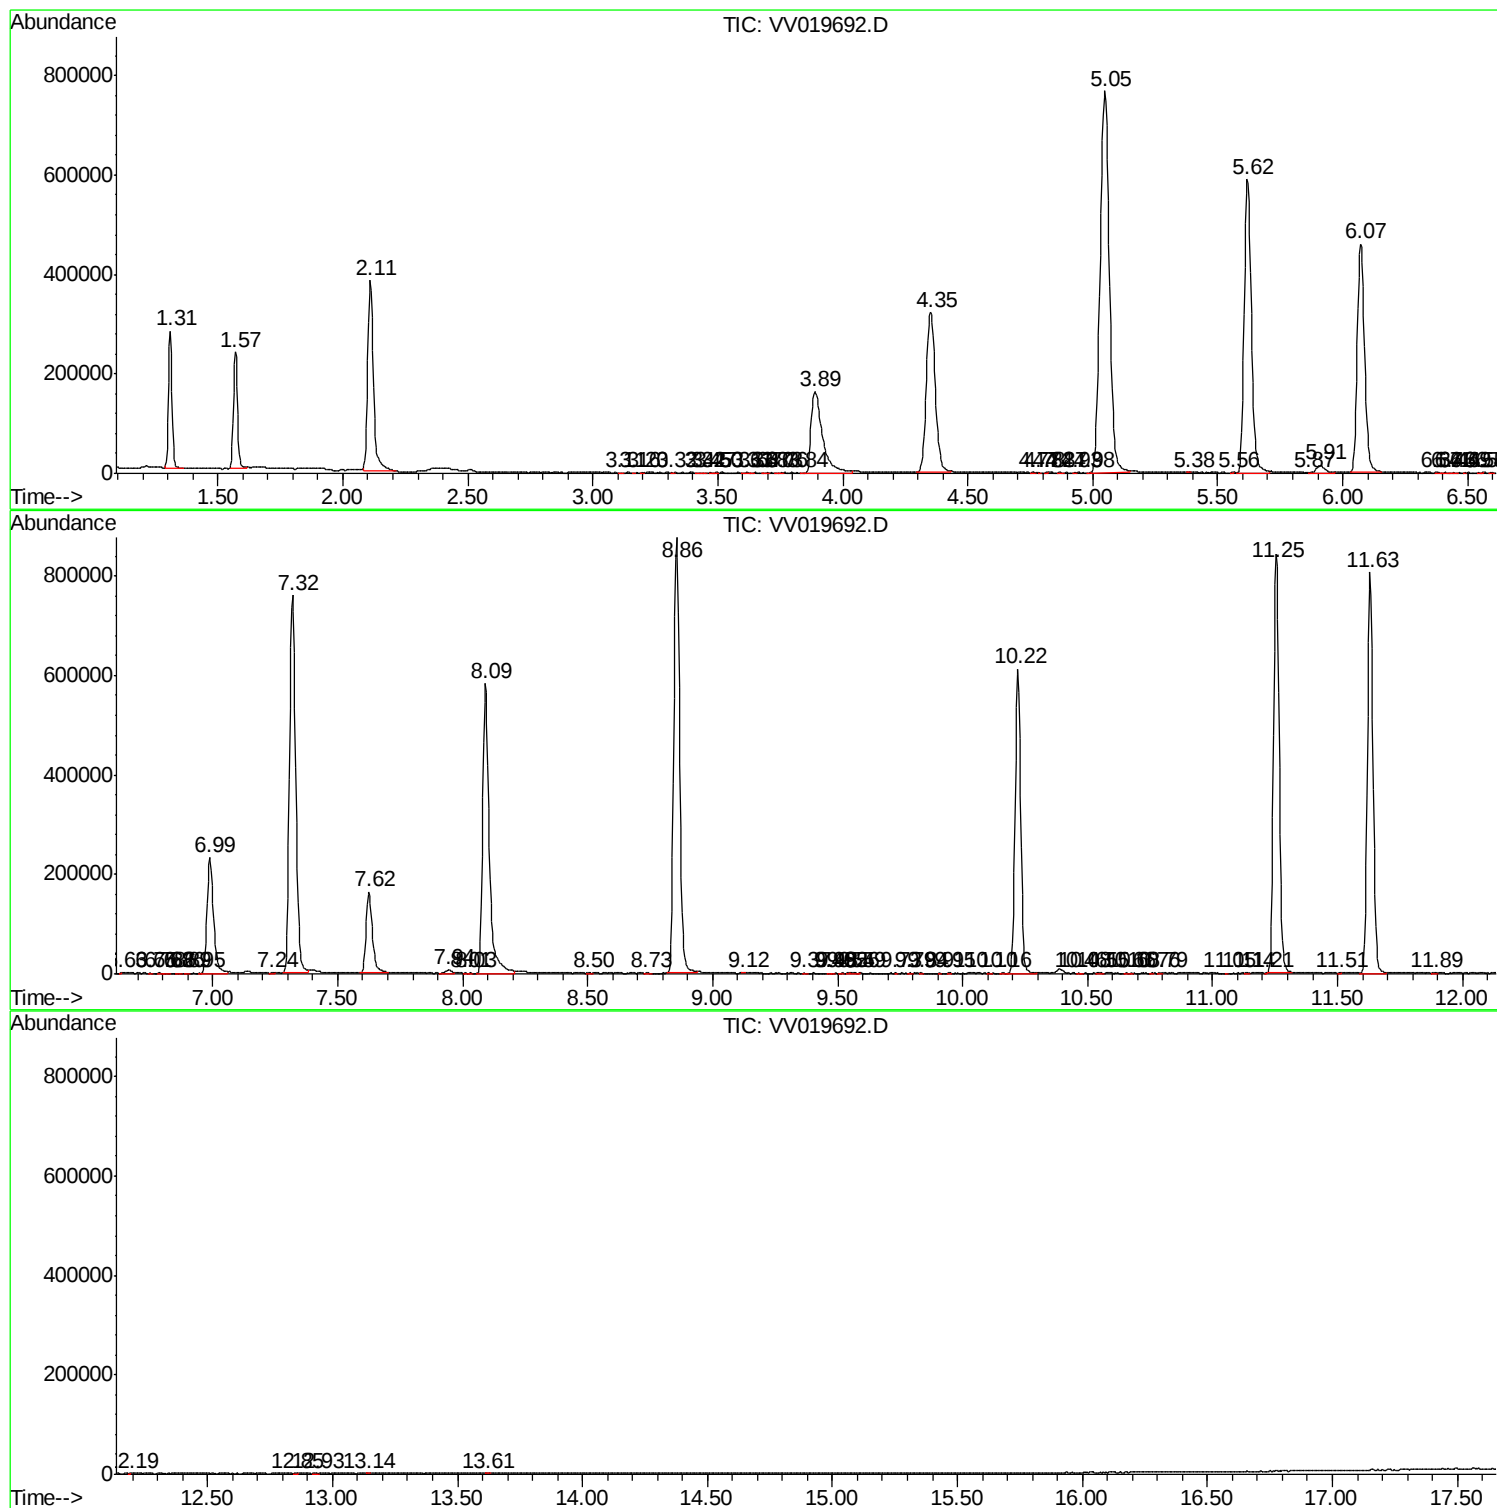

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019692.D
Acq On : 18 Dec 2020 12:09
Operator : SY/MD
Sample : L5062-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B30

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019692.D
Acq On : 18 Dec 2020 12:09
Operator : SY/MD
Sample : L5062-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B30

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc