

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019701.D
 Acq On : 18 Dec 2020 15:44
 Operator : SY/MD
 Sample : L5098-06 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	314635	320299	13.98%	1.823%
2	1.569	142	149	164	rVB	263000	297054	12.96%	1.691%
3	2.109	308	317	351	rVB	522473	804850	35.13%	4.582%
4	2.576	460	462	463	rBV	543	183	0.01%	0.001%
5	2.714	503	505	507	rBV2	542	302	0.01%	0.002%
6	2.769	518	522	526	rBV4	957	854	0.04%	0.005%
7	2.933	568	573	578	rBV3	592	536	0.02%	0.003%
8	2.981	586	588	589	rBV	459	228	0.01%	0.001%
9	3.045	604	608	610	rBV4	753	528	0.02%	0.003%
10	3.087	618	621	625	rVB2	730	440	0.02%	0.003%
11	3.109	625	628	629	rBV3	363	161	0.01%	0.001%
12	3.228	662	665	668	rBV2	424	330	0.01%	0.002%
13	3.312	687	691	692	rBV	305	200	0.01%	0.001%
14	3.344	699	701	703	rBV2	233	105	0.00%	0.001%
15	3.357	703	705	707	rBV2	553	214	0.01%	0.001%
16	3.370	707	709	710	rBV	376	167	0.01%	0.001%
17	3.396	715	717	724	rVB4	471	455	0.02%	0.003%
18	3.460	733	737	738	rBV	471	306	0.01%	0.002%
19	3.508	749	752	753	rBV	580	225	0.01%	0.001%
20	3.547	762	764	768	rVB2	741	405	0.02%	0.002%
21	3.569	768	771	773	rBV2	530	289	0.01%	0.002%
22	3.614	784	785	787	rVV	406	154	0.01%	0.001%
23	3.627	787	789	790	rVB	185	49	0.00%	0.000%
24	3.656	796	798	801	rBV2	228	112	0.00%	0.001%
25	3.714	814	816	817	rBV	332	127	0.01%	0.001%
26	3.778	834	836	842	rBV3	413	338	0.01%	0.002%
27	3.817	846	848	850	rVB	395	145	0.01%	0.001%
28	3.826	850	851	852	rBV	222	73	0.00%	0.000%
29	3.855	855	860	861	rBV2	557	405	0.02%	0.002%
30	3.894	861	872	912	rBV	166435	540483	23.59%	3.077%
31	4.354	1000	1015	1042	rVB	364694	889523	38.82%	5.064%
32	4.617	1095	1097	1099	rBV2	551	271	0.01%	0.002%
33	4.772	1143	1145	1149	rVB2	511	268	0.01%	0.002%
34	4.817	1155	1159	1161	rBV2	382	298	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019701.D
 Acq On : 18 Dec 2020 15:44
 Operator : SY/MD
 Sample : L5098-06 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	4.916	1187	1190	1193	rBV2	510	320	0.01%	0.002%
36	4.936	1193	1196	1197	rBV3	436	226	0.01%	0.001%
37	5.051	1214	1232	1258	rBV2	894648	2291285	100.00%	13.044%
38	5.322	1314	1316	1319	rBV2	624	340	0.01%	0.002%
39	5.473	1360	1363	1364	rBV2	342	170	0.01%	0.001%
40	5.550	1383	1387	1388	rBV	520	350	0.02%	0.002%
41	5.621	1396	1409	1446	rBV	716176	1439655	62.83%	8.196%
42	5.910	1487	1499	1518	rVB3	17935	40121	1.75%	0.228%
43	6.074	1535	1550	1581	rBV	518336	1054861	46.04%	6.005%
44	6.415	1653	1656	1660	rBV4	682	468	0.02%	0.003%
45	6.482	1672	1677	1679	rBV	298	268	0.01%	0.002%
46	6.518	1685	1688	1689	rBV2	379	217	0.01%	0.001%
47	6.534	1689	1693	1696	rVV2	576	423	0.02%	0.002%
48	6.559	1699	1701	1704	rBV	483	281	0.01%	0.002%
49	6.585	1708	1709	1713	rVB	406	201	0.01%	0.001%
50	6.604	1713	1715	1716	rBV	269	123	0.01%	0.001%
51	6.633	1716	1724	1726	rBV4	1066	1244	0.05%	0.007%
52	6.714	1747	1749	1753	rVB3	707	387	0.02%	0.002%
53	6.759	1760	1763	1764	rBV2	520	246	0.01%	0.001%
54	6.810	1778	1779	1781	rVB	226	82	0.00%	0.000%
55	6.846	1787	1790	1793	rBV3	456	279	0.01%	0.002%
56	6.923	1813	1814	1815	rVB3	235	45	0.00%	0.000%
57	6.990	1822	1835	1862	rBV	299381	542585	23.68%	3.089%
58	7.186	1893	1896	1899	rVB5	1102	696	0.03%	0.004%
59	7.318	1925	1937	1960	rBV	1018888	1778025	77.60%	10.122%
60	7.624	2021	2032	2057	rBV	208046	364449	15.91%	2.075%
61	7.858	2103	2105	2106	rBV	384	120	0.01%	0.001%
62	7.903	2116	2119	2121	rVB2	700	335	0.01%	0.002%
63	7.984	2137	2144	2154	rVB7	7796	13328	0.58%	0.076%
64	8.035	2159	2160	2162	rBV2	331	138	0.01%	0.001%
65	8.093	2167	2178	2215	rBV	643359	1172148	51.16%	6.673%
66	8.569	2325	2326	2330	rBV4	571	380	0.02%	0.002%
67	8.807	2397	2400	2403	rBV3	690	334	0.01%	0.002%
68	8.855	2403	2415	2442	rBV	1086468	1734848	75.72%	9.876%
69	9.231	2530	2532	2534	rBV	323	156	0.01%	0.001%
70	9.244	2534	2536	2537	rBV	384	187	0.01%	0.001%
71	9.299	2551	2553	2556	rBV4	495	254	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019701.D
 Acq On : 18 Dec 2020 15:44
 Operator : SY/MD
 Sample : L5098-06 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	9.411	2585	2588	2589	rBV2	404	216	0.01%	0.001%
73	9.540	2625	2628	2630	rBV3	692	429	0.02%	0.002%
74	9.569	2635	2637	2639	rVB3	520	247	0.01%	0.001%
75	9.585	2639	2642	2644	rBV	608	379	0.02%	0.002%
76	9.720	2683	2684	2686	rBV2	438	158	0.01%	0.001%
77	9.794	2705	2707	2708	rBV	233	76	0.00%	0.000%
78	9.833	2717	2719	2723	rBV2	568	359	0.02%	0.002%
79	10.071	2789	2793	2794	rBV	441	299	0.01%	0.002%
80	10.222	2827	2840	2862	rBV	650545	1032204	45.05%	5.876%
81	10.386	2888	2891	2892	rBV2	621	379	0.02%	0.002%
82	10.550	2938	2942	2944	rBV2	661	443	0.02%	0.003%
83	10.643	2967	2971	2975	rBV2	802	721	0.03%	0.004%
84	10.858	3035	3038	3039	rBV2	739	445	0.02%	0.003%
85	11.025	3088	3090	3097	rBV4	712	482	0.02%	0.003%
86	11.193	3139	3142	3148	rVB5	831	758	0.03%	0.004%
87	11.254	3150	3161	3188	rBV	1062953	1639370	71.55%	9.333%
88	11.630	3266	3278	3303	rBV	1023481	1587730	69.29%	9.039%
89	11.951	3376	3378	3380	rBV2	423	216	0.01%	0.001%
90	12.431	3525	3527	3529	rBV	547	337	0.01%	0.002%
91	12.649	3593	3595	3596	rBV	488	200	0.01%	0.001%
92	12.739	3622	3623	3624	rBV	517	164	0.01%	0.001%


Sum of corrected areas: 17565564

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121820\
Data File : VV019701.D
Acq On : 18 Dec 2020 15:44
Operator : SY/MD
Sample : L5098-06 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

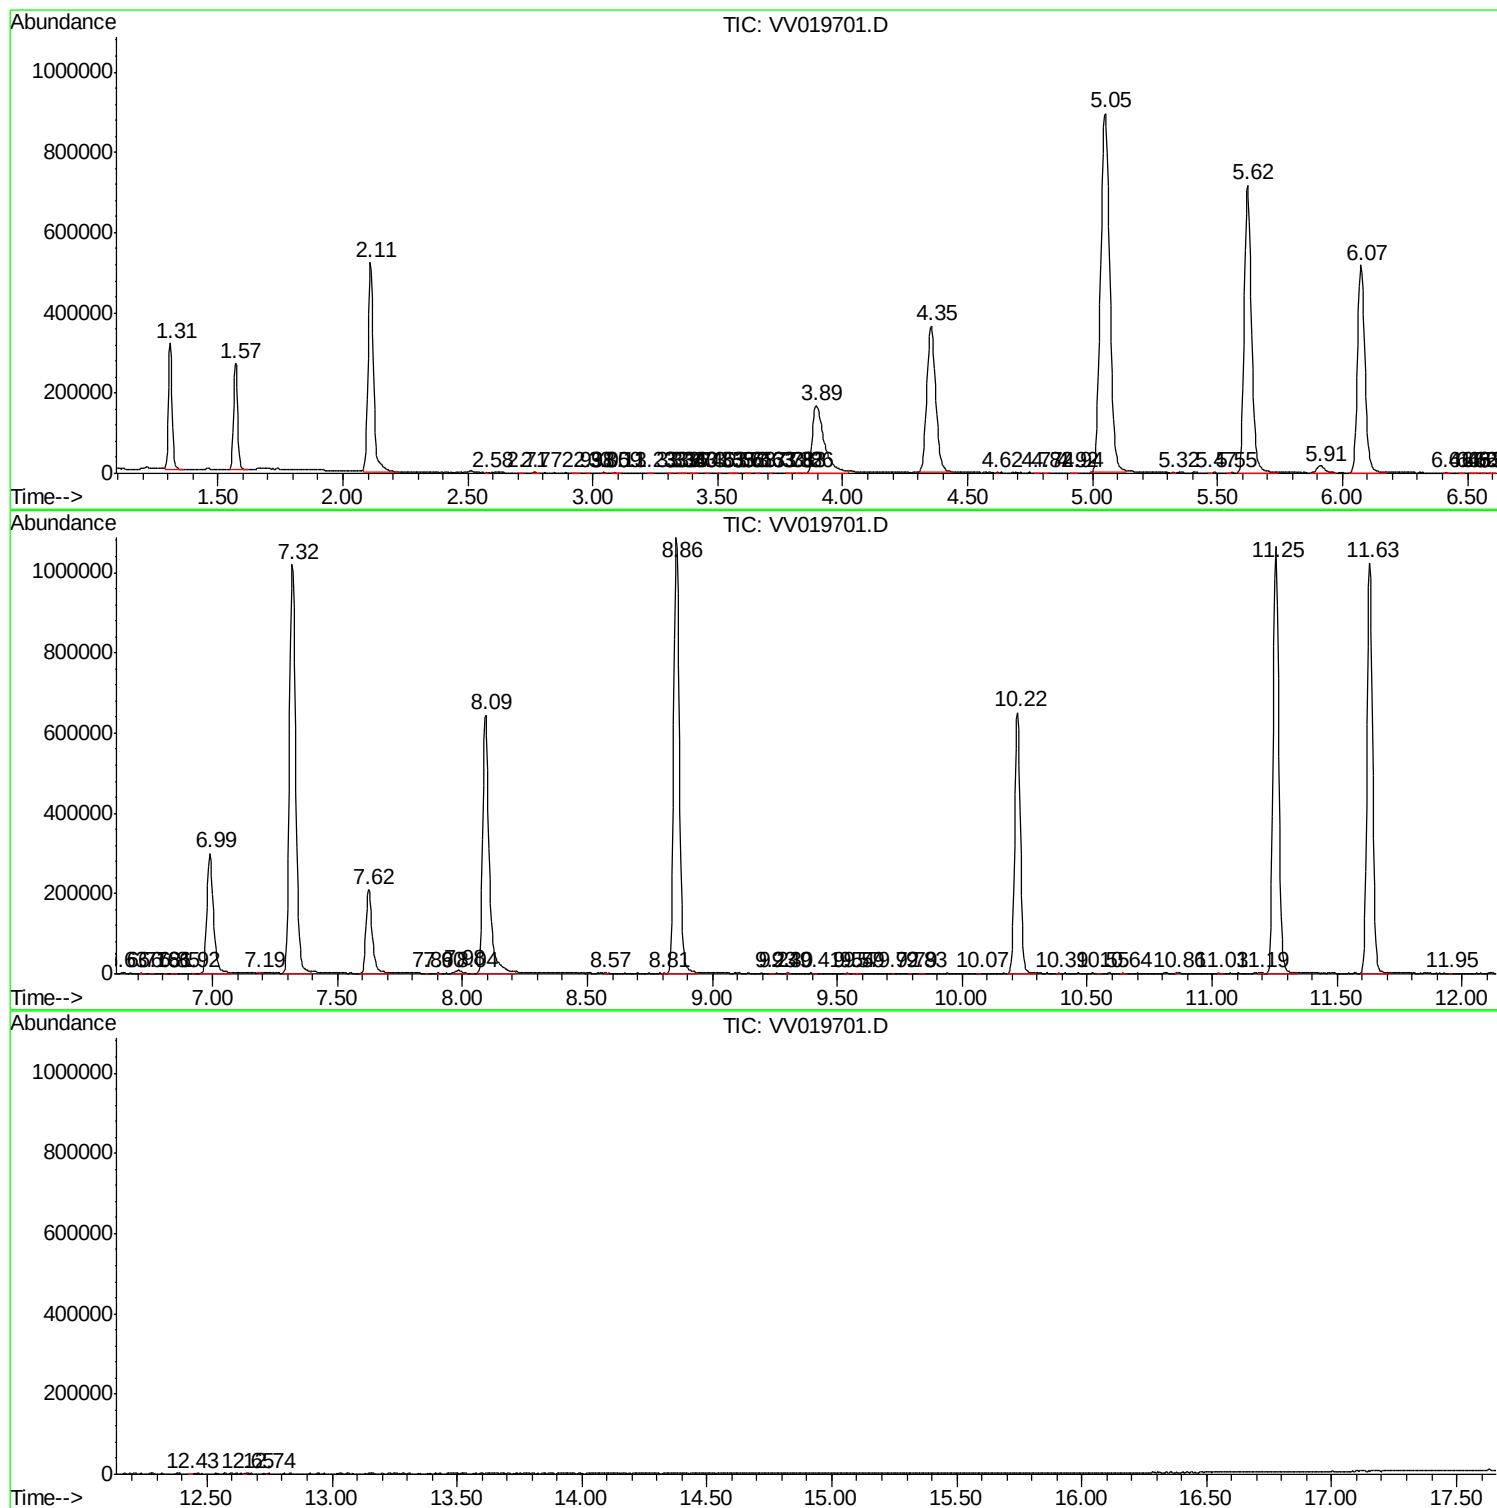

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019701.D
Acq On : 18 Dec 2020 15:44
Operator : SY/MD
Sample : L5098-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019701.D
Acq On : 18 Dec 2020 15:44
Operator : SY/MD
Sample : L5098-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc