

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019705.D
 Acq On : 18 Dec 2020 17:20
 Operator : SY/MD
 Sample : L5098-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	80	rVB	320492	313911	14.21%	1.868%
2	1.569	142	149	164	rBV	251665	287506	13.02%	1.711%
3	2.113	308	318	355	rVB	508361	801049	36.27%	4.767%
4	2.827	538	540	541	rBV	406	207	0.01%	0.001%
5	2.929	570	572	574	rVB	322	132	0.01%	0.001%
6	2.962	574	582	584	rBV5	857	1093	0.05%	0.007%
7	3.048	597	609	624	rVB2	10743	22768	1.03%	0.135%
8	3.110	626	628	629	rBV2	300	122	0.01%	0.001%
9	3.148	637	640	644	rVB3	615	347	0.02%	0.002%
10	3.171	644	647	649	rBV2	332	209	0.01%	0.001%
11	3.206	655	658	660	rBV3	604	491	0.02%	0.003%
12	3.302	685	688	690	rBV2	325	223	0.01%	0.001%
13	3.325	692	695	701	rVB4	658	793	0.04%	0.005%
14	3.360	701	706	708	rBV2	496	352	0.02%	0.002%
15	3.373	708	710	714	rVV2	280	195	0.01%	0.001%
16	3.392	714	716	718	rVV	217	69	0.00%	0.000%
17	3.409	718	721	728	rVV3	578	575	0.03%	0.003%
18	3.466	736	739	741	rBV2	335	208	0.01%	0.001%
19	3.499	746	749	752	rBV2	353	275	0.01%	0.002%
20	3.582	773	775	779	rBV2	244	178	0.01%	0.001%
21	3.611	779	784	786	rBV2	370	343	0.02%	0.002%
22	3.650	794	796	797	rBV	229	79	0.00%	0.000%
23	3.666	797	801	803	rBV3	575	425	0.02%	0.003%
24	3.888	859	870	903	rBV	159432	462311	20.93%	2.751%
25	4.354	999	1015	1048	rBV	347017	861734	39.02%	5.128%
26	4.807	1153	1156	1158	rBV2	639	342	0.02%	0.002%
27	4.849	1163	1169	1174	rBV5	562	619	0.03%	0.004%
28	4.894	1179	1183	1185	rBV3	430	298	0.01%	0.002%
29	4.958	1200	1203	1206	rBV2	409	252	0.01%	0.001%
30	5.052	1213	1232	1275	rBV2	851908	2208724	100.00%	13.144%
31	5.331	1315	1319	1321	rBV3	1070	794	0.04%	0.005%
32	5.482	1362	1366	1367	rBV2	455	309	0.01%	0.002%
33	5.621	1396	1409	1439	rBV	687757	1375993	62.30%	8.188%
34	5.852	1478	1481	1483	rBV3	745	486	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019705.D
 Acq On : 18 Dec 2020 17:20
 Operator : SY/MD
 Sample : L5098-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	5.910	1487	1499	1519	rVV2	28342	58936	2.67%	0.351%
36	6.074	1536	1550	1575	rBV	493067	1001057	45.32%	5.957%
37	6.457	1667	1669	1672	rBV	295	185	0.01%	0.001%
38	6.473	1672	1674	1679	rVB2	1022	621	0.03%	0.004%
39	6.492	1679	1680	1681	rBV	305	101	0.00%	0.001%
40	6.781	1766	1770	1771	rBV2	365	264	0.01%	0.002%
41	6.804	1775	1777	1782	rBV3	256	173	0.01%	0.001%
42	6.830	1782	1785	1789	rVB	345	218	0.01%	0.001%
43	6.852	1791	1792	1798	rVB2	303	149	0.01%	0.001%
44	6.894	1802	1805	1808	rBV	434	371	0.02%	0.002%
45	6.910	1808	1810	1811	rVB	351	112	0.01%	0.001%
46	6.923	1811	1814	1817	rBV3	237	137	0.01%	0.001%
47	6.945	1818	1821	1823	rBV	410	241	0.01%	0.001%
48	6.990	1823	1835	1857	rBV	282306	511929	23.18%	3.046%
49	7.318	1925	1937	1956	rBV	1001013	1713838	77.59%	10.199%
50	7.624	2022	2032	2062	rBV	195735	345862	15.66%	2.058%
51	7.942	2126	2131	2138	rBV5	1653	2271	0.10%	0.014%
52	8.039	2158	2161	2165	rBV3	570	428	0.02%	0.003%
53	8.090	2167	2177	2212	rBV	562762	1040093	47.09%	6.189%
54	8.505	2303	2306	2308	rBV2	554	294	0.01%	0.002%
55	8.649	2349	2351	2355	rVB2	538	347	0.02%	0.002%
56	8.691	2361	2364	2368	rBV3	594	484	0.02%	0.003%
57	8.765	2385	2387	2389	rBV2	324	100	0.00%	0.001%
58	8.785	2389	2393	2397	rBV3	523	437	0.02%	0.003%
59	8.855	2403	2415	2441	rBV	1018847	1673314	75.76%	9.957%
60	9.061	2477	2479	2481	rBV2	756	522	0.02%	0.003%
61	9.273	2544	2545	2547	rBV2	336	102	0.00%	0.001%
62	9.366	2572	2574	2578	rBV4	422	294	0.01%	0.002%
63	9.399	2582	2584	2588	rVB2	386	259	0.01%	0.002%
64	9.418	2588	2590	2591	rBV2	476	152	0.01%	0.001%
65	9.502	2613	2616	2619	rBV3	580	319	0.01%	0.002%
66	9.553	2628	2632	2635	rBV3	899	679	0.03%	0.004%
67	9.604	2646	2648	2651	rVB3	578	290	0.01%	0.002%
68	9.727	2683	2686	2690	rBV4	605	524	0.02%	0.003%
69	9.765	2695	2698	2701	rVB3	361	256	0.01%	0.002%
70	10.016	2773	2776	2777	rBV	378	249	0.01%	0.001%
71	10.026	2777	2779	2784	rVB3	559	446	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019705.D
 Acq On : 18 Dec 2020 17:20
 Operator : SY/MD
 Sample : L5098-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.087	2796	2798	2800	rVB2	783	294	0.01%	0.002%
73	10.112	2800	2806	2809	rBV2	367	403	0.02%	0.002%
74	10.148	2814	2817	2820	rBV2	529	331	0.01%	0.002%
75	10.222	2827	2840	2859	rBV	595000	931779	42.19%	5.545%
76	10.354	2879	2881	2883	rVB	610	254	0.01%	0.002%
77	10.553	2941	2943	2946	rBV2	475	221	0.01%	0.001%
78	10.617	2961	2963	2968	rVB2	623	479	0.02%	0.003%
79	10.656	2972	2975	2977	rVV2	712	446	0.02%	0.003%
80	10.682	2981	2983	2985	rVB2	407	136	0.01%	0.001%
81	10.781	3011	3014	3015	rBV2	417	251	0.01%	0.001%
82	10.868	3035	3041	3043	rBV4	795	856	0.04%	0.005%
83	11.042	3089	3095	3096	rBV3	602	607	0.03%	0.004%
84	11.170	3130	3135	3139	rBV6	1104	1103	0.05%	0.007%
85	11.254	3149	3161	3179	rBV	1046690	1598853	72.39%	9.514%
86	11.537	3244	3249	3251	rBV3	842	726	0.03%	0.004%
87	11.630	3266	3278	3299	rBV	1010377	1561391	70.69%	9.291%
88	11.990	3387	3390	3397	rBV3	896	873	0.04%	0.005%
89	12.309	3486	3489	3491	rBV2	588	344	0.02%	0.002%
90	12.357	3498	3504	3514	rVB10	2529	3721	0.17%	0.022%
91	12.511	3548	3552	3554	rBV2	685	558	0.03%	0.003%
92	12.630	3587	3589	3592	rBV	395	258	0.01%	0.002%
93	12.952	3687	3689	3691	rBV	639	266	0.01%	0.002%
94	13.045	3716	3718	3721	rBV3	488	361	0.02%	0.002%
95	13.280	3787	3791	3793	rBV3	875	705	0.03%	0.004%


Sum of corrected areas: 16804682

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121820\
Data File : VV019705.D
Acq On : 18 Dec 2020 17:20
Operator : SY/MD
Sample : L5098-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG4P1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

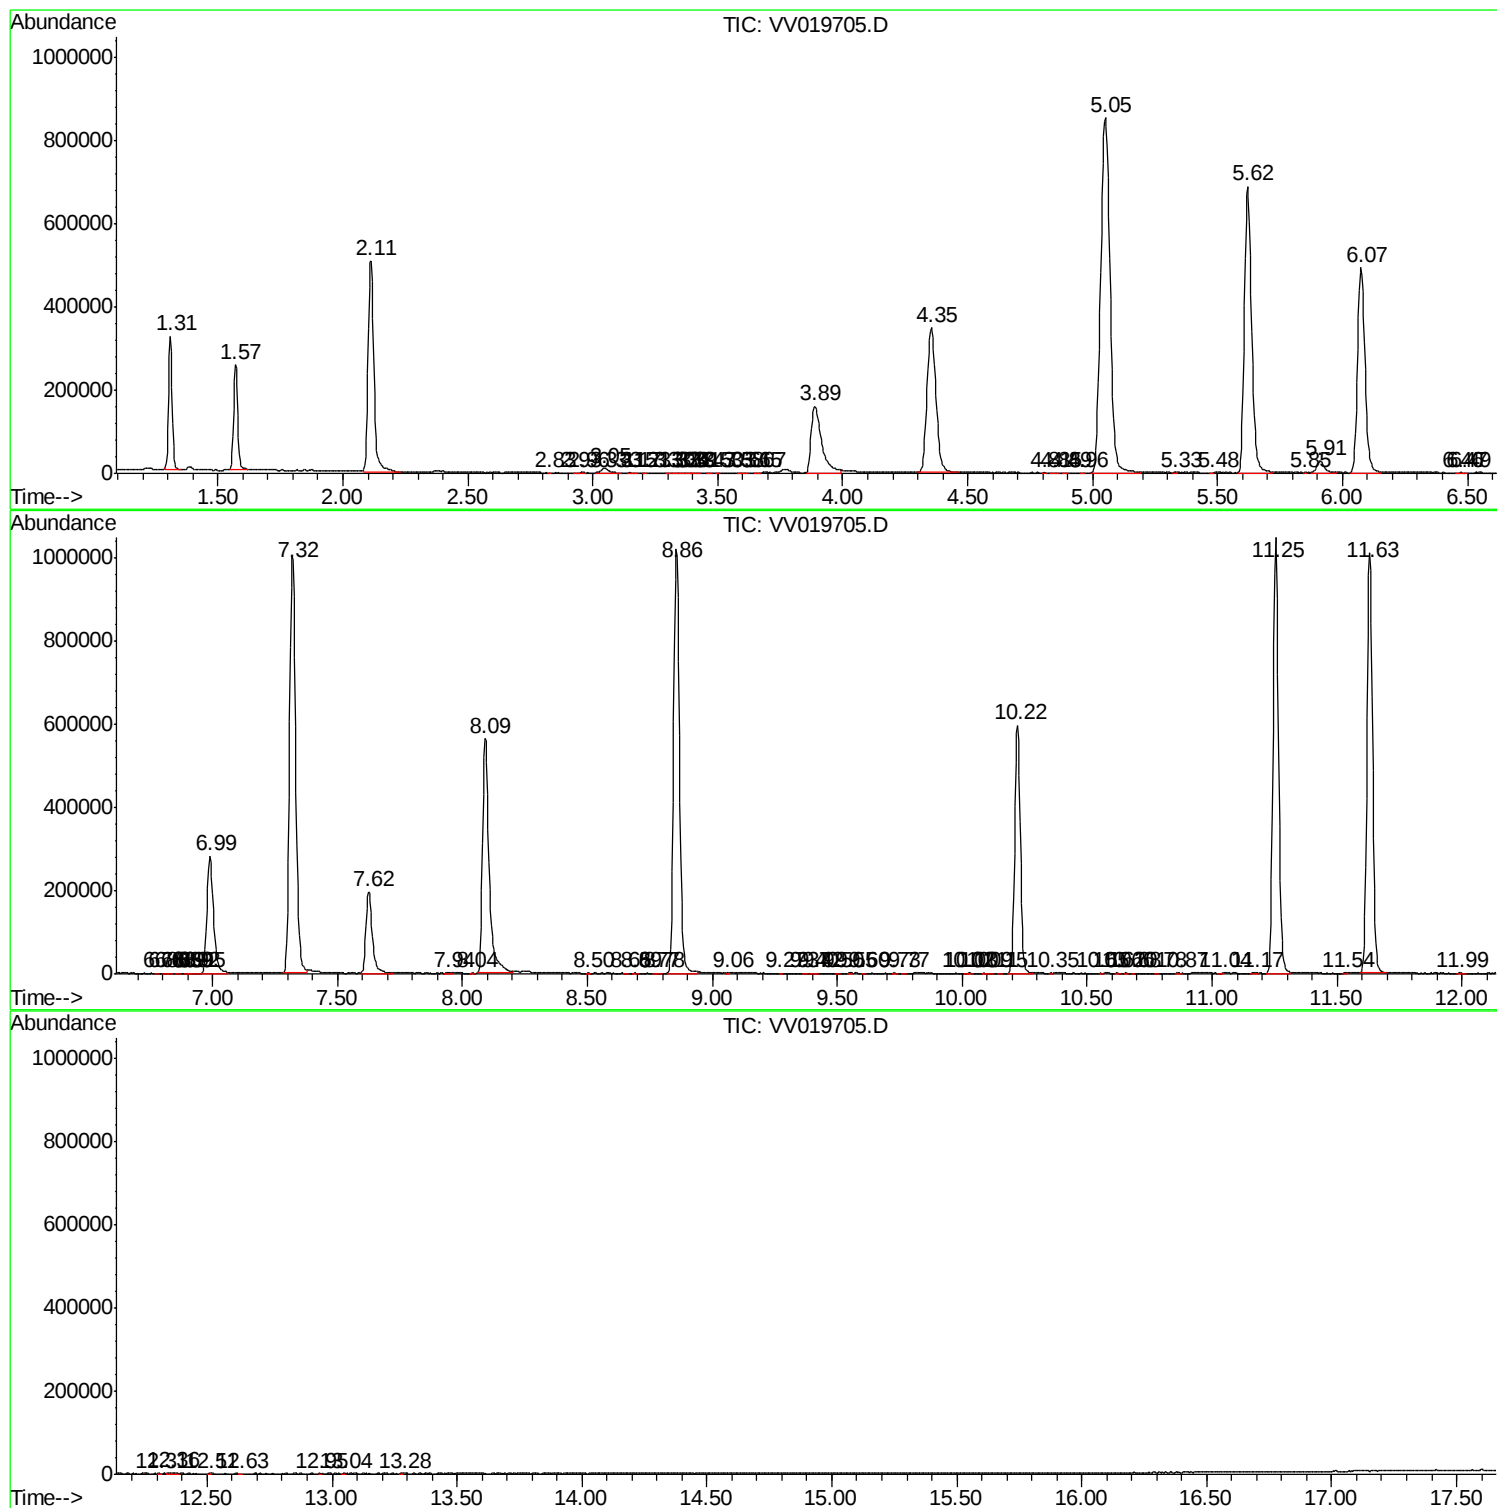

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019705.D
Acq On : 18 Dec 2020 17:20
Operator : SY/MD
Sample : L5098-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019705.D
Acq On : 18 Dec 2020 17:20
Operator : SY/MD
Sample : L5098-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc