

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019709.D
 Acq On : 18 Dec 2020 18:56
 Operator : SY/MD
 Sample : L5101-05DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FX1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	85	rVB	287537	290136	11.30%	1.509%
2	1.569	142	149	165	rVB	243104	277679	10.82%	1.444%
3	2.110	308	317	357	rVB	489274	765312	29.81%	3.980%
4	3.090	620	622	623	rBV	241	79	0.00%	0.000%
5	3.145	636	639	641	rBV3	609	341	0.01%	0.002%
6	3.261	673	675	679	rVB2	302	154	0.01%	0.001%
7	3.290	681	684	686	rBV3	466	366	0.01%	0.002%
8	3.412	720	722	727	rBV4	550	549	0.02%	0.003%
9	3.434	727	729	731	rVV	274	101	0.00%	0.001%
10	3.447	731	733	737	rBV2	419	319	0.01%	0.002%
11	3.589	774	777	779	rBV3	574	346	0.01%	0.002%
12	3.637	790	792	793	rBV	402	178	0.01%	0.001%
13	3.691	803	809	810	rBV3	321	325	0.01%	0.002%
14	3.765	828	832	837	rBV4	676	733	0.03%	0.004%
15	3.820	847	849	853	rBV2	322	220	0.01%	0.001%
16	3.897	861	873	919	rBV	156135	540471	21.05%	2.810%
17	4.354	999	1015	1047	rBV	344316	850801	33.14%	4.424%
18	4.772	1143	1145	1146	rBV	327	164	0.01%	0.001%
19	4.814	1151	1158	1161	rBV4	825	876	0.03%	0.005%
20	4.875	1175	1177	1179	rBV3	386	165	0.01%	0.001%
21	4.968	1199	1206	1207	rBV3	593	604	0.02%	0.003%
22	4.978	1207	1209	1211	rBV	333	191	0.01%	0.001%
23	5.052	1214	1232	1245	rBV2	848404	2187229	85.20%	11.373%
24	5.376	1331	1333	1334	rBV	583	242	0.01%	0.001%
25	5.621	1394	1409	1437	rBV	718928	1448788	56.44%	7.534%
26	5.913	1487	1500	1524	rVB3	16796	38522	1.50%	0.200%
27	6.000	1524	1527	1530	rBV3	843	668	0.03%	0.003%
28	6.074	1535	1550	1577	rBV	490814	996295	38.81%	5.181%
29	6.408	1650	1654	1655	rBV5	664	442	0.02%	0.002%
30	6.553	1693	1699	1701	rBV3	459	370	0.01%	0.002%
31	6.598	1706	1713	1717	rBV6	643	749	0.03%	0.004%
32	6.624	1717	1721	1723	rBV3	734	489	0.02%	0.003%
33	6.704	1744	1746	1747	rBV3	294	120	0.00%	0.001%
34	6.769	1763	1766	1768	rBV3	414	322	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019709.D
 Acq On : 18 Dec 2020 18:56
 Operator : SY/MD
 Sample : L5101-05DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FX1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.807	1774	1778	1779	rBV	753	404	0.02%	0.002%
36	6.849	1789	1791	1794	rBV	282	159	0.01%	0.001%
37	6.865	1794	1796	1801	rVB3	534	404	0.02%	0.002%
38	6.887	1801	1803	1804	rBV	246	101	0.00%	0.001%
39	6.897	1804	1806	1807	rBV	210	81	0.00%	0.000%
40	6.945	1819	1821	1822	rBV	510	221	0.01%	0.001%
41	6.990	1823	1835	1856	rBV	284955	507621	19.77%	2.640%
42	7.251	1914	1916	1919	rBV2	692	318	0.01%	0.002%
43	7.318	1925	1937	1958	rBV	973472	1681856	65.51%	8.746%
44	7.624	2020	2032	2059	rBV	195208	346182	13.49%	1.800%
45	7.907	2116	2120	2123	rBV4	874	871	0.03%	0.005%
46	7.981	2135	2143	2155	rVB7	5589	8991	0.35%	0.047%
47	8.051	2163	2165	2167	rBV2	388	183	0.01%	0.001%
48	8.093	2167	2178	2222	rBV	620378	1134009	44.17%	5.897%
49	8.801	2395	2398	2399	rBV4	513	296	0.01%	0.002%
50	8.858	2403	2416	2420	rBV	1120814	1790619	69.75%	9.311%
51	9.106	2486	2493	2497	rBV7	741	864	0.03%	0.004%
52	9.415	2586	2589	2591	rBV2	518	306	0.01%	0.002%
53	9.582	2638	2641	2643	rBV	418	229	0.01%	0.001%
54	9.630	2654	2656	2659	rVB2	616	241	0.01%	0.001%
55	9.759	2695	2696	2698	rBV	330	140	0.01%	0.001%
56	9.823	2713	2716	2717	rBV	502	262	0.01%	0.001%
57	9.855	2724	2726	2728	rBV2	462	249	0.01%	0.001%
58	9.878	2731	2733	2739	rVB4	694	327	0.01%	0.002%
59	9.987	2763	2767	2769	rBV2	388	325	0.01%	0.002%
60	10.026	2777	2779	2780	rBV2	368	142	0.01%	0.001%
61	10.074	2792	2794	2796	rBV	389	190	0.01%	0.001%
62	10.222	2826	2840	2860	rBV	634171	993847	38.71%	5.168%
63	10.723	2994	2996	2997	rBV	430	186	0.01%	0.001%
64	10.855	3034	3037	3038	rBV	673	332	0.01%	0.002%
65	11.048	3096	3097	3098	rBV	236	77	0.00%	0.000%
66	11.064	3098	3102	3104	rVV2	555	418	0.02%	0.002%
67	11.190	3131	3141	3150	rBV	66178	103778	4.04%	0.540%
68	11.257	3151	3162	3190	rVB2	1159049	2453111	95.56%	12.756%
69	11.492	3232	3235	3237	rBV3	652	421	0.02%	0.002%
70	11.633	3266	3279	3307	rBV2	1149014	2567139	100.00%	13.349%
71	11.865	3349	3351	3352	rBV	502	204	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
Data File : VV019709.D
Acq On : 18 Dec 2020 18:56
Operator : SY/MD
Sample : L5101-05DL 400X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FX1DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Title : VOC Analysis

72	12.524	3551	3556	3559	rBV7	555	599	0.02%	0.003%
73	12.588	3574	3576	3577	rBV7	600	176	0.01%	0.001%
74	12.659	3596	3598	3604	rVB5	1177	826	0.03%	0.004%
75	12.768	3626	3632	3633	rBV2	622	587	0.02%	0.003%
76	12.865	3660	3662	3665	rBV	401	159	0.01%	0.001%
77	13.270	3778	3788	3803	rBV2	114211	180152	7.02%	0.937%
78	13.514	3860	3864	3872	rBV4	806	1017	0.04%	0.005%
79	13.752	3929	3938	3952	rVB2	29677	48115	1.87%	0.250%


Sum of corrected areas: 19231081

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121820\
Data File : VV019709.D
Acq On : 18 Dec 2020 18:56
Operator : SY/MD
Sample : L5101-05DL 400X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FX1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

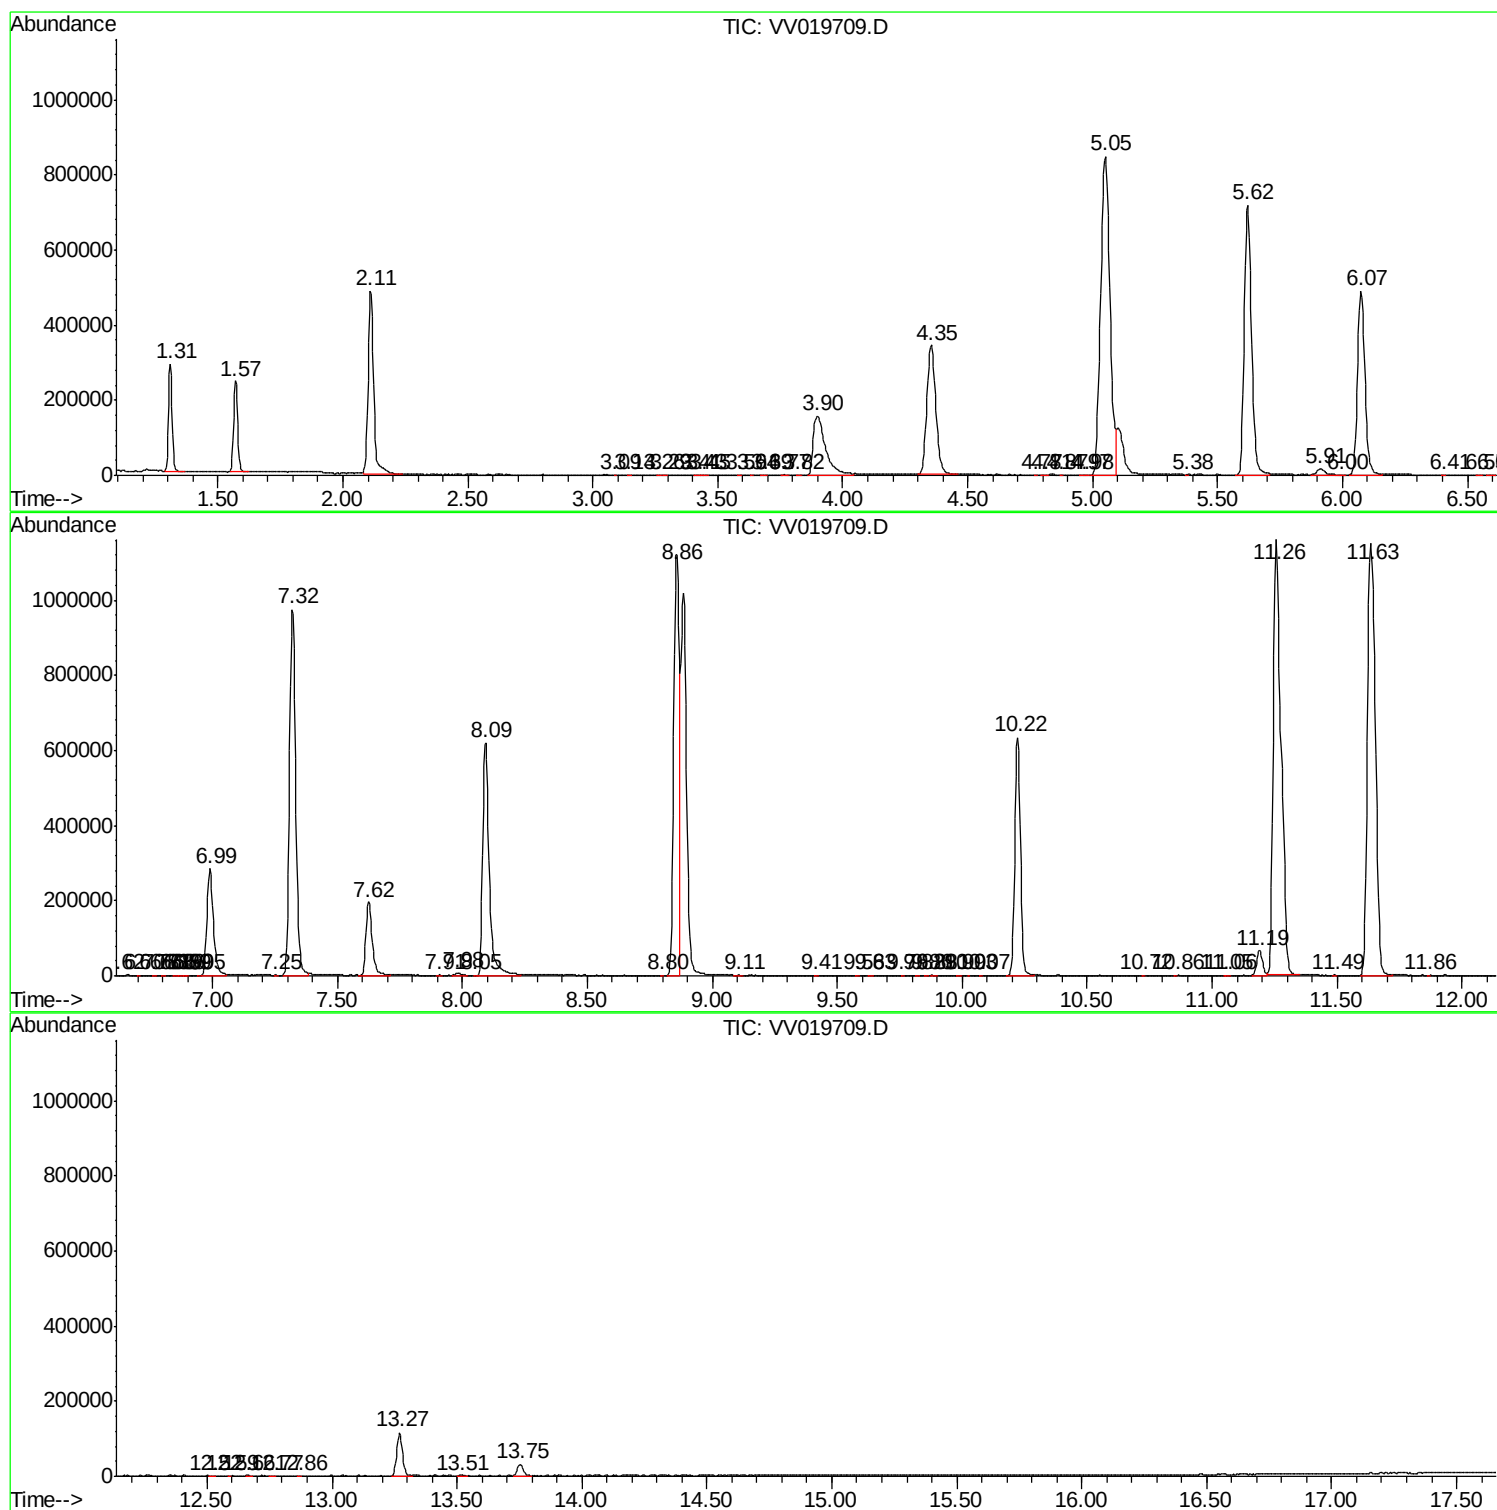

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019709.D
Acq On : 18 Dec 2020 18:56
Operator : SY/MD
Sample : L5101-05DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FX1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121820\
Data File : VV019709.D
Acq On : 18 Dec 2020 18:56
Operator : SY/MD
Sample : L5101-05DL 400X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0FX1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc