

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019716.D
 Acq On : 19 Dec 2020 00:06
 Operator : SY/MD
 Sample : L5131-05 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	265990	269648	12.64%	1.633%
2	1.570	142	149	163	rVB	231387	263683	12.36%	1.597%
3	2.110	308	317	355	rVB	456075	720338	33.76%	4.362%
4	2.750	514	516	517	rBV	703	276	0.01%	0.002%
5	2.843	543	545	548	rBV3	633	370	0.02%	0.002%
6	2.946	575	577	580	rVB2	368	174	0.01%	0.001%
7	2.991	587	591	594	rBV	499	423	0.02%	0.003%
8	3.193	652	654	660	rVB3	578	405	0.02%	0.002%
9	3.290	680	684	687	rBV2	637	563	0.03%	0.003%
10	3.402	717	719	720	rBV	162	66	0.00%	0.000%
11	3.418	720	724	727	rBV	335	196	0.01%	0.001%
12	3.438	727	730	731	rBV2	319	165	0.01%	0.001%
13	3.547	762	764	769	rVB	369	237	0.01%	0.001%
14	3.569	769	771	772	rBV	307	143	0.01%	0.001%
15	3.721	816	818	819	rBV2	376	108	0.01%	0.001%
16	3.737	821	823	826	rVB2	643	386	0.02%	0.002%
17	3.750	826	827	829	rBV2	233	116	0.01%	0.001%
18	3.769	829	833	837	rBV5	591	601	0.03%	0.004%
19	3.894	860	872	913	rBV	171844	549867	25.77%	3.330%
20	4.354	1000	1015	1044	rVB2	342373	834343	39.10%	5.053%
21	4.759	1138	1141	1147	rBV4	603	615	0.03%	0.004%
22	4.811	1155	1157	1161	rBV3	549	507	0.02%	0.003%
23	4.926	1189	1193	1197	rVB4	790	613	0.03%	0.004%
24	4.949	1197	1200	1204	rBV4	652	668	0.03%	0.004%
25	5.052	1214	1232	1267	rBV2	826316	2133986	100.00%	12.923%
26	5.380	1332	1334	1336	rBV2	454	303	0.01%	0.002%
27	5.476	1359	1364	1365	rBV3	716	531	0.02%	0.003%
28	5.621	1396	1409	1435	rBV	682533	1364267	63.93%	8.262%
29	5.862	1482	1484	1489	rVB3	678	405	0.02%	0.002%
30	5.910	1489	1499	1514	rBV2	17679	38267	1.79%	0.232%
31	6.074	1537	1550	1579	rBV	480732	976465	45.76%	5.914%
32	6.351	1635	1636	1638	rBV2	465	244	0.01%	0.001%
33	6.447	1664	1666	1668	rBV2	639	297	0.01%	0.002%
34	6.476	1671	1675	1677	rBV2	523	342	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019716.D
 Acq On : 19 Dec 2020 00:06
 Operator : SY/MD
 Sample : L5131-05 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.495	1677	1681	1683	rBV3	510	424	0.02%	0.003%
36	6.537	1692	1694	1695	rBV	355	144	0.01%	0.001%
37	6.585	1706	1709	1710	rVB3	383	176	0.01%	0.001%
38	6.605	1712	1715	1720	rBV4	803	566	0.03%	0.003%
39	6.624	1720	1721	1722	rBV4	329	98	0.00%	0.001%
40	6.733	1752	1755	1756	rBV2	364	204	0.01%	0.001%
41	6.865	1794	1796	1797	rBV	260	119	0.01%	0.001%
42	6.991	1823	1835	1860	rBV	270447	492852	23.10%	2.985%
43	7.319	1925	1937	1959	rBV	921777	1613152	75.59%	9.769%
44	7.624	2022	2032	2065	rBV	191429	337815	15.83%	2.046%
45	7.939	2126	2130	2131	rBV3	708	515	0.02%	0.003%
46	7.978	2139	2142	2144	rBV3	1667	1422	0.07%	0.009%
47	8.052	2162	2165	2167	rBV3	396	346	0.02%	0.002%
48	8.090	2167	2177	2214	rBV	623692	1149376	53.86%	6.961%
49	8.759	2380	2385	2386	rBV3	659	560	0.03%	0.003%
50	8.855	2403	2415	2444	rBV	1028572	1662401	77.90%	10.068%
51	9.270	2541	2544	2547	rBV2	740	511	0.02%	0.003%
52	9.322	2557	2560	2562	rBV3	614	264	0.01%	0.002%
53	9.383	2577	2579	2581	rVB3	599	252	0.01%	0.002%
54	9.479	2607	2609	2613	rVB3	446	279	0.01%	0.002%
55	9.502	2613	2616	2617	rBV3	404	224	0.01%	0.001%
56	9.585	2639	2642	2645	rBV3	581	366	0.02%	0.002%
57	9.605	2645	2648	2652	rVB2	828	522	0.02%	0.003%
58	9.688	2672	2674	2676	rBV	253	133	0.01%	0.001%
59	9.736	2684	2689	2692	rBV3	481	575	0.03%	0.003%
60	9.871	2729	2731	2732	rBV	610	266	0.01%	0.002%
61	9.945	2752	2754	2756	rBV3	517	244	0.01%	0.001%
62	9.987	2764	2767	2769	rBV2	616	378	0.02%	0.002%
63	10.032	2776	2781	2786	rBV4	620	761	0.04%	0.005%
64	10.103	2798	2803	2805	rBV2	538	409	0.02%	0.002%
65	10.222	2827	2840	2861	rBV	633273	1000034	46.86%	6.056%
66	10.386	2887	2891	2893	rBV2	826	506	0.02%	0.003%
67	10.582	2949	2952	2953	rBV2	739	348	0.02%	0.002%
68	10.624	2961	2965	2967	rBV	688	462	0.02%	0.003%
69	10.785	3011	3015	3018	rBV4	851	661	0.03%	0.004%
70	10.801	3018	3020	3023	rVB	577	346	0.02%	0.002%
71	10.871	3041	3042	3043	rBV	299	62	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019716.D
 Acq On : 19 Dec 2020 00:06
 Operator : SY/MD
 Sample : L5131-05 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.958	3067	3069	3075	rBV4	518	551	0.03%	0.003%
73	10.984	3075	3077	3079	rVV	390	165	0.01%	0.001%
74	11.016	3084	3087	3093	rVB4	758	813	0.04%	0.005%
75	11.045	3093	3096	3102	rBV2	790	740	0.03%	0.004%
76	11.087	3106	3109	3110	rBV	394	247	0.01%	0.001%
77	11.254	3149	3161	3182	rBV	1032062	1581724	74.12%	9.579%
78	11.630	3266	3278	3299	rBV	957630	1499034	70.25%	9.078%
79	12.238	3464	3467	3469	rBV2	778	445	0.02%	0.003%
80	12.277	3477	3479	3484	rVB3	652	401	0.02%	0.002%
81	12.350	3499	3502	3505	rVB2	504	327	0.02%	0.002%
82	12.431	3524	3527	3531	rBV	565	325	0.02%	0.002%
83	13.231	3774	3776	3778	rBV2	466	287	0.01%	0.002%


Sum of corrected areas: 16512450

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121820\
Data File : VV019716.D
Acq On : 19 Dec 2020 00:06
Operator : SY/MD
Sample : L5131-05 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H04

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

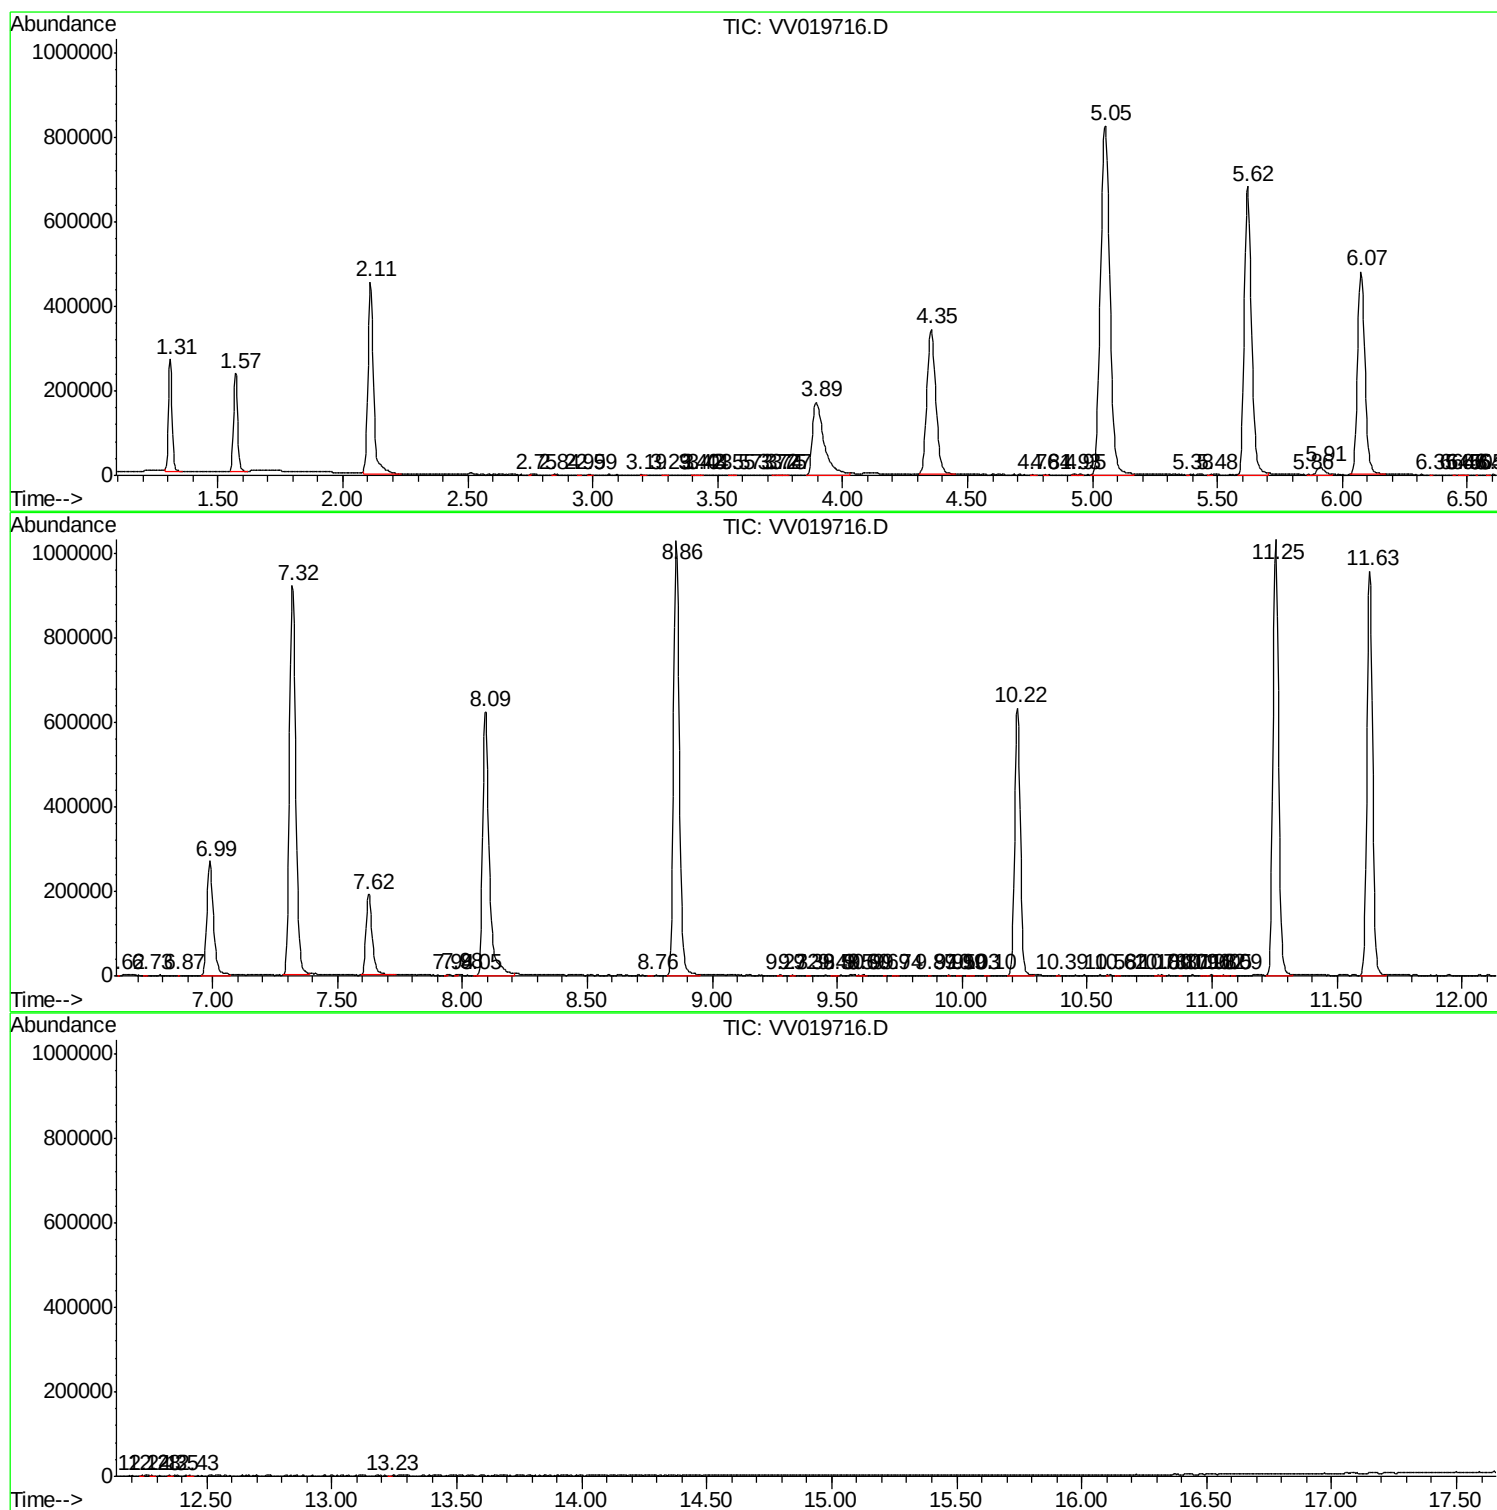

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019716.D
Acq On : 19 Dec 2020 00:06
Operator : SY/MD
Sample : L5131-05 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H04

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019716.D
Acq On : 19 Dec 2020 00:06
Operator : SY/MD
Sample : L5131-05 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H04

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc