

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019717.D
 Acq On : 19 Dec 2020 00:30
 Operator : SY/MD
 Sample : L5131-06 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	78	rVB	265954	266158	12.48%	1.641%
2	1.569	143	149	161	rVB	235134	260875	12.23%	1.609%
3	2.110	308	317	345	rVB	454928	699590	32.80%	4.315%
4	2.933	570	573	576	rBV2	508	424	0.02%	0.003%
5	3.016	597	599	602	rBV2	586	369	0.02%	0.002%
6	3.032	602	604	605	rBV2	413	168	0.01%	0.001%
7	3.158	641	643	645	rBV3	594	259	0.01%	0.002%
8	3.177	647	649	654	rVB3	780	570	0.03%	0.004%
9	3.209	654	659	664	rBV5	851	847	0.04%	0.005%
10	3.232	664	666	667	rBV5	295	145	0.01%	0.001%
11	3.270	676	678	681	rBV3	390	263	0.01%	0.002%
12	3.412	717	722	727	rVB2	657	585	0.03%	0.004%
13	3.434	727	729	731	rBV2	627	302	0.01%	0.002%
14	3.499	745	749	751	rBV2	454	335	0.02%	0.002%
15	3.627	785	789	791	rBV2	188	125	0.01%	0.001%
16	3.637	791	792	795	rVB	303	136	0.01%	0.001%
17	3.653	795	797	799	rBV3	302	138	0.01%	0.001%
18	3.672	799	803	804	rBV2	129	96	0.00%	0.001%
19	3.682	804	806	809	rBV3	387	195	0.01%	0.001%
20	3.775	833	835	836	rBV	420	147	0.01%	0.001%
21	3.801	841	843	847	rBV2	414	271	0.01%	0.002%
22	3.827	847	851	854	rVB3	291	201	0.01%	0.001%
23	3.894	859	872	903	rBV	164961	507459	23.79%	3.130%
24	4.354	998	1015	1038	rBV	343071	843439	39.55%	5.202%
25	4.592	1087	1089	1093	rBV3	511	369	0.02%	0.002%
26	4.717	1125	1128	1131	rBV2	415	281	0.01%	0.002%
27	4.884	1177	1180	1183	rBV4	472	441	0.02%	0.003%
28	4.926	1190	1193	1197	rBV2	548	463	0.02%	0.003%
29	5.052	1214	1232	1263	rBV2	823482	2132791	100.00%	13.154%
30	5.447	1353	1355	1358	rVB2	721	310	0.01%	0.002%
31	5.463	1358	1360	1362	rBV3	640	271	0.01%	0.002%
32	5.621	1394	1409	1437	rBV	663240	1333294	62.51%	8.223%
33	5.913	1490	1500	1517	rVB3	17460	35857	1.68%	0.221%
34	6.074	1535	1550	1576	rBV	483597	986215	46.24%	6.082%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019717.D
 Acq On : 19 Dec 2020 00:30
 Operator : SY/MD
 Sample : L5131-06 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.351	1634	1636	1639	rBV2	405	233	0.01%	0.001%
36	6.405	1650	1653	1661	rVB	15829	9594	0.45%	0.059%
37	6.470	1670	1673	1674	rBV2	517	247	0.01%	0.002%
38	6.563	1699	1702	1703	rBV3	252	154	0.01%	0.001%
39	6.640	1718	1726	1731	rBV7	1089	1414	0.07%	0.009%
40	6.865	1790	1796	1798	rBV4	530	544	0.03%	0.003%
41	6.907	1806	1809	1815	rBV5	497	491	0.02%	0.003%
42	6.939	1817	1819	1821	rBV2	236	93	0.00%	0.001%
43	6.990	1824	1835	1865	rVV	274548	493817	23.15%	3.046%
44	7.318	1924	1937	1966	rBV	939215	1624286	76.16%	10.017%
45	7.624	2022	2032	2057	rBV	189290	332092	15.57%	2.048%
46	7.936	2125	2129	2131	rBV3	720	567	0.03%	0.003%
47	8.006	2149	2151	2155	rVB3	429	184	0.01%	0.001%
48	8.093	2167	2178	2212	rBV	588752	1086866	50.96%	6.703%
49	8.505	2303	2306	2311	rBV4	626	506	0.02%	0.003%
50	8.855	2403	2415	2443	rBV	991318	1605913	75.30%	9.904%
51	9.100	2489	2491	2494	rBV3	774	497	0.02%	0.003%
52	9.302	2548	2554	2559	rBV4	1062	1294	0.06%	0.008%
53	9.322	2559	2560	2562	rVV2	370	139	0.01%	0.001%
54	9.376	2575	2577	2580	rBV2	509	287	0.01%	0.002%
55	9.469	2603	2606	2609	rVB	316	165	0.01%	0.001%
56	9.521	2620	2622	2623	rBV	251	133	0.01%	0.001%
57	9.559	2628	2634	2636	rBV5	619	679	0.03%	0.004%
58	9.646	2660	2661	2664	rBV	271	156	0.01%	0.001%
59	9.666	2665	2667	2668	rVB2	576	133	0.01%	0.001%
60	9.675	2668	2670	2672	rBV	425	175	0.01%	0.001%
61	9.739	2688	2690	2691	rBV	312	82	0.00%	0.001%
62	9.855	2722	2726	2730	rBV4	648	519	0.02%	0.003%
63	9.907	2739	2742	2745	rVB3	504	308	0.01%	0.002%
64	9.936	2748	2751	2752	rBV2	424	206	0.01%	0.001%
65	9.990	2765	2768	2770	rBV2	529	394	0.02%	0.002%
66	10.016	2774	2776	2780	rVB3	716	377	0.02%	0.002%
67	10.039	2780	2783	2785	rBV3	378	252	0.01%	0.002%
68	10.096	2800	2801	2803	rVB	491	128	0.01%	0.001%
69	10.112	2803	2806	2807	rBV	292	175	0.01%	0.001%
70	10.164	2820	2822	2826	rBV2	377	304	0.01%	0.002%
71	10.222	2828	2840	2857	rBV	623157	972858	45.61%	6.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121820\
 Data File : VV019717.D
 Acq On : 19 Dec 2020 00:30
 Operator : SY/MD
 Sample : L5131-06 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.524	2933	2934	2936	rBV3	269	116	0.01%	0.001%
73	10.556	2936	2944	2948	rVV2	852	999	0.05%	0.006%
74	10.646	2969	2972	2975	rBV2	351	229	0.01%	0.001%
75	10.666	2975	2978	2982	rVB2	542	391	0.02%	0.002%
76	10.685	2982	2984	2986	rBV2	334	161	0.01%	0.001%
77	10.723	2993	2996	3002	rVB2	680	548	0.03%	0.003%
78	10.756	3002	3006	3007	rBV2	584	372	0.02%	0.002%
79	10.855	3035	3037	3041	rVB3	724	387	0.02%	0.002%
80	10.881	3043	3045	3048	rBV	418	257	0.01%	0.002%
81	11.026	3087	3090	3094	rBV	464	353	0.02%	0.002%
82	11.100	3108	3113	3114	rBV2	360	265	0.01%	0.002%
83	11.129	3120	3122	3125	rBV	454	191	0.01%	0.001%
84	11.145	3125	3127	3130	rBV3	403	228	0.01%	0.001%
85	11.254	3149	3161	3179	rBV	980154	1496444	70.16%	9.229%
86	11.514	3238	3242	3244	rVB	458	283	0.01%	0.002%
87	11.527	3244	3246	3248	rBV2	601	319	0.01%	0.002%
88	11.630	3265	3278	3299	rBV	959373	1500685	70.36%	9.255%
89	11.974	3383	3385	3389	rBV2	570	344	0.02%	0.002%
90	12.071	3410	3415	3417	rBV2	614	541	0.03%	0.003%
91	12.450	3530	3533	3537	rBV3	706	525	0.02%	0.003%
92	12.473	3538	3540	3545	rBV2	485	369	0.02%	0.002%
93	12.813	3642	3646	3648	rBV2	854	641	0.03%	0.004%
94	13.157	3752	3753	3755	rBV	483	198	0.01%	0.001%


Sum of corrected areas: 16214497

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121820\
Data File : VV019717.D
Acq On : 19 Dec 2020 00:30
Operator : SY/MD
Sample : L5131-06 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

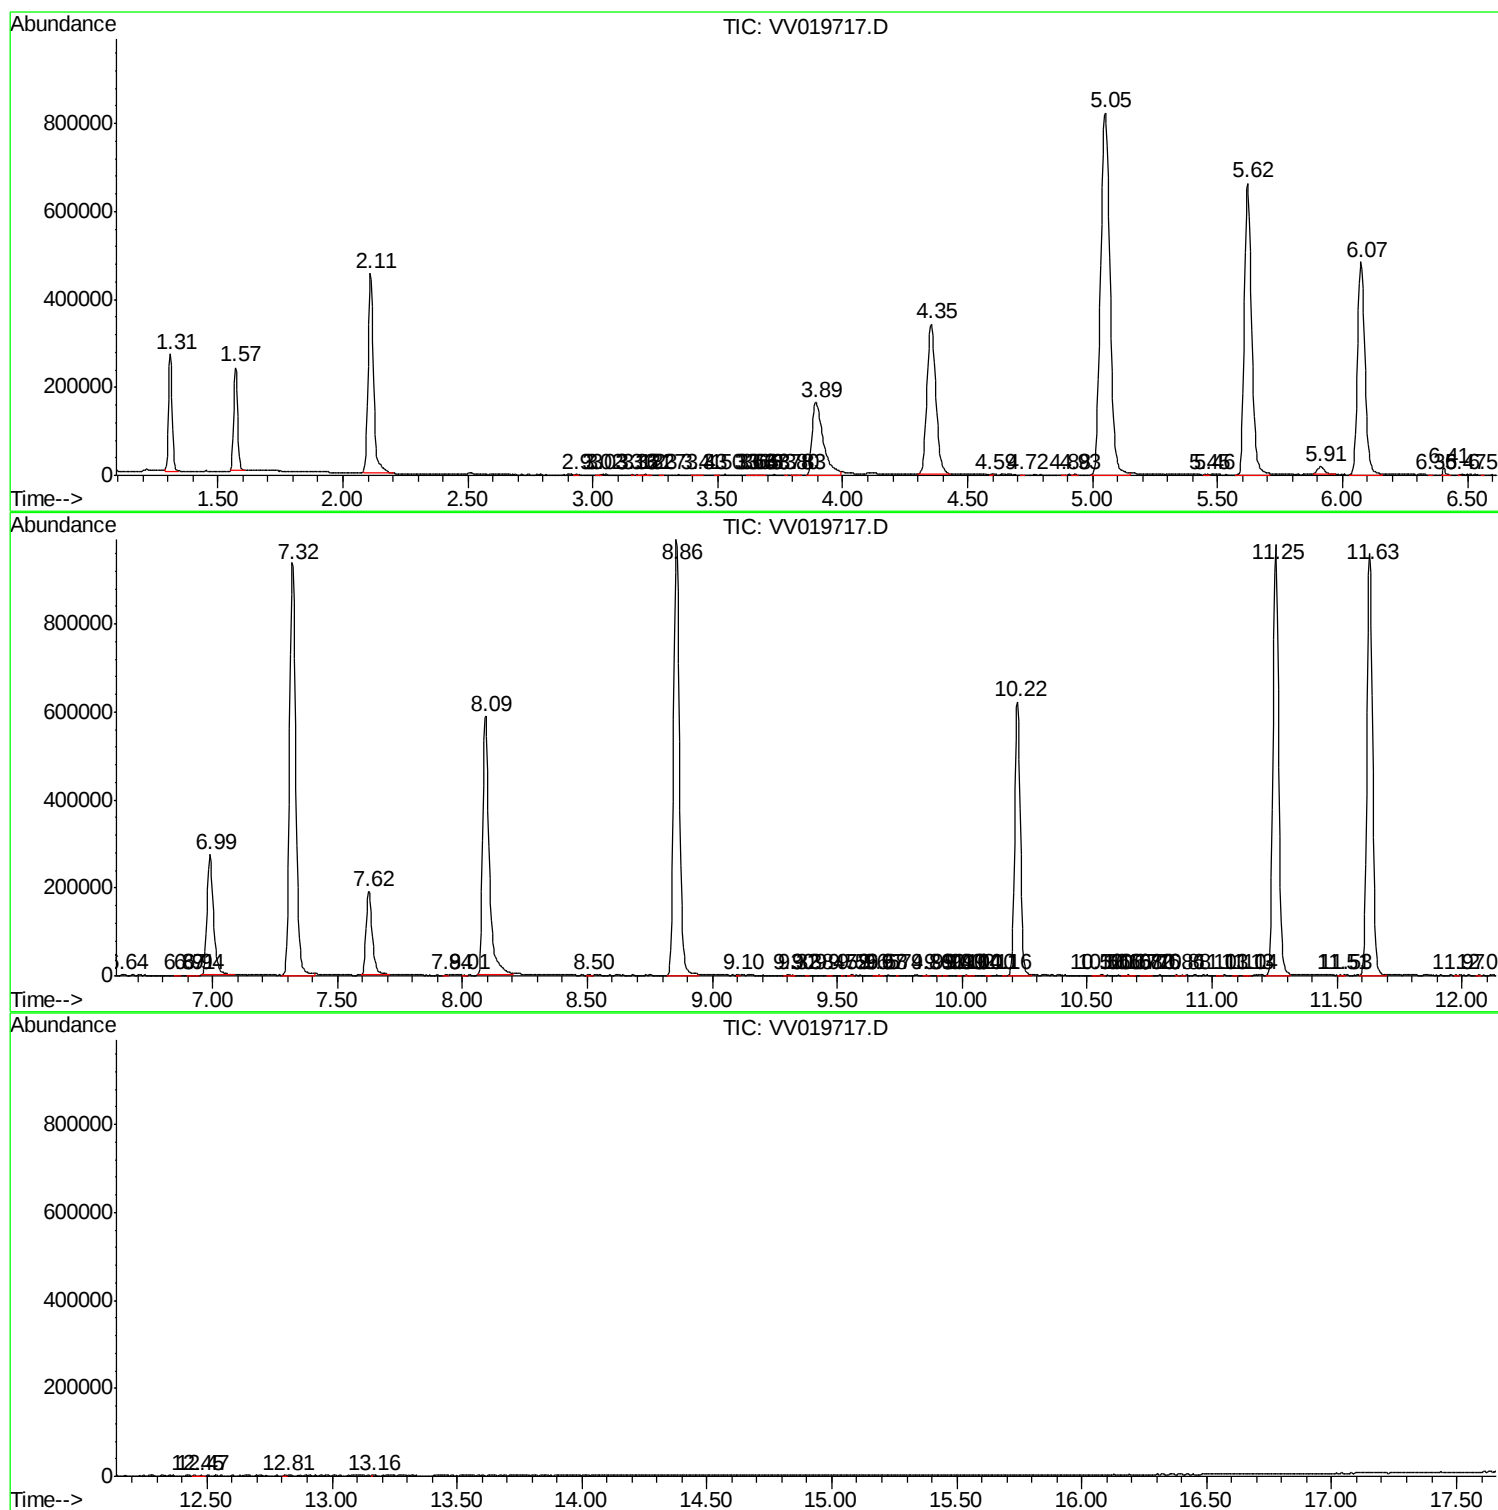

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019717.D
Acq On : 19 Dec 2020 00:30
Operator : SY/MD
Sample : L5131-06 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121820\
Data File : VV019717.D
Acq On : 19 Dec 2020 00:30
Operator : SY/MD
Sample : L5131-06 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H05

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
