


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121820\
 Data File : VV019688.D
 Acq On : 18 Dec 2020 08:44
 Operator : SY/MD
 Sample : BFB68
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB68

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 21 06:23:42 2020

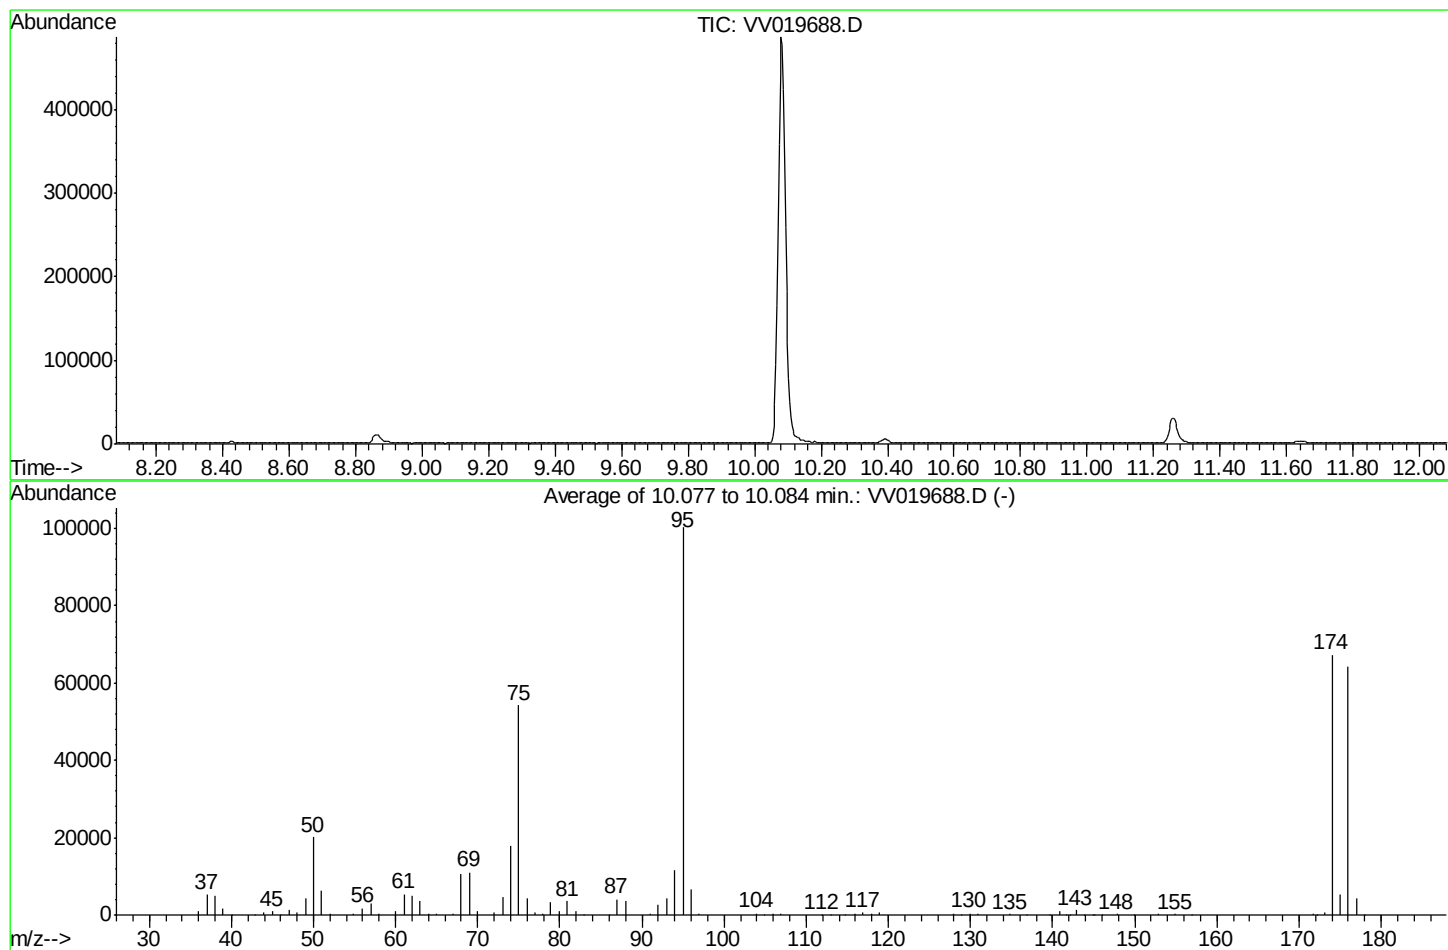

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	20130	PASS
75	95	30	80	54.0	54178	PASS
95	95	100	100	100.0	100309	PASS
96	95	5	9	6.7	6733	PASS
173	174	0.00	2	0.9	573	PASS
174	95	50	120	67.0	67248	PASS
175	174	5	9	7.7	5188	PASS
176	174	95	101	95.5	64208	PASS
177	176	5	9	6.9	4404	PASS

m/z	Abundance
36.00	1051.0
37.00	5214.0
38.00	4611.0
39.10	1750.0
40.00	308.0
40.80	153.0
42.90	129.0
44.00	1319.0
45.00	1035.0
46.00	107.0
47.00	1357.0
48.00	637.0
49.00	4133.0
50.00	19312.0
51.00	6253.0
52.00	324.0
54.90	394.0
56.00	1731.0
57.00	2825.0
57.90	236.0
60.00	905.0
61.00	5140.0
62.00	4907.0
63.00	3386.0
64.00	413.0
65.00	290.0
67.00	349.0
68.00	10240.0
69.00	10558.0
70.00	974.0
71.90	520.0
73.00	4114.0
74.00	17064.0
75.00	51456.0
76.00	4395.0
76.90	584.0
77.90	430.0
78.90	3030.0
79.90	942.0
80.90	3491.0
81.90	769.0
86.00	122.0
86.90	3835.0
88.00	3368.0
90.90	449.0
92.00	2777.0
93.00	3776.0
94.00	11023.0
95.00	94504.0
96.00	6469.0
96.90	284.0
103.90	394.0
104.90	173.0
105.90	319.0
106.90	197.0
111.90	112.0
112.90	130.0
114.80	149.0
115.90	371.0
116.90	578.0
117.90	399.0
118.90	524.0
127.90	303.0
128.80	146.0
129.90	451.0
130.90	239.0
134.90	248.0
136.80	137.0
139.70	117.0
140.80	873.0
141.70	116.0
142.90	1052.0
143.90	103.0
144.90	114.0
147.80	202.0
152.90	203.0
155.00	230.0
156.90	183.0
172.20	260.0
174.00	62360.0
175.00	4982.0
176.00	59696.0
177.00	3886.0
177.90	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
36.00	1019.0
37.00	5517.0
38.00	5059.0
39.00	1811.0
40.00	363.0
40.80	134.0
42.90	100.0
44.00	1427.0
45.00	1026.0
46.00	125.0
47.10	1397.0
48.00	697.0
49.00	4340.0
50.00	20720.0
51.00	6720.0
52.00	395.0
54.90	397.0
56.00	1906.0
57.00	3011.0
57.90	251.0
60.00	1031.0
61.00	5657.0
62.00	5293.0
63.00	3635.0
63.90	499.0
65.00	326.0
67.00	399.0
68.00	11032.0
69.00	11428.0
70.00	1037.0
71.90	556.0
73.00	4648.0
74.00	18640.0
75.00	56400.0
76.00	4680.0
76.90	661.0
77.90	439.0
78.90	3268.0
79.90	1029.0
80.90	3726.0
81.90	890.0
82.90	119.0
86.00	142.0
86.90	4098.0
88.00	3839.0
90.90	467.0
92.00	2870.0
93.00	4385.0
94.00	11861.0
95.00	103864.0
96.00	6973.0
96.90	292.0
104.00	441.0
104.90	175.0
105.90	429.0
106.90	212.0
111.90	102.0
112.90	120.0
114.70	150.0
115.90	402.0
116.90	664.0
117.90	448.0
118.90	568.0
128.00	270.0
128.90	179.0
129.90	453.0
130.90	231.0
134.80	272.0
136.80	167.0
139.70	122.0
140.80	949.0
142.00	131.0
142.90	1200.0
145.10	102.0
146.00	117.0
147.80	253.0
152.90	220.0
154.90	213.0
156.90	163.0
171.80	252.0
173.10	848.0
174.00	69704.0
175.00	5394.0
176.00	66592.0
177.00	4556.0
177.90	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
36.00	999.0
37.00	5093.0
38.00	5031.0
39.00	1694.0
40.00	347.0
40.90	111.0
44.00	1407.0
45.00	903.0
46.00	136.0
47.10	1453.0
48.00	654.0
49.00	4253.0
50.00	20360.0
51.00	6257.0
52.00	396.0
54.90	354.0
56.00	1771.0
57.00	2872.0
57.90	221.0
60.00	979.0
61.00	5314.0
62.00	4916.0
63.00	3499.0
63.90	523.0
65.00	327.0
67.00	409.0
68.00	10584.0
69.00	10884.0
70.00	928.0
71.90	524.0
73.00	4921.0
74.00	18256.0
75.00	54680.0
76.00	4314.0
77.00	648.0
77.80	436.0
78.90	3312.0
79.90	994.0
80.90	3647.0
81.90	891.0
82.90	131.0
86.00	145.0
86.90	4145.0
88.00	3881.0
91.00	437.0
92.00	2807.0
93.00	4526.0
94.00	11559.0
95.00	102560.0
96.10	6759.0
97.00	234.0
104.00	439.0
104.80	172.0
105.90	477.0
106.90	144.0
115.90	379.0
116.90	643.0
117.90	440.0
118.90	539.0
127.80	271.0
129.00	193.0
129.90	420.0
130.90	188.0
134.70	264.0
136.90	173.0
140.90	920.0
142.10	154.0
142.90	1277.0
145.90	129.0
147.90	282.0
149.90	103.0
152.90	154.0
154.90	194.0
156.80	141.0
171.80	280.0
173.10	872.0
174.00	69680.0
175.00	5188.0
176.00	66336.0
177.00	4770.0
178.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

Scan 2784 (10.042 min): VV019688.D
BFB68

m/z	Abundance
38.90	138.0
39.90	310.0
40.90	138.0
43.90	747.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68