

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033450.D
 Acq On : 18 Dec 2023 12:20
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 19 01:12:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	180819	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	197218	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	80383	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	53086	38.124	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.240%		
7) Chloroethane-d5	1.532	69	55734	44.601	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.200%		
11) 1,1-Dichloroethene-d2	2.060	65	28786	41.528	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.060%		
21) 2-Butanone-d5	3.786	46	93955	133.879	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	133.880%#		
24) Chloroform-d	4.249	84	141431	51.347	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.700%		
26) 1,2-Dichloroethane-d4	4.940	65	97198	57.443	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	114.880%		
32) Benzene-d6	4.960	84	245979	46.309	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.620%		
36) 1,2-Dichloropropane-d6	5.989	67	82682	51.288	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.580%		
41) Toluene-d8	7.246	98	206673	42.523	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.040%		
43) trans-1,3-Dichloroprop...	7.554	79	35676	45.155	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.320%		
47) 2-Hexanone-d5	8.024	63	61501	113.423	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	113.420%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	131734	56.855	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	113.720%		
66) 1,2-Dichlorobenzene-d4	11.564	152	89339	59.144	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	118.280%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.554	75	2160	1.038	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033450.D
Acq On : 18 Dec 2023 12:20
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 19 01:12:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 20:24:09 2023
Response via : Initial Calibration

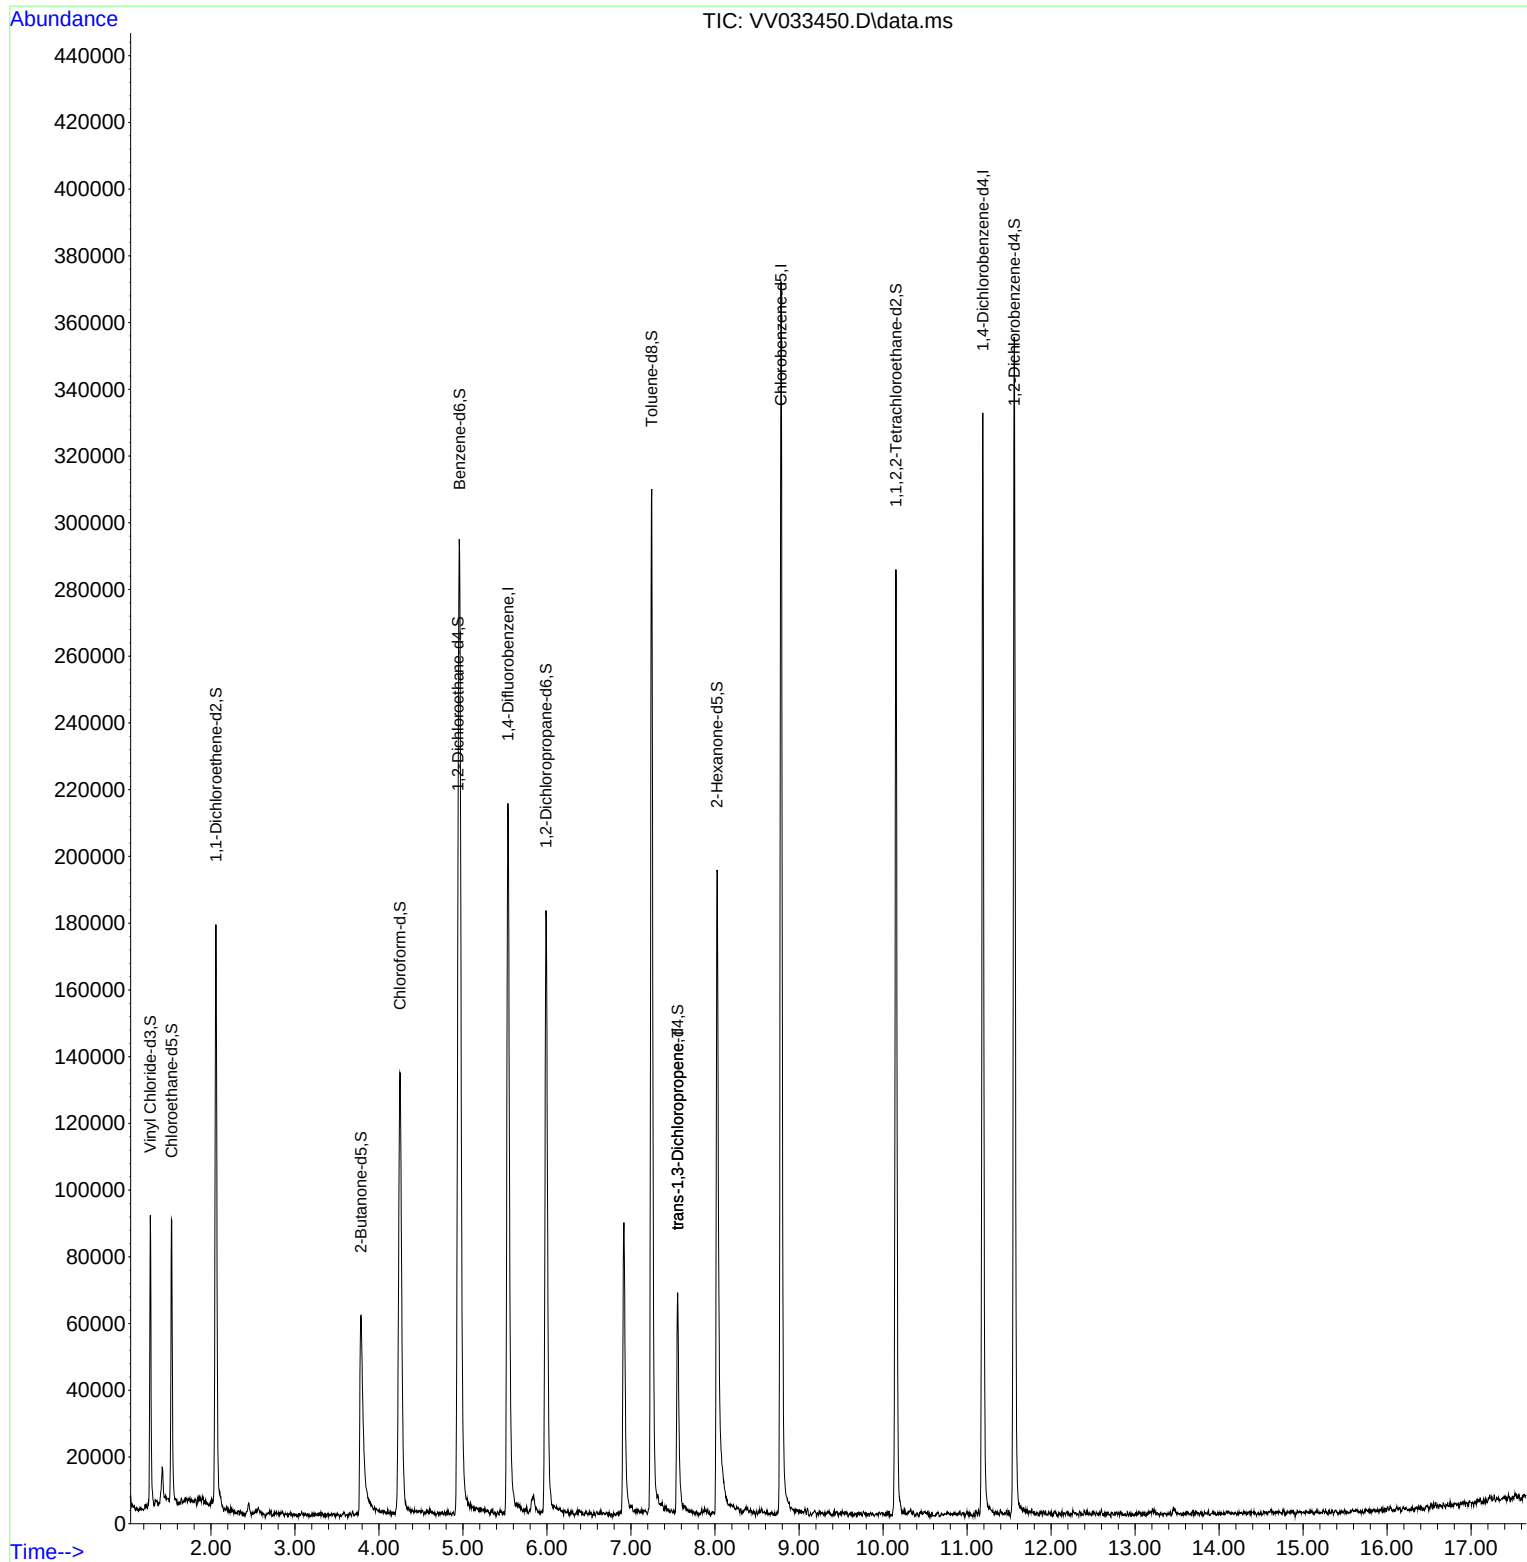

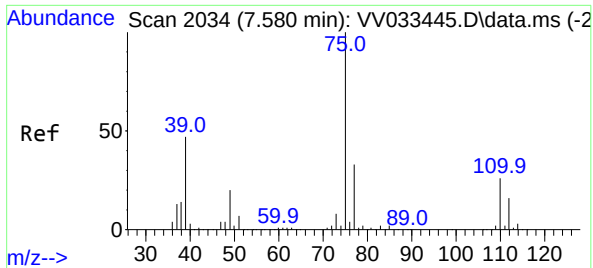

#44
trans-1,3-Dichloropropene
Concen: 1.038 ug/L
RT: 7.554 min Scan# 20
Delta R.T. -0.026 min
Lab File: VV033450.D
Acq: 18 Dec 2023 12:20

Instrument :
MSVOA_V
ClientSampleId :

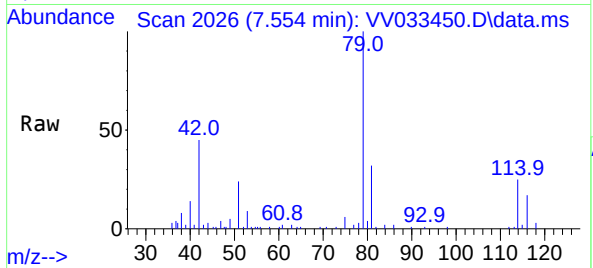

Tgt Ion: 75 Resp: 2160
Ion Ratio Lower Upper
75 100
77 37.3 22.4 41.6

