

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033453.D
 Acq On : 18 Dec 2023 13:30
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 19 01:13:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	201594	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	211140	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	88356	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	59308	38.203	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.400%		
7) Chloroethane-d5	1.529	69	60256	43.250	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.500%		
11) 1,1-Dichloroethene-d2	2.059	65	31207	40.381	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.760%		
21) 2-Butanone-d5	3.783	46	89611	114.530	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	114.530%		
24) Chloroform-d	4.249	84	142678	46.461	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.920%		
26) 1,2-Dichloroethane-d4	4.944	65	96409	51.105	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.220%		
32) Benzene-d6	4.963	84	254215	44.704	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.400%		
36) 1,2-Dichloropropane-d6	5.989	67	84200	48.786	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.580%		
41) Toluene-d8	7.246	98	213602	41.050	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.100%		
43) trans-1,3-Dichloroprop...	7.554	79	36625	43.300	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.600%		
47) 2-Hexanone-d5	8.024	63	57868	99.686	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.690%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	126663	51.062	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	102.120%		
66) 1,2-Dichlorobenzene-d4	11.564	152	88478	53.289	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.580%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.548	75	2031	0.912	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033453.D
Acq On : 18 Dec 2023 13:30
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 19 01:13:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 20:24:09 2023
Response via : Initial Calibration

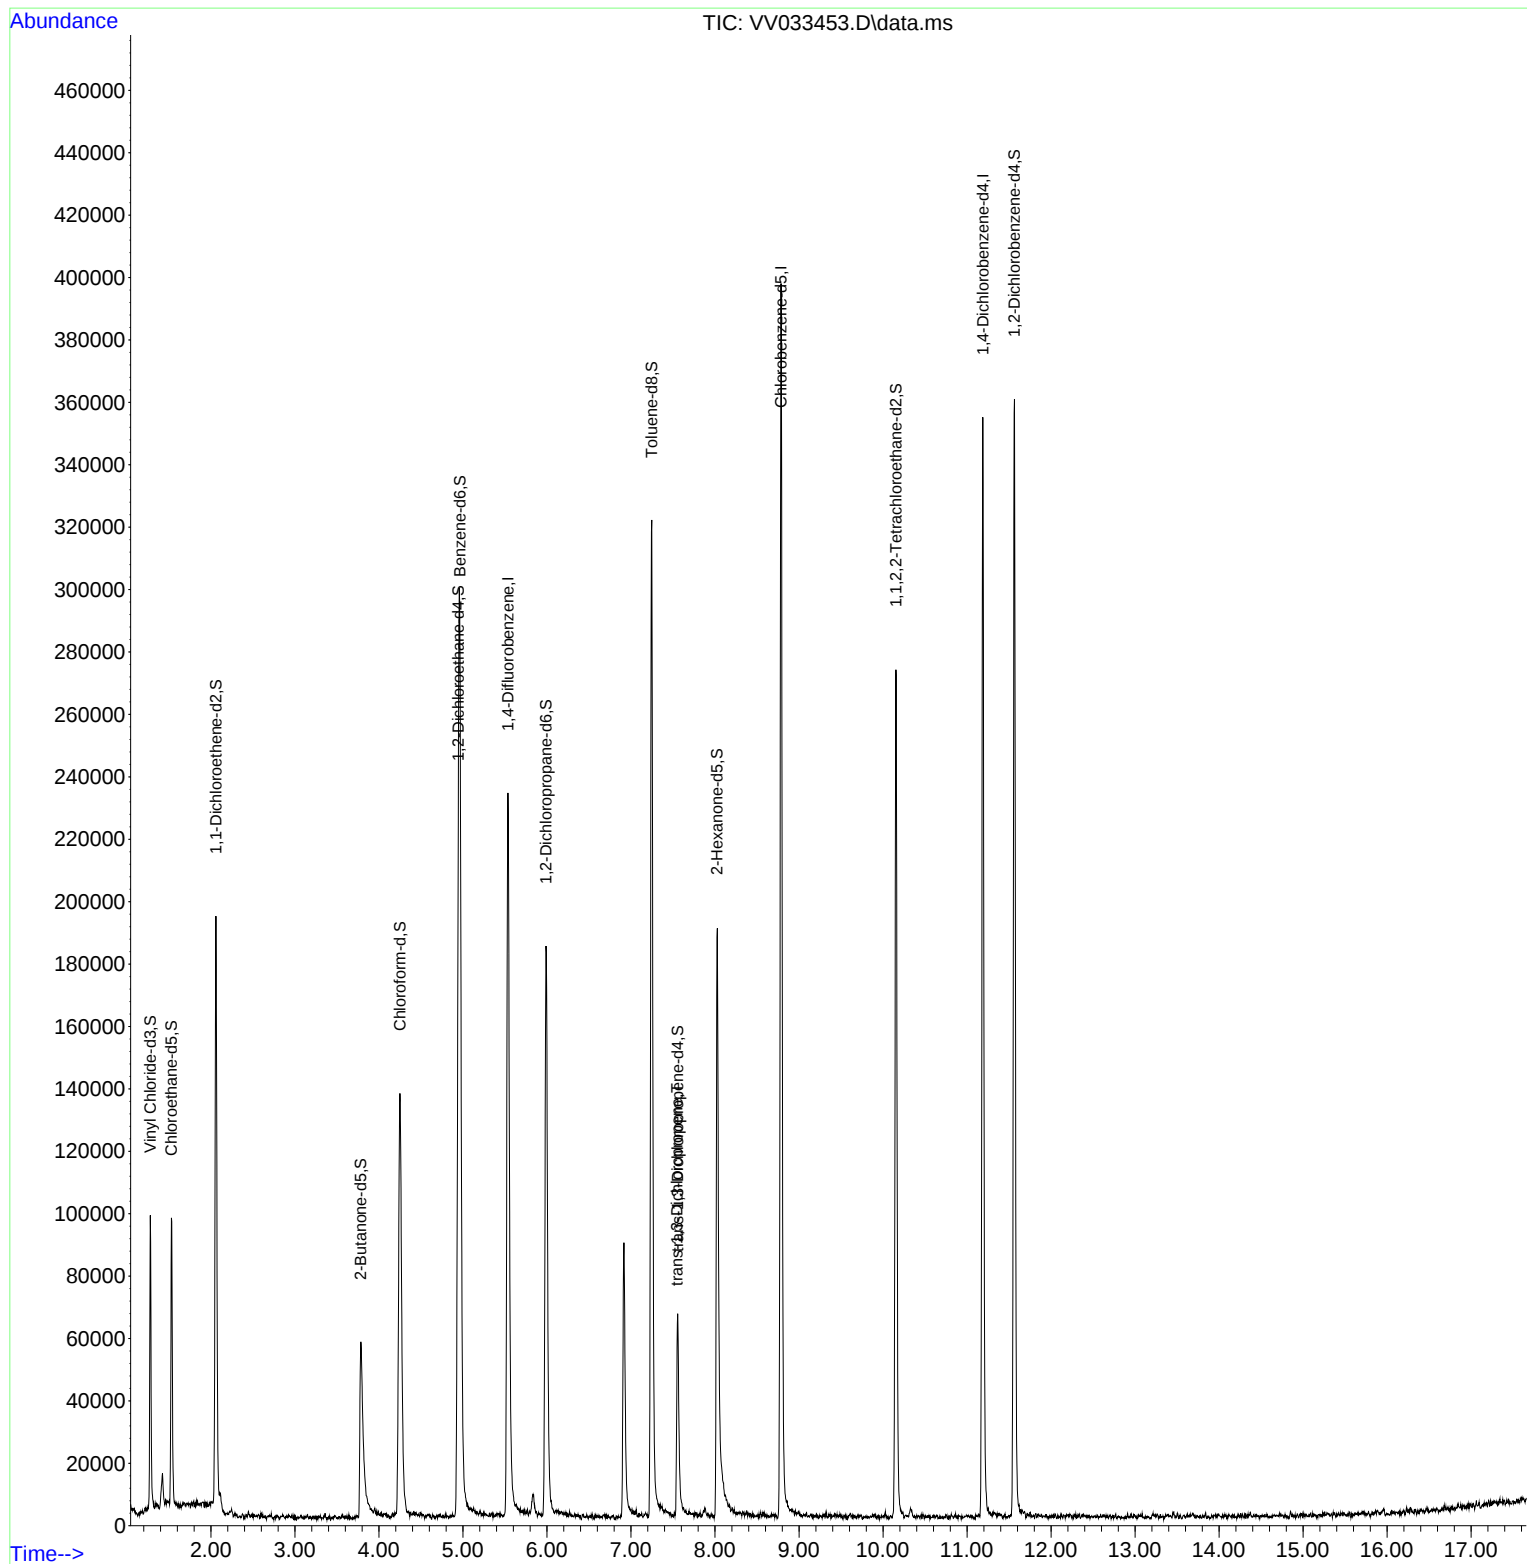

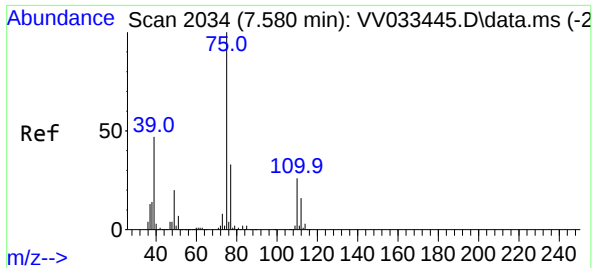

#44
trans-1,3-Dichloropropene
Concen: 0.912 ug/L
RT: 7.548 min Scan# 2031
Delta R.T. -0.032 min
Lab File: VV033453.D
Acq: 18 Dec 2023 13:30

Instrument :
MSVOA_V
ClientSampleId :

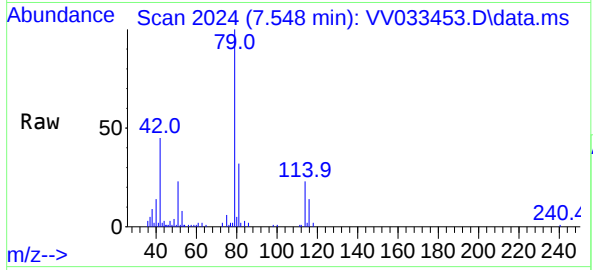

Tgt Ion:	75	Resp:	2031
Ion	Ratio	Lower	Upper
75	100		
77	31.8	22.4	41.6

