

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033446.D
 Acq On : 18 Dec 2023 10:41
 Operator : SY/MD
 Sample : VV1218MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	108136	112596	12.45%	1.639%
2	1.532	146	153	165	rVB	101971	121621	13.45%	1.770%
3	2.059	309	317	330	rVB	211191	300447	33.22%	4.373%
4	2.445	430	437	438	rBV7	2977	3545	0.39%	0.052%
5	2.529	461	463	465	rBV2	1001	510	0.06%	0.007%
6	2.638	493	497	500	rVB4	990	846	0.09%	0.012%
7	2.661	501	504	506	rVB3	1478	808	0.09%	0.012%
8	2.674	506	508	510	rBV2	741	516	0.06%	0.008%
9	2.738	526	528	529	rBV2	995	409	0.05%	0.006%
10	2.793	544	545	546	rBV	716	225	0.02%	0.003%
11	2.883	570	573	575	rBV3	899	458	0.05%	0.007%
12	2.899	575	578	583	rVB5	1592	1207	0.13%	0.018%
13	2.921	583	585	589	rBV4	947	427	0.05%	0.006%
14	2.979	600	603	606	rBV4	884	597	0.07%	0.009%
15	3.066	628	630	631	rBV	627	337	0.04%	0.005%
16	3.143	652	654	656	rBV	664	358	0.04%	0.005%
17	3.207	671	674	679	rVB5	1373	883	0.10%	0.013%
18	3.233	679	682	683	rBV2	662	348	0.04%	0.005%
19	3.291	697	700	705	rVB7	1625	1189	0.13%	0.017%
20	3.310	705	706	707	rBV	838	234	0.03%	0.003%
21	3.365	721	723	724	rBV2	811	291	0.03%	0.004%
22	3.426	741	742	746	rBV3	497	341	0.04%	0.005%
23	3.445	746	748	751	rVV2	1099	685	0.08%	0.010%
24	3.583	789	791	794	rBV4	1234	901	0.10%	0.013%
25	3.715	829	832	833	rBV3	1024	540	0.06%	0.008%
26	3.735	836	838	841	rVB4	1262	566	0.06%	0.008%
27	3.751	841	843	844	rBV2	820	328	0.04%	0.005%
28	3.783	844	853	880	rBV	57429	164142	18.15%	2.389%
29	4.249	985	998	1022	rBV	149482	372191	41.16%	5.417%
30	4.561	1093	1095	1096	rBV2	767	210	0.02%	0.003%
31	4.693	1134	1136	1138	rBV3	963	396		

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033446.D
 Acq On : 18 Dec 2023 10:41
 Operator : SY/MD
 Sample : VV1218MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	5.535	1387	1398	1421	rBV	255690	535633	59.23%	7.796%
38	5.989	1527	1539	1560	rBV2	199052	418426	46.27%	6.090%
39	6.603	1729	1730	1733	rVB3	1026	560	0.06%	0.008%
40	6.747	1771	1775	1777	rBV4	2066	1680	0.19%	0.024%
41	6.776	1782	1784	1787	rVV4	1102	641	0.07%	0.009%
42	6.841	1802	1804	1808	rVB4	1319	872	0.10%	0.013%
43	6.857	1808	1809	1814	rBV5	841	470	0.05%	0.007%
44	6.915	1815	1827	1848	rBV	97290	188735	20.87%	2.747%
45	7.059	1870	1872	1873	rBV3	1404	485	0.05%	0.007%
46	7.246	1918	1930	1950	rBV	374161	665027	73.54%	9.680%
47	7.554	2018	2026	2044	rVB	72266	125628	13.89%	1.829%
48	7.940	2144	2146	2151	rVB5	1633	1228	0.14%	0.018%
49	7.966	2151	2154	2157	rBV4	2127	1775	0.20%	0.026%
50	8.024	2162	2172	2210	rBV	193567	397657	43.97%	5.788%
51	8.516	2324	2325	2326	rBV2	1057	236	0.03%	0.003%
52	8.603	2350	2352	2354	rBV3	1097	604	0.07%	0.009%
53	8.680	2373	2376	2379	rBV5	1286	1028	0.11%	0.015%
54	8.786	2398	2409	2430	rBV	431029	712491	78.79%	10.371%
55	9.406	2601	2602	2605	rVB3	789	344	0.04%	0.005%
56	9.564	2647	2651	2654	rVB5	969	839	0.09%	0.012%
57	9.580	2654	2656	2657	rBV2	1191	505	0.06%	0.007%
58	9.612	2662	2666	2667	rBV3	1703	857	0.09%	0.012%
59	9.648	2674	2677	2680	rBV5	1301	878	0.10%	0.013%
60	9.667	2680	2683	2686	rBV4	1531	958	0.11%	0.014%
61	9.770	2713	2715	2718	rBV3	974	719	0.08%	0.010%
62	9.812	2723	2728	2731	rBV5	1526	1248	0.14%	0.018%
63	9.934	2764	2766	2768	rBV2	837	404	0.04%	0.006%
64	9.998	2783	2786	2788	rBV3	1126	629	0.07%	0.009%
65	10.027	2794	2795	2797	rBV2	1213	525	0.06%	0.008%
66	10.152	2823	2834	2849	rBV	291564	464660	51.38%	6.763%
67	10.339	2891	2892	2896	rBV4	1098	916	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033446.D
 Acq On : 18 Dec 2023 10:41
 Operator : SY/MD
 Sample : VV1218MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.223	3476	3478	3483	rVB5	1654	979	0.11%	0.014%
78	12.249	3483	3486	3488	rBV3	963	730	0.08%	0.011%
79	12.271	3491	3493	3494	rBV2	1290	383	0.04%	0.006%
80	12.284	3495	3497	3501	rVB4	1369	663	0.07%	0.010%
81	12.451	3547	3549	3552	rBV4	813	551	0.06%	0.008%
82	12.641	3606	3608	3610	rVB3	1028	357	0.04%	0.005%
83	12.657	3610	3613	3614	rBV2	1633	658	0.07%	0.010%
84	12.667	3614	3616	3618	rVB3	1512	645	0.07%	0.009%
85	12.766	3644	3647	3648	rBV3	863	440	0.05%	0.006%
86	12.827	3664	3666	3668	rBV3	1121	718	0.08%	0.010%
87	12.889	3682	3685	3686	rBV2	887	489	0.05%	0.007%
88	13.165	3768	3771	3772	rBV3	925	479	0.05%	0.007%
89	13.255	3797	3799	3802	rBV3	772	614	0.07%	0.009%
90	13.348	3827	3828	3830	rVB2	760	233	0.03%	0.003%
91	13.445	3852	3858	3870	rVB2	10161	17856	1.97%	0.260%
92	13.622	3911	3913	3915	rBV3	1144	706	0.08%	0.010%
93	13.686	3924	3933	3944	rBV3	6772	12515	1.38%	0.182%
94	14.155	4075	4079	4083	rBV6	1284	1432	0.16%	0.021%
95	14.416	4158	4160	4162	rVB3	1145	387	0.04%	0.006%
96	14.451	4169	4171	4174	rBV4	1133	537	0.06%	0.008%
97	14.570	4207	4208	4211	rBV3	864	388	0.04%	0.006%
98	14.757	4262	4266	4267	rBV4	1572	1143	0.13%	0.017%
99	14.898	4306	4310	4313	rBV4	1622	1405	0.16%	0.020%
100	15.477	4486	4490	4492	rBV5	1800	1458	0.16%	0.021%



Sum of corrected areas: 6870212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033446.D
Acq On : 18 Dec 2023 10:41
Operator : SY/MD
Sample : VV1218MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

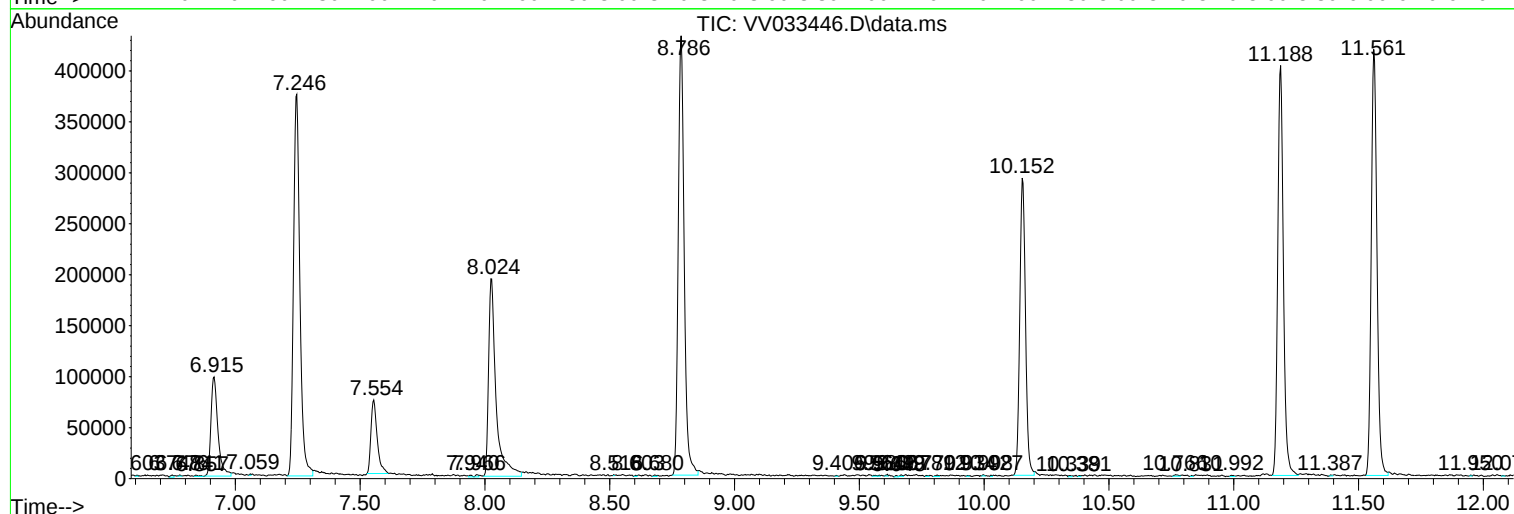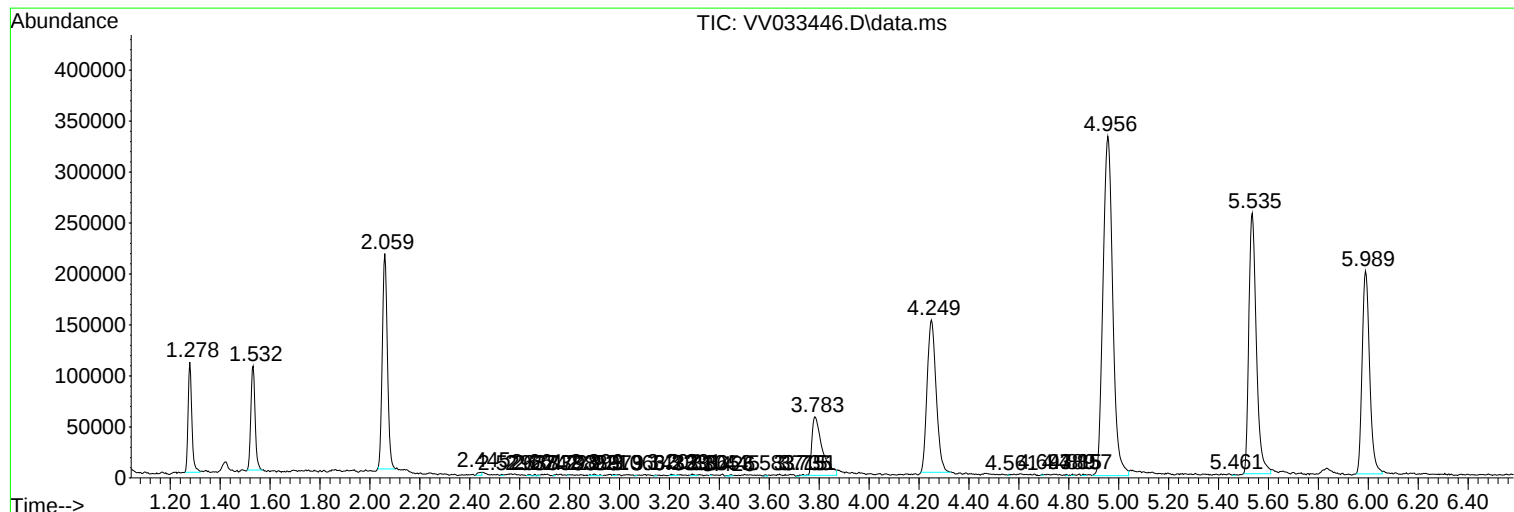

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033446.D
Acq On : 18 Dec 2023 10:41
Operator : SY/MD
Sample : VV1218MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033446.D
Acq On : 18 Dec 2023 10:41
Operator : SY/MD
Sample : VV1218MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc