

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033447.D
 Acq On : 18 Dec 2023 11:05
 Operator : SY/MD
 Sample : VV1218WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rVB	106153	107574	12.12%	1.606%
2	1.532	146	153	168	rVB	105968	124446	14.02%	1.858%
3	2.060	308	317	328	rBV	203789	295649	33.30%	4.414%
4	2.867	566	568	569	rBV2	1006	428	0.05%	0.006%
5	2.999	607	609	612	rBV4	1275	576	0.06%	0.009%
6	3.095	637	639	641	rBV2	782	408	0.05%	0.006%
7	3.163	658	660	663	rBV3	895	496	0.06%	0.007%
8	3.384	728	729	731	rBV2	1011	504	0.06%	0.008%
9	3.394	731	732	733	rBV	674	242	0.03%	0.004%
10	3.491	759	762	765	rVB4	1932	1018	0.11%	0.015%
11	3.503	765	766	767	rBV	555	156	0.02%	0.002%
12	3.516	769	770	772	rBV2	761	386	0.04%	0.006%
13	3.626	801	804	806	rBV4	799	549	0.06%	0.008%
14	3.638	806	808	812	rVB5	1078	579	0.07%	0.009%
15	3.658	812	814	816	rBV3	1051	584	0.07%	0.009%
16	3.706	827	829	830	rBV2	913	384	0.04%	0.006%
17	3.719	830	833	837	rVV4	1237	801	0.09%	0.012%
18	3.783	845	853	879	rBV	59462	164384	18.51%	2.454%
19	4.076	942	944	946	rBV3	1433	687	0.08%	0.010%
20	4.249	987	998	1021	rVB	144159	360758	40.63%	5.386%
21	4.957	1202	1218	1257	rBV3	329109	887929	100.00%	13.255%
22	5.378	1346	1349	1352	rBV5	1377	1302	0.15%	0.019%
23	5.535	1387	1398	1422	rBV	249698	525335	59.16%	7.842%
24	5.989	1527	1539	1563	rBV	196655	410122	46.19%	6.122%
25	6.426	1673	1675	1677	rBV3	1174	693	0.08%	0.010%
26	6.513	1699	1702	1703	rBV2	1493	783	0.09%	0.012%
27	6.915	1817	1827	1847	rBV	96975	188599	21.24%	2.815%
28	7.246	1919	1930	1950	rBV	360760	643640	72.49%	9.609%
29	7.555	2017	2026	2044	rBV	70172	126179	14.21%	1.884%
30	8.027	2163	2173	2205	rBV	191980	398857	44.92%	5.954%
31	8.786	2398	2409	2433	rBV	423453	699814	78.81%	10.447%
32	9.236	2547	2549	2552	rBV3	1330	826	0.09%	0.012%
33	9.320	2573	2575	2577	rBV3	1368	741	0.08%	0.011%
34	9.423	2605	2607	2611	rBV5	1186	622	0.07%	0.009%
35	9.522	2636	2638	2641	rVB4	1265	514	0.06%	0.008%
36	9.783	2716	2719	2722	rBV4	1600	1310	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033447.D
 Acq On : 18 Dec 2023 11:05
 Operator : SY/MD
 Sample : VV1218WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	9.828	2730	2733	2735	rBV2	1713	1139	0.13%	0.017%
38	9.976	2777	2779	2781	rBV4	907	351	0.04%	0.005%
39	10.098	2815	2817	2821	rBV4	1065	877	0.10%	0.013%
40	10.153	2823	2834	2849	rBV	290577	461456	51.97%	6.889%
41	10.487	2931	2938	2943	rBV10	2322	3095	0.35%	0.046%
42	10.712	3004	3008	3010	rBV4	1321	879	0.10%	0.013%
43	10.799	3033	3035	3036	rBV2	1221	575	0.06%	0.009%
44	10.892	3062	3064	3065	rBV2	1028	391	0.04%	0.006%
45	10.928	3072	3075	3077	rBV2	858	372	0.04%	0.006%
46	11.005	3097	3099	3100	rBV2	1011	305	0.03%	0.005%
47	11.046	3110	3112	3114	rBV	840	391	0.04%	0.006%
48	11.088	3123	3125	3131	rVB4	964	692	0.08%	0.010%
49	11.188	3145	3156	3177	rBV	388015	621463	69.99%	9.277%
50	11.500	3251	3253	3255	rBV3	1181	632	0.07%	0.009%
51	11.561	3262	3272	3290	rBV	410392	649927	73.20%	9.702%
52	11.915	3381	3382	3383	rBV	1187	396	0.04%	0.006%
53	12.153	3454	3456	3458	rBV3	1196	575	0.06%	0.009%
54	12.246	3482	3485	3488	rBV4	1327	798	0.09%	0.012%
55	12.587	3588	3591	3592	rBV3	1707	895	0.10%	0.013%
56	12.783	3649	3652	3653	rBV2	1662	1033	0.12%	0.015%
57	12.963	3706	3708	3711	rBV4	1025	527	0.06%	0.008%
58	13.169	3769	3772	3776	rVB5	1755	1260	0.14%	0.019%
59	13.352	3827	3829	3833	rBV4	1030	663	0.07%	0.010%
60	13.641	3917	3919	3920	rBV	1376	638	0.07%	0.010%
61	14.201	4091	4093	4097	rBV4	1456	1116	0.13%	0.017%
62	14.824	4286	4287	4288	rBV	880	311	0.04%	0.005%




Sum of corrected areas: 6698632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033447.D
Acq On : 18 Dec 2023 11:05
Operator : SY/MD
Sample : VV1218WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

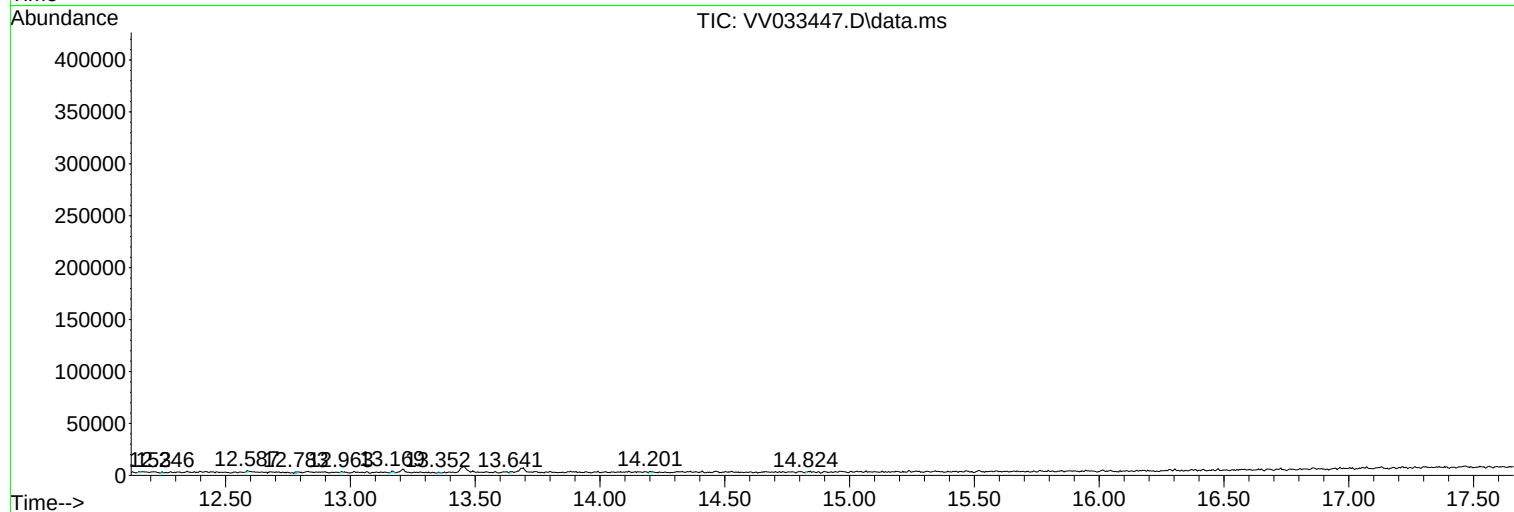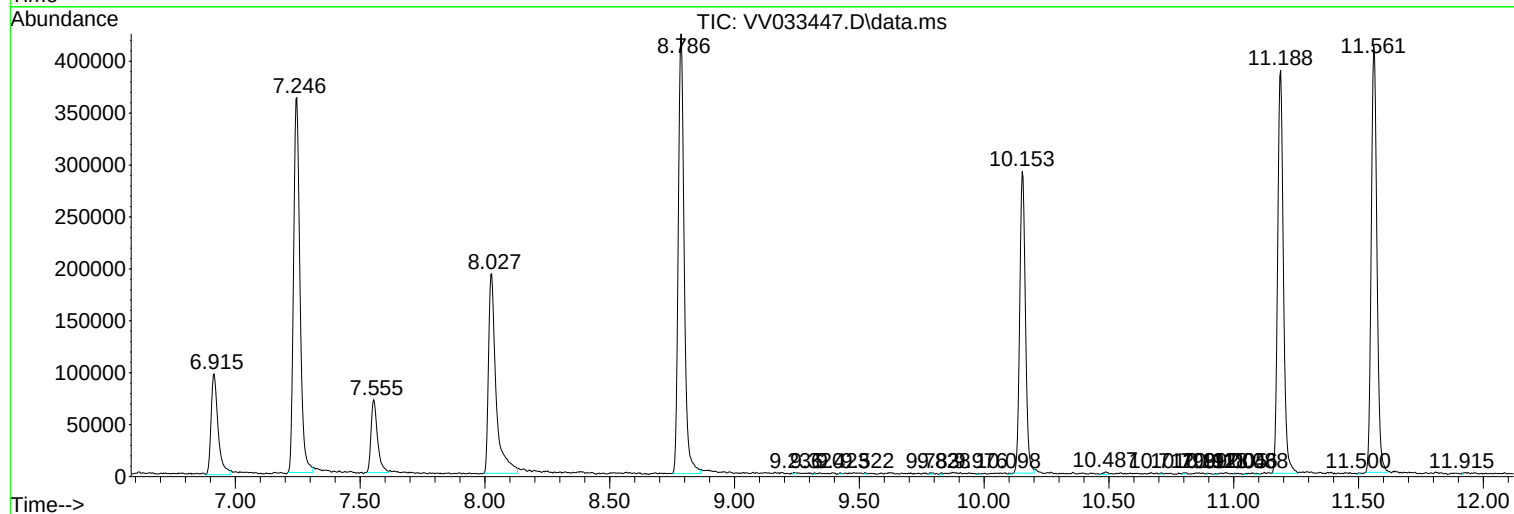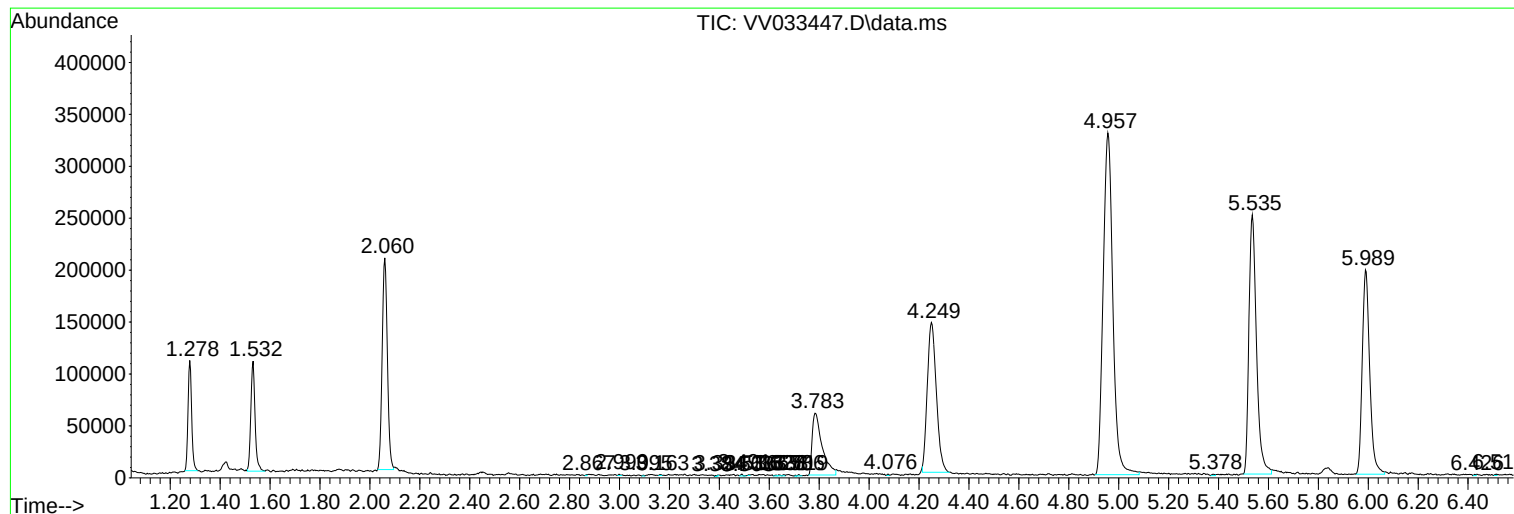

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033447.D
Acq On : 18 Dec 2023 11:05
Operator : SY/MD
Sample : VV1218WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033447.D
Acq On : 18 Dec 2023 11:05
Operator : SY/MD
Sample : VV1218WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------