

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033448.D
 Acq On : 18 Dec 2023 11:34
 Operator : SY/MD
 Sample : 05802-19DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	105620	109894	8.93%	1.510%
2	1.529	146	152	164	rVB	97676	114197	9.28%	1.569%
3	2.060	308	317	332	rVB	203555	293230	23.83%	4.029%
4	2.388	416	419	421	rBV3	1646	1091	0.09%	0.015%
5	2.442	432	436	447	rVB8	5137	8439	0.69%	0.116%
6	2.677	507	509	511	rBV3	1302	650	0.05%	0.009%
7	2.719	519	522	527	rBV7	1202	663	0.05%	0.009%
8	2.802	544	548	550	rBV5	1014	743	0.06%	0.010%
9	3.024	614	617	621	rBV5	950	737	0.06%	0.010%
10	3.060	626	628	631	rBV3	1119	723	0.06%	0.010%
11	3.162	656	660	662	rBV3	750	574	0.05%	0.008%
12	3.211	673	675	679	rBV5	826	612	0.05%	0.008%
13	3.304	700	704	706	rBV4	858	708	0.06%	0.010%
14	3.352	717	719	722	rBV3	1500	1061	0.09%	0.015%
15	3.445	744	748	750	rBV4	1056	909	0.07%	0.012%
16	3.532	772	775	778	rBV5	967	727	0.06%	0.010%
17	3.783	844	853	879	rBV2	54424	153096	12.44%	2.103%
18	4.105	949	953	956	rBV6	1850	1469	0.12%	0.020%
19	4.249	982	998	1023	rBV	144060	375867	30.55%	5.164%
20	4.600	1104	1107	1109	rBV3	1350	885	0.07%	0.012%
21	4.613	1109	1111	1113	rVV3	1072	494	0.04%	0.007%
22	4.860	1185	1188	1189	rBV3	1346	724	0.06%	0.010%
23	4.870	1189	1191	1197	rVB6	1384	1220	0.10%	0.017%
24	4.957	1202	1218	1243	rVV2	317870	850711	69.14%	11.688%
25	5.478	1378	1380	1382	rBV3	1087	551	0.04%	0.008%
26	5.532	1387	1397	1426	rVV	239392	506481	41.16%	6.958%
27	5.812	1481	1484	1485	rBV2	2510	1471	0.12%	0.020%
28	5.989	1526	1539	1558	rBV	192990	402381	32.70%	5.528%
29	6.268	1624	1626	1629	rBV4	1419	940	0.08%	0.013%
30	6.288	1629	1632	1634	rBV4	1327	904	0.07%	0.012%
31	6.384	1660	1662	1664	rBV3	1504	605	0.05%	0.008%
32	6.596	1726	1728	1732	rVB4	1296	902	0.07%	0.012%
33	6.722	1764	1767	1769	rVB4	1296	632	0.05%	0.009%
34	6.744	1769	1774	1780	rVB9	1463	1733	0.14%	0.024%
35	6.773	1780	1783	1786	rVB5	1084	817	0.07%	0.011%
36	6.789	1786	1788	1793	rBV6	1376	1007	0.08%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033448.D
 Acq On : 18 Dec 2023 11:34
 Operator : SY/MD
 Sample : 05802-19DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.915	1817	1827	1844	rBV	88282	170206	13.83%	2.338%
38	7.243	1917	1929	1950	rBV	356367	637532	51.81%	8.759%
39	7.555	2017	2026	2042	rBV	70430	125955	10.24%	1.730%
40	7.905	2132	2135	2138	rBV4	1202	1001	0.08%	0.014%
41	7.969	2150	2155	2158	rBV6	2081	1977	0.16%	0.027%
42	8.024	2163	2172	2203	rVV	175577	352172	28.62%	4.838%
43	8.561	2335	2339	2342	rVB4	1138	737	0.06%	0.010%
44	8.741	2391	2395	2397	rBV4	1187	752	0.06%	0.010%
45	8.786	2397	2409	2440	rBV2	409393	784960	63.79%	10.784%
46	9.169	2525	2528	2530	rBV3	1488	772	0.06%	0.011%
47	9.310	2569	2572	2574	rBV4	1400	756	0.06%	0.010%
48	9.329	2574	2578	2579	rBV3	1450	1150	0.09%	0.016%
49	9.416	2601	2605	2609	rBV7	1886	1639	0.13%	0.023%
50	9.545	2643	2645	2651	rVB6	1052	976	0.08%	0.013%
51	9.690	2686	2690	2692	rBV4	999	753	0.06%	0.010%
52	9.731	2701	2703	2704	rBV2	1154	573	0.05%	0.008%
53	9.908	2756	2758	2761	rBV3	1232	838	0.07%	0.012%
54	9.966	2773	2776	2777	rBV3	1108	489	0.04%	0.007%
55	9.985	2780	2782	2786	rVB5	2331	1269	0.10%	0.017%
56	10.005	2786	2788	2793	rBV5	894	658	0.05%	0.009%
57	10.153	2822	2834	2854	rBV	284045	449433	36.53%	6.175%
58	10.291	2875	2877	2884	rVB6	1496	921	0.07%	0.013%
59	10.362	2896	2899	2900	rBV2	967	515	0.04%	0.007%
60	10.458	2926	2929	2932	rBV4	923	772	0.06%	0.011%
61	10.481	2932	2936	2937	rBV3	1292	1012	0.08%	0.014%
62	10.577	2962	2966	2967	rBV4	834	537	0.04%	0.007%
63	10.587	2967	2969	2975	rVB6	827	668	0.05%	0.009%
64	10.622	2977	2980	2984	rVB5	1156	808	0.07%	0.011%
65	10.693	2998	3002	3004	rBV4	1152	645	0.05%	0.009%
66	10.767	3021	3025	3026	rBV3	951	682	0.06%	0.009%
67	10.850	3048	3051	3053	rBV3	1865	1078	0.09%	0.015%
68	10.940	3075	3079	3081	rBV4	1495	1129	0.09%	0.016%
69	10.979	3090	3091	3094	rBV3	815	542	0.04%	0.007%
70	11.072	3117	3120	3121	rBV2	807	496	0.04%	0.007%
71	11.188	3145	3156	3175	rBV	380878	640501	52.05%	8.800%
72	11.567	3262	3274	3304	rVB3	522953	1230472	100.00%	16.905%
73	11.751	3328	3331	3333	rBV4	1591	940	0.08%	0.013%
74	11.863	3365	3366	3369	rVB2	1320	601	0.05%	0.008%
75	12.091	3433	3437	3441	rBV6	1365	1294	0.11%	0.018%
76	12.217	3472	3476	3479	rBV3	1706	1469	0.12%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033448.D
 Acq On : 18 Dec 2023 11:34
 Operator : SY/MD
 Sample : 05802-19DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.265	3486	3491	3494	rBV7	1144	1308	0.11%	0.018%
78	12.297	3499	3501	3505	rVV4	1085	707	0.06%	0.010%
79	12.664	3613	3615	3618	rVB4	1593	753	0.06%	0.010%
80	12.689	3620	3623	3625	rBV4	1178	818	0.07%	0.011%
81	12.882	3680	3683	3685	rBV5	1354	636	0.05%	0.009%
82	12.911	3690	3692	3694	rBV3	985	548	0.04%	0.008%
83	12.947	3700	3703	3709	rBV5	1294	1326	0.11%	0.018%
84	12.969	3709	3710	3715	rBV5	915	647	0.05%	0.009%
85	13.005	3719	3721	3723	rBV3	1419	743	0.06%	0.010%
86	13.088	3743	3747	3751	rBV7	1270	1059	0.09%	0.015%
87	13.136	3760	3762	3765	rVB4	1241	552	0.04%	0.008%
88	13.320	3815	3819	3820	rBV4	1471	1136	0.09%	0.016%
89	13.500	3870	3875	3877	rBV7	1398	1384	0.11%	0.019%
90	13.779	3958	3962	3964	rBV6	1331	1003	0.08%	0.014%
91	13.911	4000	4003	4007	rBV6	1134	1030	0.08%	0.014%
92	14.008	4031	4033	4036	rBV4	1031	598	0.05%	0.008%
93	14.075	4051	4054	4057	rBV5	1606	990	0.08%	0.014%
94	14.127	4068	4070	4072	rBV2	1046	486	0.04%	0.007%
95	14.297	4118	4123	4124	rBV3	1256	715	0.06%	0.010%
96	14.503	4181	4187	4191	rBV5	1617	1879	0.15%	0.026%
97	14.786	4271	4275	4276	rBV3	746	539	0.04%	0.007%
98	14.918	4314	4316	4317	rBV2	1154	489	0.04%	0.007%
99	15.451	4480	4482	4483	rBV2	1206	535	0.04%	0.007%
100	15.590	4523	4525	4531	rVB7	1651	1295	0.11%	0.018%


Sum of corrected areas: 7278704

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033448.D
Acq On : 18 Dec 2023 11:34
Operator : SY/MD
Sample : 05802-19DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

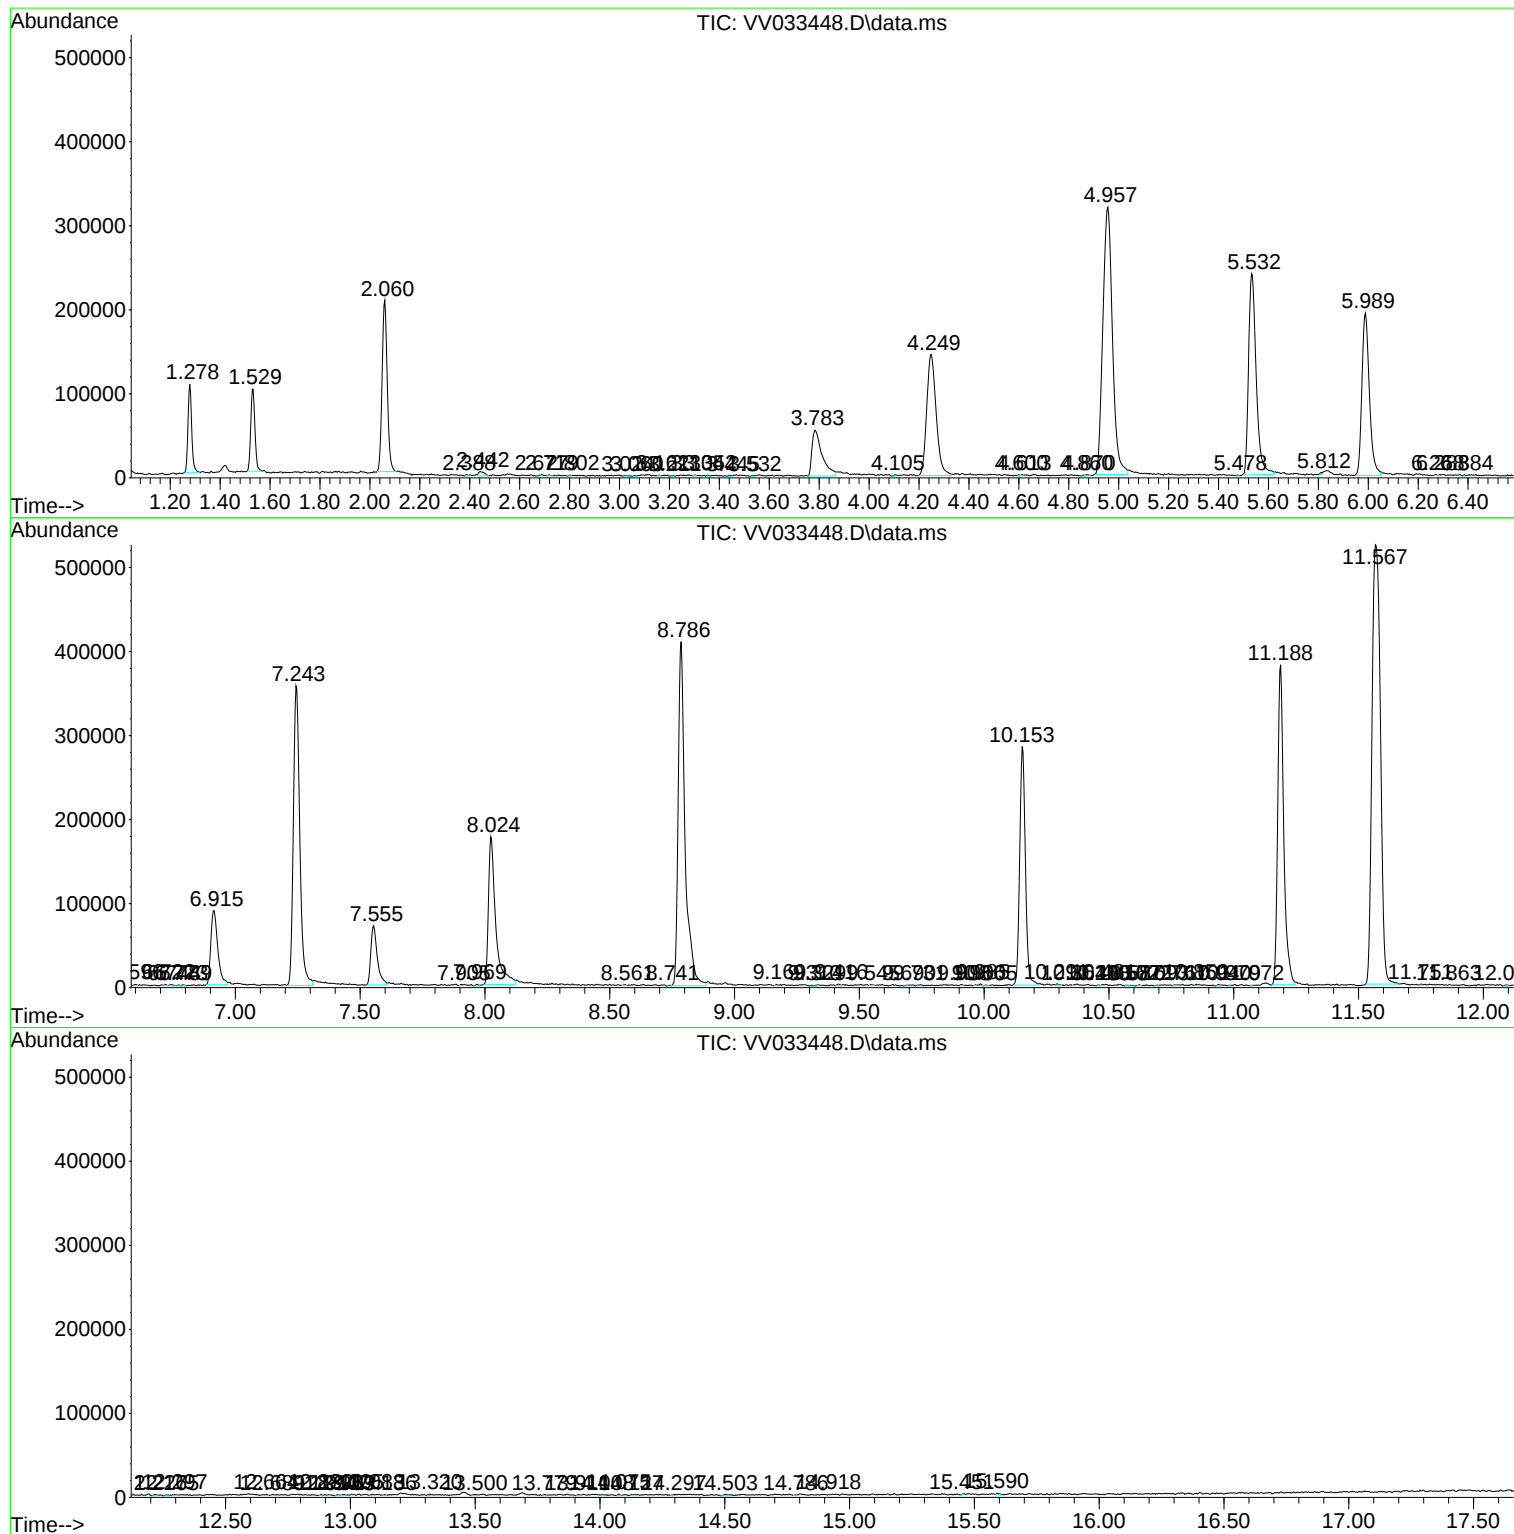

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033448.D
Acq On : 18 Dec 2023 11:34
Operator : SY/MD
Sample : 05802-19DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033448.D
Acq On : 18 Dec 2023 11:34
Operator : SY/MD
Sample : 05802-19DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------