

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033449.D
 Acq On : 18 Dec 2023 11:57
 Operator : SY/MD
 Sample : 05802-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	102779	105927	12.37%	1.606%
2	1.532	146	153	167	rVB	99334	120184	14.04%	1.823%
3	2.060	309	317	327	rBV	196686	274638	32.07%	4.165%
4	2.751	529	532	534	rBV3	746	571	0.07%	0.009%
5	2.844	558	561	568	rVB6	1839	1587	0.19%	0.024%
6	2.873	568	570	571	rBV	980	467	0.05%	0.007%
7	2.908	579	581	582	rBV	707	314	0.04%	0.005%
8	3.056	624	627	628	rBV	1288	629	0.07%	0.010%
9	3.092	636	638	640	rBV3	490	263	0.03%	0.004%
10	3.124	644	648	651	rVB4	1182	886	0.10%	0.013%
11	3.140	651	653	654	rBV	1227	556	0.06%	0.008%
12	3.195	668	670	671	rBV2	803	338	0.04%	0.005%
13	3.262	686	691	694	rBV6	1221	1151	0.13%	0.017%
14	3.291	698	700	701	rVV2	518	155	0.02%	0.002%
15	3.359	719	721	724	rBV4	924	573	0.07%	0.009%
16	3.397	729	733	734	rBV3	1018	751	0.09%	0.011%
17	3.452	749	750	752	rBV2	756	410	0.05%	0.006%
18	3.494	761	763	767	rBV4	928	740	0.09%	0.011%
19	3.642	806	809	811	rBV4	1250	748	0.09%	0.011%
20	3.654	811	813	816	rVV2	1284	624	0.07%	0.009%
21	3.690	822	824	827	rBV3	834	552	0.06%	0.008%
22	3.786	842	854	880	rBV	56395	162158	18.94%	2.459%
23	4.249	983	998	1023	rBV	145198	375809	43.89%	5.699%
24	4.619	1111	1113	1114	rBV2	1176	437	0.05%	0.007%
25	4.889	1195	1197	1198	rBV	996	465	0.05%	0.007%
26	4.957	1202	1218	1246	rVV2	317769	856269	100.00%	12.985%
27	5.535	1387	1398	1421	rBV	253973	520201	60.75%	7.888%
28	5.796	1477	1479	1481	rBV3	1639	819	0.10%	0.012%
29	5.989	1528	1539	1570	rVB	191124	399911	46.70%	6.064%
30	6.458	1683	1685	1688	rVB3	1633	826	0.10%	0.013%
31	6.818	1795	1797	1800	rVB5	1242	676	0.08%	0.010%
32	6.834	1800	1802	1803	rBV2	1225	469	0.05%	0.007%
33	6.915	1817	1827	1843	rBV	92954	175054	20.44%	2.655%
34	7.124	1890	1892	1894	rBV3	1252	743	0.09%	0.011%
35	7.162	1901	1904	1906	rBV4	1636	1038	0.12%	0.016%
36	7.246	1920	1930	1948	rBV	346517	604843	70.64%	9.172%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033449.D
 Acq On : 18 Dec 2023 11:57
 Operator : SY/MD
 Sample : 05802-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.555	2017	2026	2051	rBV	69926	126603	14.79%	1.920%
38	7.818	2106	2108	2110	rBV2	1126	545	0.06%	0.008%
39	7.879	2117	2127	2136	rBV2	11354	21271	2.48%	0.323%
40	7.940	2144	2146	2147	rBV2	1388	694	0.08%	0.011%
41	8.027	2164	2173	2201	rBV	188184	374177	43.70%	5.674%
42	8.468	2305	2310	2311	rBV5	1738	1326	0.15%	0.020%
43	8.747	2395	2397	2398	rBV2	826	457	0.05%	0.007%
44	8.786	2398	2409	2429	rVV	423741	697627	81.47%	10.579%
45	9.191	2534	2535	2538	rBV3	826	416	0.05%	0.006%
46	9.432	2609	2610	2613	rBV4	1409	646	0.08%	0.010%
47	9.583	2652	2657	2663	rBV10	1778	2231	0.26%	0.034%
48	9.616	2663	2667	2670	rBV5	1055	856	0.10%	0.013%
49	9.760	2707	2712	2714	rBV5	1265	1226	0.14%	0.019%
50	9.808	2725	2727	2731	rBV4	1095	675	0.08%	0.010%
51	9.825	2731	2732	2735	rVB3	869	400	0.05%	0.006%
52	10.001	2785	2787	2789	rVB3	1481	542	0.06%	0.008%
53	10.066	2805	2807	2808	rBV2	1381	600	0.07%	0.009%
54	10.153	2824	2834	2856	rBV	281536	452497	52.85%	6.862%
55	10.329	2882	2889	2898	rVB4	10070	15581	1.82%	0.236%
56	10.461	2928	2930	2933	rBV3	1004	704	0.08%	0.011%
57	10.590	2967	2970	2971	rBV2	847	493	0.06%	0.007%
58	10.638	2983	2985	2988	rBV4	963	503	0.06%	0.008%
59	10.731	3012	3014	3017	rVB4	1489	720	0.08%	0.011%
60	10.763	3021	3024	3025	rBV3	765	361	0.04%	0.005%
61	10.808	3036	3038	3040	rBV2	971	478	0.06%	0.007%
62	10.844	3046	3049	3050	rBV3	904	528	0.06%	0.008%
63	10.915	3069	3071	3073	rBV3	989	396	0.05%	0.006%
64	10.966	3085	3087	3088	rBV2	1336	606	0.07%	0.009%
65	11.079	3118	3122	3125	rBV5	980	878	0.10%	0.013%
66	11.188	3144	3156	3176	rBV	390056	615045	71.83%	9.327%
67	11.500	3246	3253	3254	rBV6	2419	2559	0.30%	0.039%
68	11.509	3254	3256	3259	rVV4	3406	2299	0.27%	0.035%
69	11.561	3262	3272	3294	rVB	398786	644583	75.28%	9.775%
70	12.236	3480	3482	3483	rBV2	689	368	0.04%	0.006%
71	12.268	3490	3492	3496	rBV4	1082	738	0.09%	0.011%
72	12.287	3496	3498	3500	rBV3	960	448	0.05%	0.007%
73	12.349	3515	3517	3518	rBV2	1443	494	0.06%	0.007%
74	12.374	3523	3525	3526	rBV2	772	252	0.03%	0.004%
75	12.403	3529	3534	3536	rBV5	767	680	0.08%	0.010%
76	12.419	3536	3539	3541	rBV3	1326	897	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033449.D
Acq On : 18 Dec 2023 11:57
Operator : SY/MD
Sample : 05802-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis

77	12.445	3545	3547	3548	rBV	1001	215	0.03%	0.003%
78	12.551	3578	3580	3582	rBV3	1018	512	0.06%	0.008%
79	12.882	3681	3683	3686	rBV4	897	495	0.06%	0.008%
80	12.895	3686	3687	3692	rVV4	887	440	0.05%	0.007%
81	13.168	3768	3772	3777	rVB6	1166	862	0.10%	0.013%
82	13.291	3808	3810	3811	rBV2	1107	554	0.06%	0.008%
83	13.371	3833	3835	3838	rBV4	624	477	0.06%	0.007%
84	13.603	3903	3907	3909	rBV4	1144	758	0.09%	0.011%
85	14.014	4034	4035	4038	rBV3	1187	634	0.07%	0.010%
86	14.030	4038	4040	4043	rVV4	1178	760	0.09%	0.012%
87	14.178	4079	4086	4087	rBV6	1440	1661	0.19%	0.025%
88	14.419	4159	4161	4165	rBV4	1020	871	0.10%	0.013%
89	14.599	4212	4217	4218	rBV5	1331	1151	0.13%	0.017%
90	14.934	4319	4321	4324	rBV4	1598	860	0.10%	0.013%




Sum of corrected areas: 6594432

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033449.D
Acq On : 18 Dec 2023 11:57
Operator : SY/MD
Sample : 05802-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

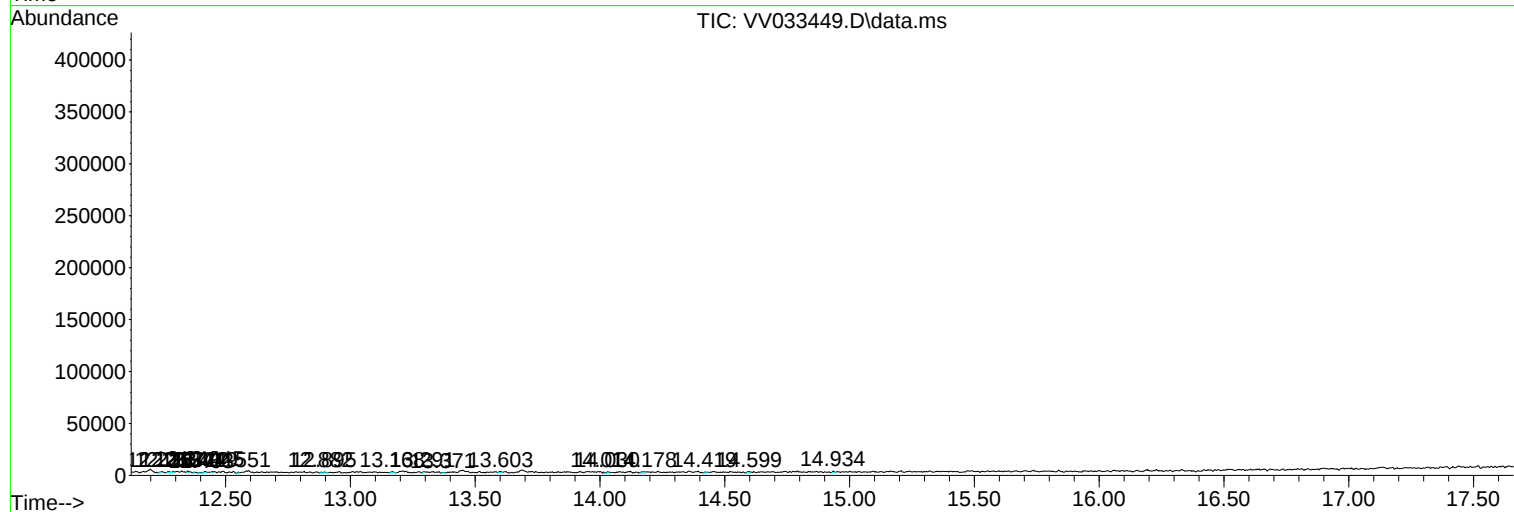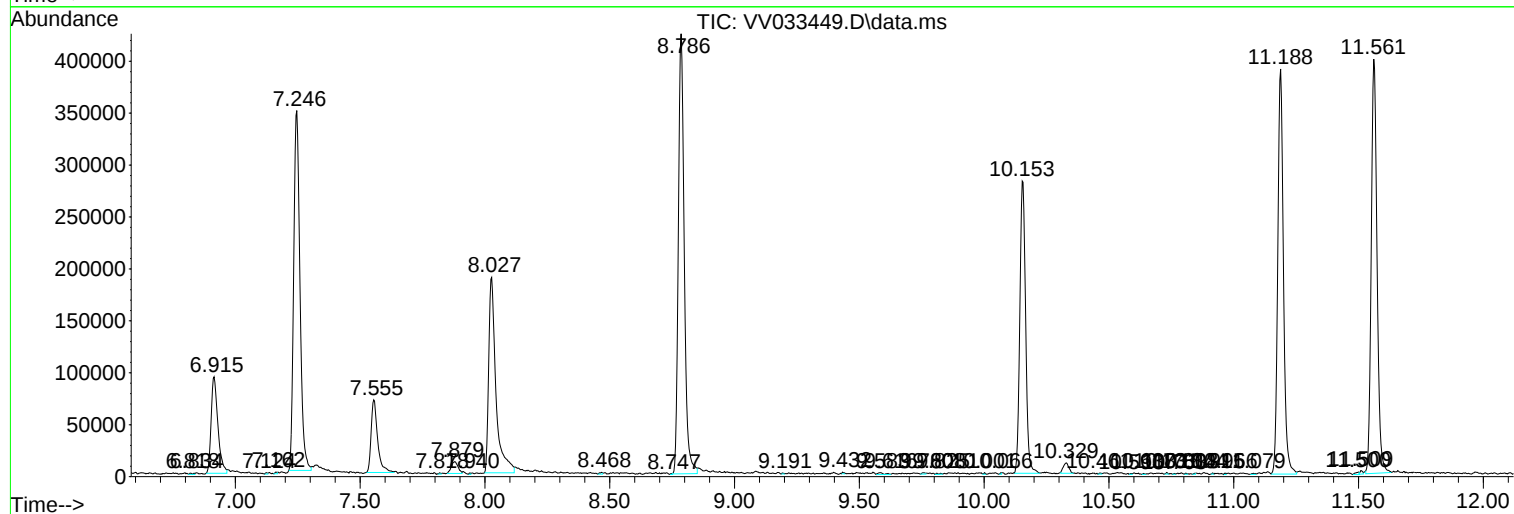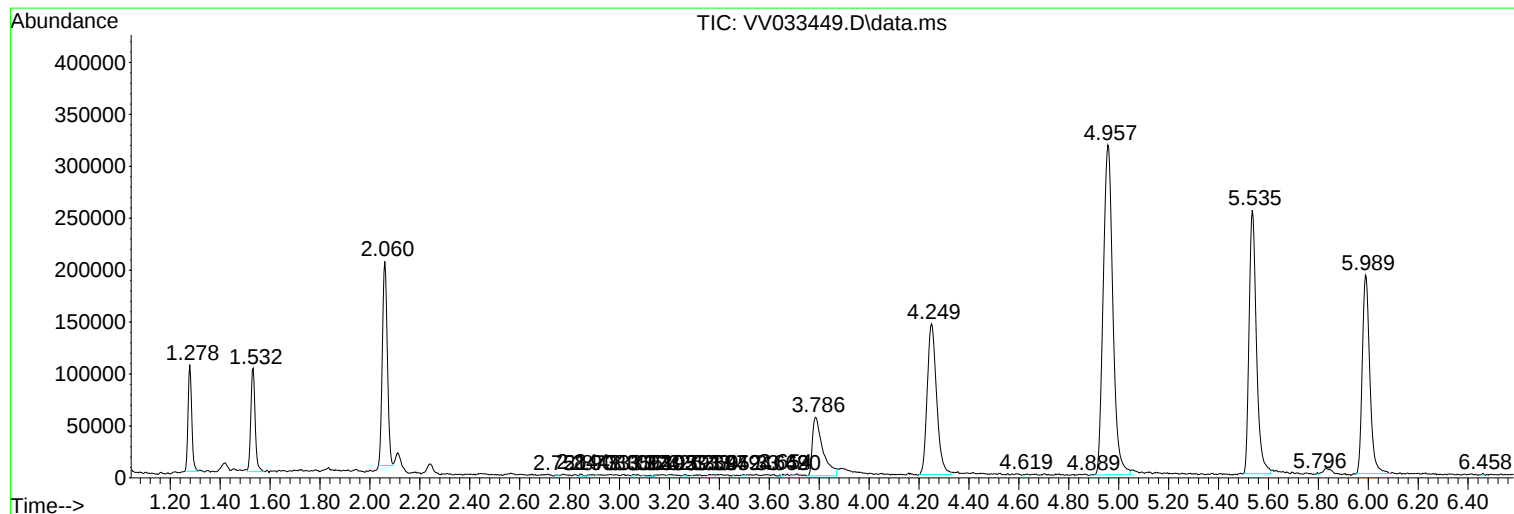

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033449.D
Acq On : 18 Dec 2023 11:57
Operator : SY/MD
Sample : 05802-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033449.D
Acq On : 18 Dec 2023 11:57
Operator : SY/MD
Sample : 05802-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------