

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033450.D
 Acq On : 18 Dec 2023 12:20
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	86604	91381	11.48%	1.514%
2	1.529	146	152	166	rVB	84230	101136	12.71%	1.675%
3	2.060	309	317	330	rVB	170491	242262	30.44%	4.013%
4	2.233	369	371	373	rBV3	1716	847	0.11%	0.014%
5	2.281	383	386	389	rBV4	1253	849	0.11%	0.014%
6	2.352	403	408	409	rBV4	1348	1184	0.15%	0.020%
7	2.487	448	450	453	rBV4	947	547	0.07%	0.009%
8	2.658	499	503	504	rBV3	1200	691	0.09%	0.011%
9	2.699	514	516	519	rBV3	1155	629	0.08%	0.010%
10	2.924	584	586	588	rBV3	1042	598	0.08%	0.010%
11	3.150	653	656	658	rBV3	846	495	0.06%	0.008%
12	3.204	669	673	675	rBV5	1033	649	0.08%	0.011%
13	3.240	682	684	687	rBV3	1076	650	0.08%	0.011%
14	3.301	700	703	704	rVV3	1013	590	0.07%	0.010%
15	3.362	720	722	724	rVB3	1032	540	0.07%	0.009%
16	3.497	760	764	765	rBV3	944	611	0.08%	0.010%
17	3.506	765	767	770	rVV5	1019	685	0.09%	0.011%
18	3.545	774	779	781	rBV5	829	797	0.10%	0.013%
19	3.622	800	803	805	rVB3	1149	747	0.09%	0.012%
20	3.638	805	808	810	rBV3	1161	736	0.09%	0.012%
21	3.686	819	823	828	rBV8	1526	1457	0.18%	0.024%
22	3.786	843	854	881	rBV	59953	170539	21.42%	2.825%
23	4.104	951	953	955	rBV2	1313	550	0.07%	0.009%
24	4.249	981	998	1018	rBV	132355	341073	42.85%	5.650%
25	4.825	1175	1177	1181	rBV4	1307	708	0.09%	0.012%
26	4.957	1201	1218	1245	rBV3	292465	795984	100.00%	13.185%
27	5.413	1356	1360	1365	rBV8	1293	1232	0.15%	0.020%
28	5.442	1365	1369	1372	rBV5	1653	1378	0.17%	0.023%
29	5.535	1387	1398	1425	rBV	212041	444936	55.90%	7.370%
30	5.989	1527	1539	1560	rBV	180247	375863	47.22%	6.226%
31	6.214	1604	1609	1611	rBV5	1613	1688	0.21%	0.028%
32	6.284	1627	1631	1634	rBV5	1492	1214	0.15%	0.020%
33	6.378	1657	1660	1661	rBV3	1679	698	0.09%	0.012%
34	6.558	1714	1716	1719	rVB3	1098	679	0.09%	0.011%
35	6.741	1769	1773	1774	rBV4	1172	704	0.09%	0.012%
36	6.764	1778	1780	1783	rVB3	768	484	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033450.D
 Acq On : 18 Dec 2023 12:20
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.792	1786	1789	1790	rBV2	1141	576	0.07%	0.010%
38	6.915	1817	1827	1848	rVV	87282	168657	21.19%	2.794%
39	7.246	1919	1930	1950	rBV	305677	548514	68.91%	9.086%
40	7.554	2017	2026	2044	rBV	65737	118294	14.86%	1.959%
41	7.773	2091	2094	2095	rBV3	985	588	0.07%	0.010%
42	7.956	2148	2151	2152	rBV3	1213	734	0.09%	0.012%
43	8.024	2163	2172	2205	rBV	193129	396922	49.87%	6.575%
44	8.497	2314	2319	2322	rBV7	1569	1368	0.17%	0.023%
45	8.532	2328	2330	2333	rBV4	1247	597	0.08%	0.010%
46	8.641	2361	2364	2367	rBV3	680	530	0.07%	0.009%
47	8.786	2398	2409	2436	rBV	368987	612328	76.93%	10.143%
48	9.101	2502	2507	2513	rVB9	2380	2612	0.33%	0.043%
49	9.220	2540	2544	2546	rBV5	1069	893	0.11%	0.015%
50	9.416	2601	2605	2606	rBV4	1609	886	0.11%	0.015%
51	9.516	2633	2636	2637	rBV3	1395	756	0.09%	0.013%
52	9.545	2643	2645	2651	rBV6	962	781	0.10%	0.013%
53	9.632	2669	2672	2675	rVB3	1486	1139	0.14%	0.019%
54	9.693	2688	2691	2692	rBV3	1456	687	0.09%	0.011%
55	9.767	2710	2714	2718	rBV7	1502	1617	0.20%	0.027%
56	9.796	2721	2723	2725	rVB3	1020	516	0.06%	0.009%
57	10.053	2799	2803	2806	rBV5	1155	841	0.11%	0.014%
58	10.152	2820	2834	2856	rBV	283768	458240	57.57%	7.590%
59	10.252	2863	2865	2868	rVB4	1805	790	0.10%	0.013%
60	10.583	2964	2968	2971	rBV4	1386	1142	0.14%	0.019%
61	10.763	3022	3024	3028	rBV4	1048	707	0.09%	0.012%
62	10.943	3077	3080	3082	rBV4	928	733	0.09%	0.012%
63	10.992	3091	3095	3096	rBV3	932	733	0.09%	0.012%
64	11.107	3127	3131	3133	rBV4	1914	1638	0.21%	0.027%
65	11.136	3136	3140	3143	rBV4	1705	1168	0.15%	0.019%
66	11.188	3145	3156	3173	rBV	330106	516417	64.88%	8.554%
67	11.336	3198	3202	3205	rBV5	1262	940	0.12%	0.016%
68	11.397	3217	3221	3224	rBV6	1721	1510	0.19%	0.025%
69	11.493	3249	3251	3253	rVB3	1617	517	0.06%	0.009%
70	11.506	3253	3255	3258	rVB4	1169	510	0.06%	0.008%
71	11.561	3258	3272	3293	rBV	353691	582090	73.13%	9.642%
72	11.908	3378	3380	3385	rBV5	1301	1065	0.13%	0.018%
73	12.004	3409	3410	3415	rVB4	1527	743	0.09%	0.012%
74	12.091	3435	3437	3441	rBV5	1066	866	0.11%	0.014%
75	12.130	3447	3449	3454	rBV6	1438	741	0.09%	0.012%
76	12.149	3454	3455	3457	rBV2	983	490	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033450.D
 Acq On : 18 Dec 2023 12:20
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.233	3478	3481	3482	rBV3	910	521	0.07%	0.009%
78	12.258	3487	3489	3492	rBV3	1469	924	0.12%	0.015%
79	12.339	3511	3514	3519	rBV6	1528	1455	0.18%	0.024%
80	12.394	3528	3531	3532	rBV2	1314	625	0.08%	0.010%
81	12.429	3539	3542	3544	rBV3	1370	637	0.08%	0.011%
82	12.493	3560	3562	3565	rBV3	1255	824	0.10%	0.014%
83	12.641	3606	3608	3610	rBV2	1124	506	0.06%	0.008%
84	12.660	3610	3614	3615	rBV4	1167	581	0.07%	0.010%
85	12.721	3630	3633	3635	rBV4	1489	1174	0.15%	0.019%
86	12.908	3689	3691	3695	rVB5	1346	813	0.10%	0.013%
87	12.937	3695	3700	3702	rBV5	1269	776	0.10%	0.013%
88	12.963	3706	3708	3712	rBV4	1038	611	0.08%	0.010%
89	13.094	3747	3749	3753	rBV4	1224	833	0.10%	0.014%
90	13.117	3753	3756	3758	rVB2	1218	595	0.07%	0.010%
91	13.226	3788	3790	3793	rBV4	1124	539	0.07%	0.009%
92	13.442	3854	3857	3858	rBV2	1065	505	0.06%	0.008%
93	13.715	3937	3942	3943	rBV4	1028	747	0.09%	0.012%
94	13.725	3943	3945	3950	rVV5	1193	993	0.12%	0.016%
95	13.824	3975	3976	3981	rVV4	1027	747	0.09%	0.012%
96	14.056	4046	4048	4052	rVB4	911	484	0.06%	0.008%
97	14.528	4192	4195	4197	rBV3	1269	860	0.11%	0.014%
98	14.799	4276	4279	4281	rBV3	1216	663	0.08%	0.011%
99	14.930	4312	4320	4324	rBV6	2084	2894	0.36%	0.048%
100	15.239	4413	4416	4421	rBV6	1240	1084	0.14%	0.018%




Sum of corrected areas: 6037078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033450.D
Acq On : 18 Dec 2023 12:20
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

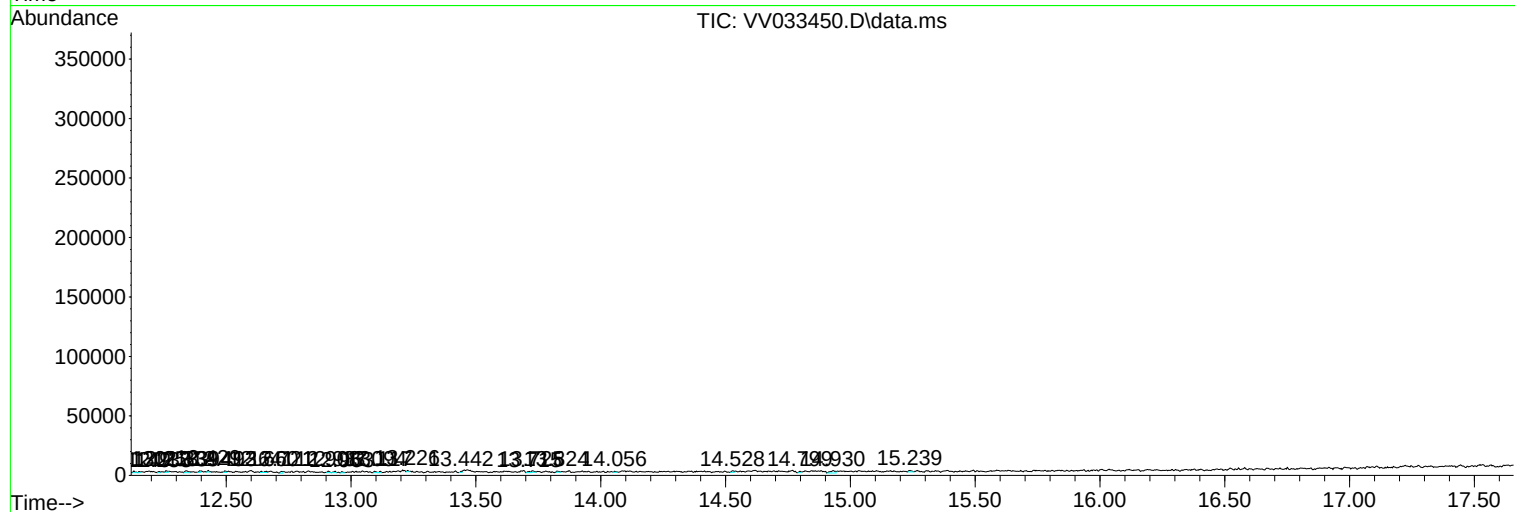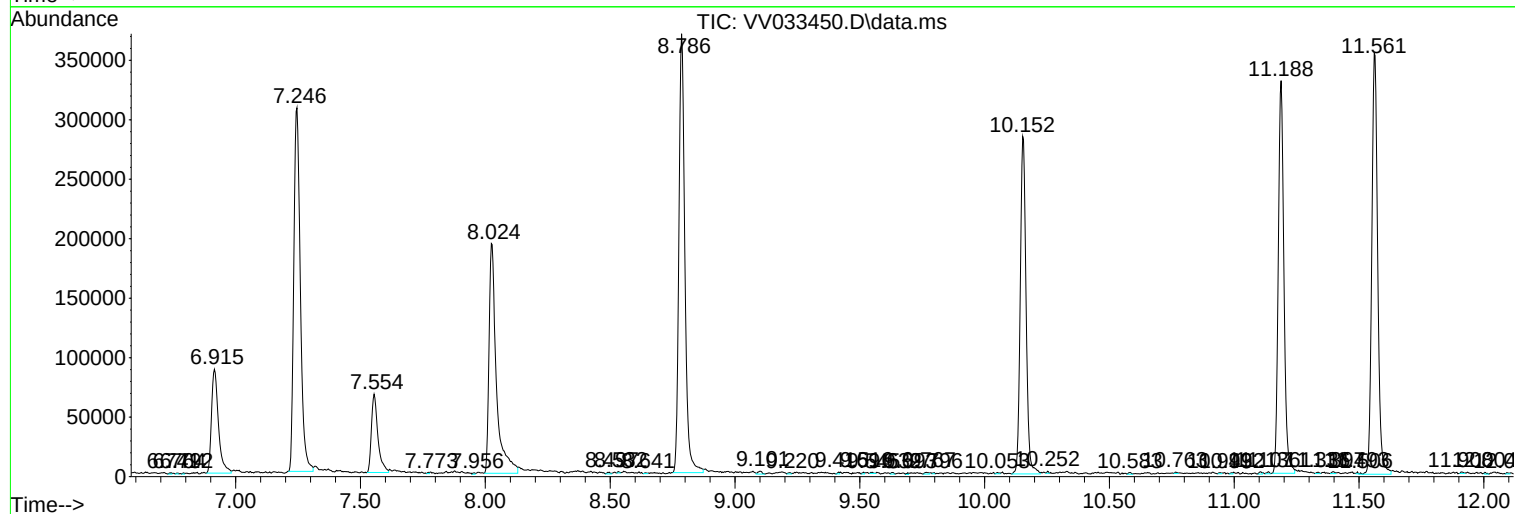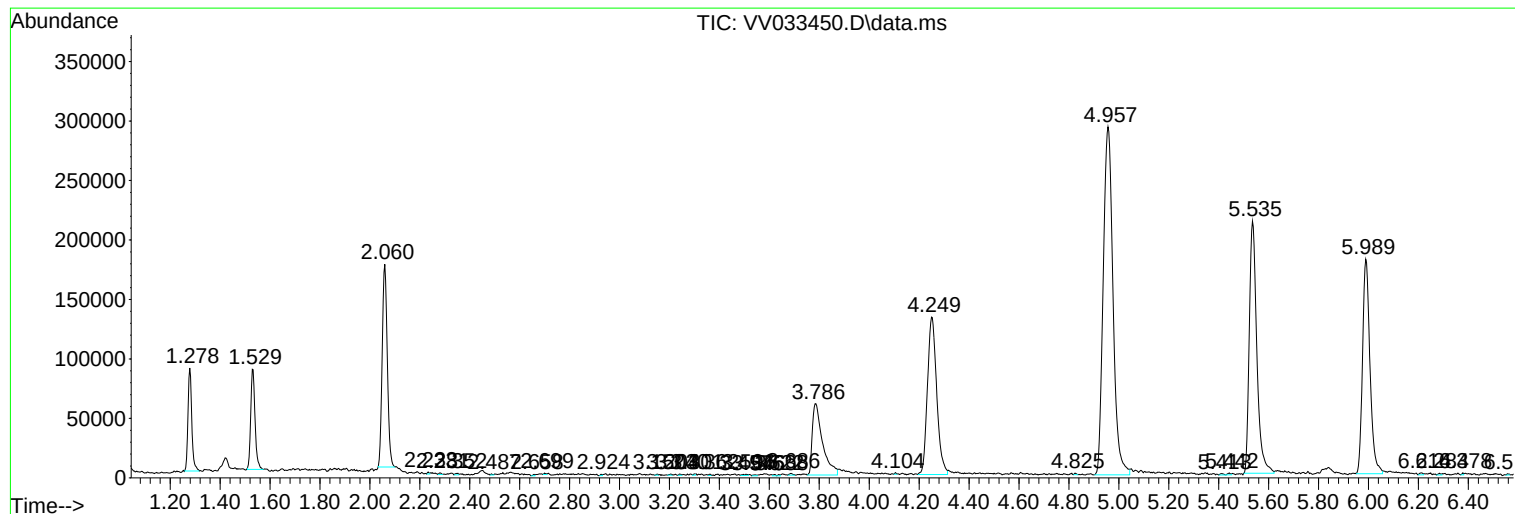

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033450.D
Acq On : 18 Dec 2023 12:20
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033450.D
Acq On : 18 Dec 2023 12:20
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------