

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033451.D
 Acq On : 18 Dec 2023 12:43
 Operator : SY/MD
 Sample : 05794-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	96831	100893	12.17%	1.575%
2	1.532	146	153	165	rVB	95714	116944	14.11%	1.825%
3	2.060	309	317	331	rVB	191714	275441	33.24%	4.299%
4	2.416	422	428	429	rBV6	1641	1500	0.18%	0.023%
5	2.535	461	465	468	rBV5	1681	1034	0.12%	0.016%
6	2.625	490	493	496	rVB5	890	647	0.08%	0.010%
7	2.751	530	532	533	rBV2	1660	705	0.09%	0.011%
8	2.841	558	560	564	rVB5	1281	881	0.11%	0.014%
9	2.870	564	569	574	rBV7	1502	1254	0.15%	0.020%
10	2.899	574	578	580	rVV4	1504	975	0.12%	0.015%
11	2.912	580	582	587	rVB6	1160	733	0.09%	0.011%
12	2.957	594	596	598	rBV3	1322	742	0.09%	0.012%
13	3.056	625	627	629	rBV3	1338	602	0.07%	0.009%
14	3.085	633	636	641	rVB6	1212	1162	0.14%	0.018%
15	3.124	645	648	653	rBV6	894	902	0.11%	0.014%
16	3.188	666	668	672	rBV3	1152	902	0.11%	0.014%
17	3.217	672	677	680	rVV6	1117	1060	0.13%	0.017%
18	3.272	691	694	696	rBV3	1105	643	0.08%	0.010%
19	3.310	700	706	708	rBV7	1101	1148	0.14%	0.018%
20	3.326	708	711	714	rVB5	1276	918	0.11%	0.014%
21	3.400	730	734	735	rBV3	1161	880	0.11%	0.014%
22	3.561	781	784	788	rBV4	1380	913	0.11%	0.014%
23	3.667	815	817	819	rBV3	1083	767	0.09%	0.012%
24	3.725	833	835	837	rBV2	1068	620	0.07%	0.010%
25	3.786	844	854	880	rBV	58263	160845	19.41%	2.511%
26	4.249	986	998	1021	rVB	136148	342508	41.33%	5.346%
27	4.568	1095	1097	1102	rVB5	1581	988	0.12%	0.015%
28	4.706	1137	1140	1141	rBV3	1023	587	0.07%	0.009%
29	4.773	1159	1161	1163	rBV2	1281	646	0.08%	0.010%
30	4.957	1201	1218	1242	rBV2	308486	828718	100.00%	12.935%
31	5.326	1329	1333	1335	rBV5	1708	1553	0.19%	0.024%
32	5.484	1380	1382	1383	rBV2	1728	765	0.09%	0.012%
33	5.535	1387	1398	1419	rVV	247033	512618	61.86%	8.001%
34	5.989	1528	1539	1564	rBV	184774	384154	46.36%	5.996%
35	6.455	1680	1684	1689	rBV7	1168	1206	0.15%	0.019%
36	6.532	1705	1708	1712	rVB5	1211	681	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033451.D
 Acq On : 18 Dec 2023 12:43
 Operator : SY/MD
 Sample : 05794-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.567	1716	1719	1723	rVB6	1166	1069	0.13%	0.017%
38	6.616	1731	1734	1736	rBV3	1130	819	0.10%	0.013%
39	6.767	1779	1781	1785	rBV5	1105	670	0.08%	0.010%
40	6.844	1802	1805	1806	rBV3	1269	688	0.08%	0.011%
41	6.915	1815	1827	1847	rBV	88489	172667	20.84%	2.695%
42	7.095	1881	1883	1885	rBV3	1363	828	0.10%	0.013%
43	7.140	1895	1897	1899	rBV3	1058	642	0.08%	0.010%
44	7.246	1918	1930	1952	rBV	331119	598243	72.19%	9.338%
45	7.500	2006	2009	2011	rBV4	1749	1267	0.15%	0.020%
46	7.555	2017	2026	2044	rBV	65449	119873	14.46%	1.871%
47	7.821	2106	2109	2112	rBV4	1250	932	0.11%	0.015%
48	7.850	2116	2118	2123	rVV5	1572	1089	0.13%	0.017%
49	7.902	2130	2134	2136	rVB5	1078	703	0.08%	0.011%
50	7.953	2147	2150	2152	rBV4	1610	1000	0.12%	0.016%
51	8.027	2163	2173	2207	rBV	188992	389229	46.97%	6.075%
52	8.786	2398	2409	2426	rBV	411827	679237	81.96%	10.602%
53	9.098	2504	2506	2508	rBV3	1268	602	0.07%	0.009%
54	9.178	2528	2531	2534	rBV4	1662	1367	0.16%	0.021%
55	9.320	2573	2575	2578	rBV3	1097	651	0.08%	0.010%
56	9.381	2592	2594	2599	rVB4	1587	992	0.12%	0.015%
57	9.407	2599	2602	2605	rBV4	937	771	0.09%	0.012%
58	9.455	2614	2617	2619	rBV3	1180	859	0.10%	0.013%
59	9.606	2660	2664	2665	rBV4	2224	1228	0.15%	0.019%
60	9.657	2678	2680	2683	rVB3	1395	673	0.08%	0.011%
61	9.718	2696	2699	2701	rBV3	1269	668	0.08%	0.010%
62	9.789	2718	2721	2724	rBV5	1646	1119	0.14%	0.017%
63	9.882	2746	2750	2752	rBV4	1142	800	0.10%	0.012%
64	10.072	2807	2809	2815	rBV7	1079	1161	0.14%	0.018%
65	10.153	2824	2834	2852	rBV	276442	441560	53.28%	6.892%
66	10.297	2877	2879	2882	rVB3	1129	632	0.08%	0.010%
67	10.487	2934	2938	2940	rBV5	1383	1143	0.14%	0.018%
68	10.513	2944	2946	2949	rVB3	1910	1162	0.14%	0.018%
69	10.532	2949	2952	2957	rBV4	1566	1195	0.14%	0.019%
70	10.609	2972	2976	2980	rVB5	1790	1286	0.16%	0.020%
71	10.635	2980	2984	2986	rBV5	1071	874	0.11%	0.014%
72	10.657	2989	2991	2994	rVB3	1388	683	0.08%	0.011%
73	11.008	3098	3100	3105	rBV4	1829	1762	0.21%	0.028%
74	11.053	3112	3114	3117	rBV3	1002	628	0.08%	0.010%
75	11.082	3120	3123	3124	rBV3	1084	664	0.08%	0.010%
76	11.140	3139	3141	3144	rVB4	1231	613	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033451.D
 Acq On : 18 Dec 2023 12:43
 Operator : SY/MD
 Sample : 05794-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	11.188	3144	3156	3176	rBV	384357	599131	72.30%	9.352%
78	11.464	3241	3242	3245	rBV3	1018	647	0.08%	0.010%
79	11.561	3262	3272	3290	rBV	390633	606973	73.24%	9.474%
80	11.734	3324	3326	3331	rBV5	1444	767	0.09%	0.012%
81	11.789	3339	3343	3345	rBV4	1364	977	0.12%	0.015%
82	12.294	3498	3500	3506	rVB7	1438	1122	0.14%	0.018%
83	12.323	3506	3509	3515	rVB7	1389	1488	0.18%	0.023%
84	12.355	3515	3519	3522	rBV5	1078	916	0.11%	0.014%
85	12.477	3555	3557	3560	rBV4	1194	734	0.09%	0.011%
86	12.596	3589	3594	3599	rBV8	2254	2923	0.35%	0.046%
87	12.712	3627	3630	3635	rBV4	1389	1462	0.18%	0.023%
88	12.773	3647	3649	3651	rBV3	1091	597	0.07%	0.009%
89	12.905	3687	3690	3694	rBV5	1163	685	0.08%	0.011%
90	13.387	3837	3840	3843	rBV5	869	599	0.07%	0.009%
91	13.966	4018	4020	4023	rBV4	1196	697	0.08%	0.011%
92	13.982	4023	4025	4029	rVV3	1514	1061	0.13%	0.017%
93	14.066	4049	4051	4054	rBV3	1123	638	0.08%	0.010%
94	14.217	4096	4098	4101	rBV4	1014	586	0.07%	0.009%
95	14.281	4116	4118	4121	rBV3	1375	597	0.07%	0.009%
96	14.699	4245	4248	4250	rBV4	1117	691	0.08%	0.011%
97	15.091	4366	4370	4373	rBV6	1213	1036	0.13%	0.016%
98	15.152	4385	4389	4391	rVV4	1131	932	0.11%	0.015%
99	15.336	4443	4446	4449	rBV5	1196	1039	0.13%	0.016%
100	15.413	4466	4470	4471	rBV2	1193	716	0.09%	0.011%




Sum of corrected areas: 6406598

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033451.D
Acq On : 18 Dec 2023 12:43
Operator : SY/MD
Sample : 05794-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

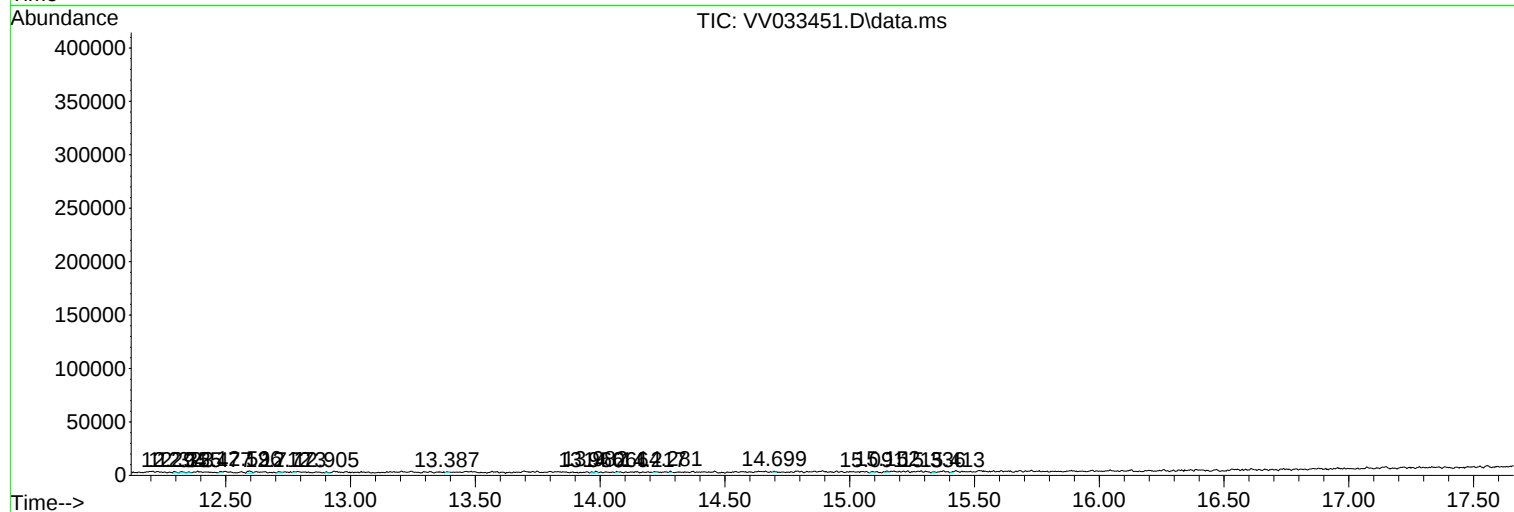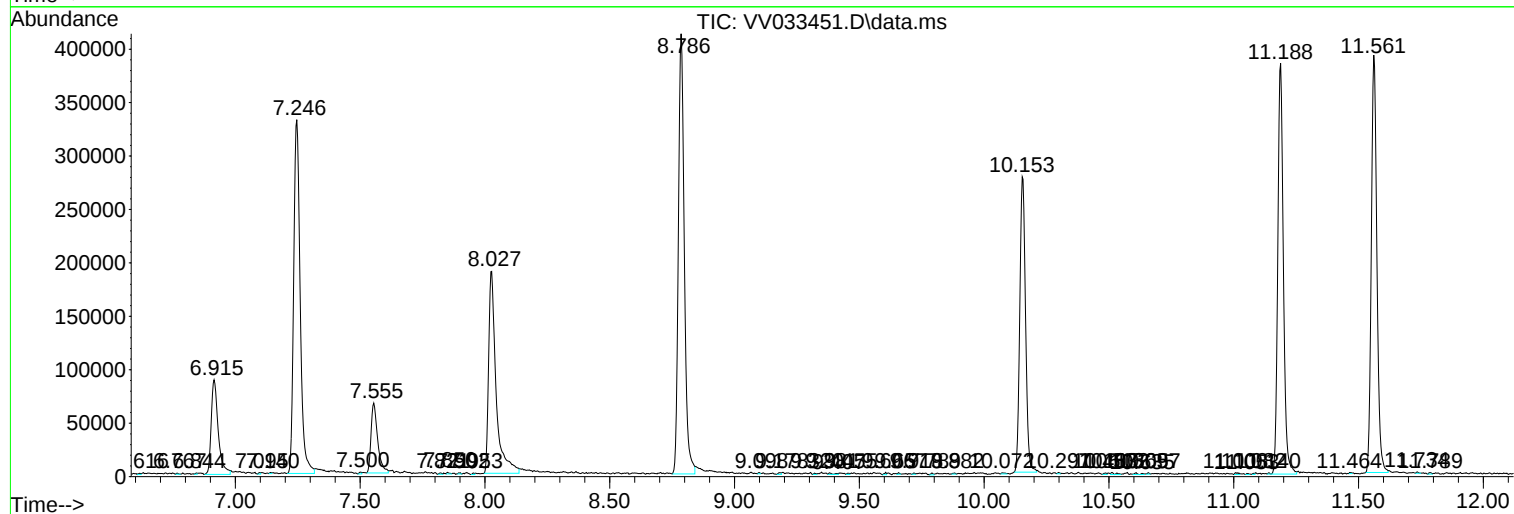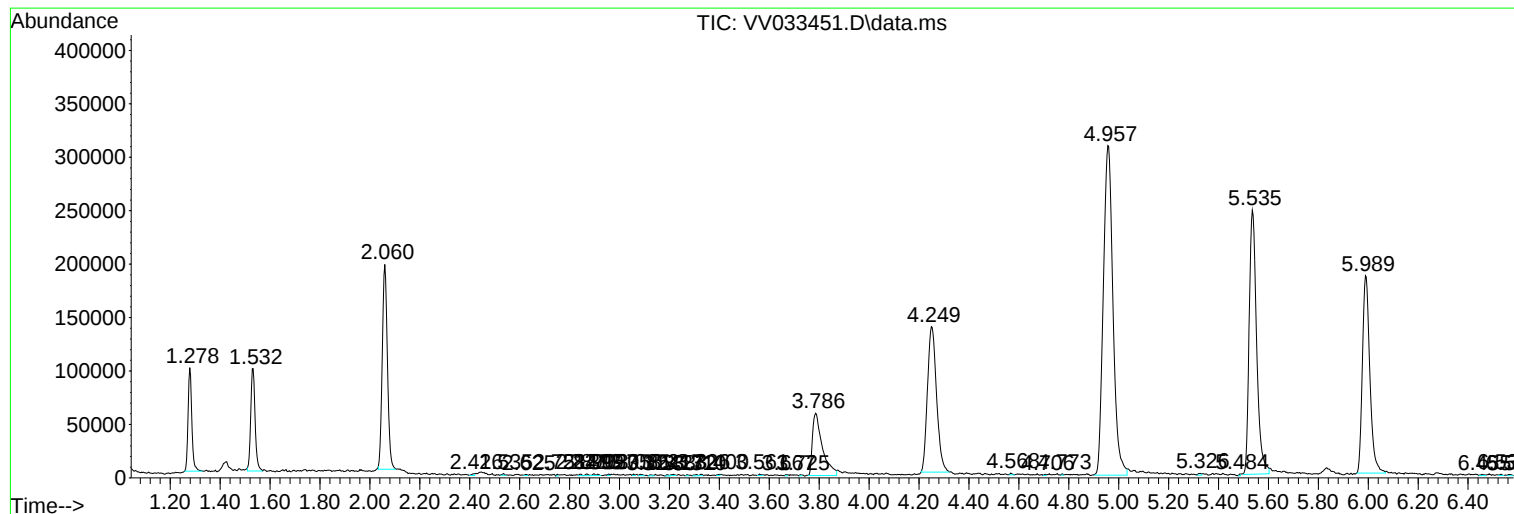

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033451.D
Acq On : 18 Dec 2023 12:43
Operator : SY/MD
Sample : 05794-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033451.D
Acq On : 18 Dec 2023 12:43
Operator : SY/MD
Sample : 05794-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc