

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033452.D
 Acq On : 18 Dec 2023 13:06
 Operator : SY/MD
 Sample : 05794-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	100586	103615	12.42%	1.613%
2	1.532	146	153	169	rVB	96846	115354	13.83%	1.796%
3	2.060	308	317	328	rBV	194125	279569	33.51%	4.353%
4	2.449	432	438	443	rVB10	1639	2264	0.27%	0.035%
5	2.661	500	504	506	rBV5	1969	1344	0.16%	0.021%
6	2.712	518	520	523	rBV4	1069	769	0.09%	0.012%
7	2.764	532	536	538	rBV4	841	625	0.07%	0.010%
8	2.780	539	541	545	rVV4	939	670	0.08%	0.010%
9	2.979	600	603	605	rBV3	1253	848	0.10%	0.013%
10	3.246	681	686	688	rBV5	1710	1222	0.15%	0.019%
11	3.349	716	718	722	rVB2	841	598	0.07%	0.009%
12	3.368	722	724	727	rBV5	1021	611	0.07%	0.010%
13	3.384	727	729	734	rVV6	800	599	0.07%	0.009%
14	3.410	734	737	740	rVV5	1158	866	0.10%	0.013%
15	3.445	745	748	753	rVB5	1139	853	0.10%	0.013%
16	3.474	753	757	759	rBV5	966	861	0.10%	0.013%
17	3.487	759	761	766	rVB6	1166	845	0.10%	0.013%
18	3.513	766	769	775	rVB5	1295	1161	0.14%	0.018%
19	3.539	775	777	780	rBV4	1168	754	0.09%	0.012%
20	3.577	785	789	792	rBV6	898	692	0.08%	0.011%
21	3.619	800	802	806	rBV5	988	731	0.09%	0.011%
22	3.716	829	832	834	rBV4	1136	722	0.09%	0.011%
23	3.786	845	854	884	rVV	56883	156798	18.80%	2.441%
24	4.095	947	950	955	rBV6	1628	1169	0.14%	0.018%
25	4.169	970	973	975	rBV4	1334	627	0.08%	0.010%
26	4.249	985	998	1025	rVB	139342	357340	42.84%	5.564%
27	4.436	1054	1056	1057	rBV2	1369	707	0.08%	0.011%
28	4.777	1158	1162	1165	rVB4	1029	812	0.10%	0.013%
29	4.809	1170	1172	1174	rBV2	1052	611	0.07%	0.010%
30	4.957	1202	1218	1245	rBV2	309986	834184	100.00%	12.988%
31	5.256	1309	1311	1313	rBV3	1991	973	0.12%	0.015%
32	5.535	1386	1398	1427	rBV	243982	519026	62.22%	8.081%
33	5.989	1528	1539	1560	rBV	191288	384786	46.13%	5.991%
34	6.172	1595	1596	1599	rBV3	1348	696	0.08%	0.011%
35	6.359	1651	1654	1656	rBV4	1026	673	0.08%	0.010%
36	6.510	1697	1701	1703	rBV5	1796	1211	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033452.D
 Acq On : 18 Dec 2023 13:06
 Operator : SY/MD
 Sample : 05794-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.580	1721	1723	1725	rBV3	1270	809	0.10%	0.013%
38	6.709	1761	1763	1767	rVB4	1795	1184	0.14%	0.018%
39	6.735	1767	1771	1773	rBV4	1135	658	0.08%	0.010%
40	6.860	1806	1810	1813	rBV5	1006	775	0.09%	0.012%
41	6.915	1816	1827	1844	rBV	90041	172241	20.65%	2.682%
42	7.246	1918	1930	1952	rBV	338631	609750	73.10%	9.493%
43	7.555	2017	2026	2043	rBV	66870	121427	14.56%	1.891%
44	8.027	2163	2173	2192	rBV	188165	365440	43.81%	5.690%
45	8.365	2275	2278	2279	rBV3	1991	1266	0.15%	0.020%
46	8.490	2313	2317	2320	rBV5	1327	1016	0.12%	0.016%
47	8.545	2331	2334	2337	rBV5	1481	1046	0.13%	0.016%
48	8.680	2373	2376	2380	rBV4	864	716	0.09%	0.011%
49	8.735	2389	2393	2394	rBV4	1434	771	0.09%	0.012%
50	8.786	2398	2409	2435	rVV	414739	684813	82.09%	10.662%
51	9.037	2484	2487	2490	rBV4	1509	908	0.11%	0.014%
52	9.075	2494	2499	2502	rBV5	1532	1720	0.21%	0.027%
53	9.391	2594	2597	2600	rVB5	1439	1146	0.14%	0.018%
54	9.426	2605	2608	2611	rBV5	994	798	0.10%	0.012%
55	9.484	2621	2626	2627	rBV4	1649	865	0.10%	0.013%
56	9.577	2653	2655	2660	rVV5	957	595	0.07%	0.009%
57	9.815	2725	2729	2731	rBV3	778	631	0.08%	0.010%
58	9.989	2780	2783	2784	rBV4	1204	626	0.08%	0.010%
59	10.066	2805	2807	2809	rVV3	1191	584	0.07%	0.009%
60	10.153	2821	2834	2851	rBV	281014	453133	54.32%	7.055%
61	10.452	2925	2927	2929	rBV3	1125	659	0.08%	0.010%
62	10.571	2960	2964	2965	rBV4	1040	697	0.08%	0.011%
63	10.609	2973	2976	2978	rBV4	1737	920	0.11%	0.014%
64	10.641	2983	2986	2988	rBV3	1348	870	0.10%	0.014%
65	10.706	3005	3006	3010	rVB5	1236	589	0.07%	0.009%
66	10.834	3042	3046	3049	rBV4	1313	1043	0.13%	0.016%
67	10.905	3066	3068	3073	rBV5	1106	665	0.08%	0.010%
68	11.005	3095	3099	3102	rBV5	1242	924	0.11%	0.014%
69	11.059	3111	3116	3118	rBV6	1101	884	0.11%	0.014%
70	11.101	3125	3129	3131	rBV4	920	725	0.09%	0.011%
71	11.188	3144	3156	3172	rBV	366881	582120	69.78%	9.063%
72	11.371	3210	3213	3214	rBV3	1131	685	0.08%	0.011%
73	11.561	3262	3272	3292	rBV2	379026	606313	72.68%	9.440%
74	11.850	3358	3362	3365	rBV6	1932	1541	0.18%	0.024%
75	11.944	3388	3391	3397	rBV8	1111	952	0.11%	0.015%
76	12.349	3515	3517	3521	rVB4	1451	904	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033452.D
 Acq On : 18 Dec 2023 13:06
 Operator : SY/MD
 Sample : 05794-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.484	3556	3559	3560	rBV3	995	582	0.07%	0.009%
78	12.664	3611	3615	3619	rBV5	816	803	0.10%	0.013%
79	12.715	3629	3631	3633	rVB3	1278	616	0.07%	0.010%
80	12.734	3633	3637	3643	rBV6	1485	1644	0.20%	0.026%
81	12.972	3706	3711	3713	rVB5	1016	718	0.09%	0.011%
82	13.091	3746	3748	3751	rBV3	1191	787	0.09%	0.012%
83	13.159	3767	3769	3774	rBV5	879	837	0.10%	0.013%
84	13.297	3810	3812	3816	rBV5	1198	725	0.09%	0.011%
85	13.403	3842	3845	3846	rBV3	1006	634	0.08%	0.010%
86	13.458	3854	3862	3867	rBV10	2758	4080	0.49%	0.064%
87	13.538	3885	3887	3891	rBV4	1089	660	0.08%	0.010%
88	13.564	3893	3895	3899	rVB5	1106	664	0.08%	0.010%
89	13.844	3981	3982	3987	rVB5	1079	624	0.07%	0.010%
90	13.972	4020	4022	4025	rVV4	1169	690	0.08%	0.011%
91	14.001	4025	4031	4034	rVB6	1245	1112	0.13%	0.017%
92	14.021	4034	4037	4040	rBV4	1048	755	0.09%	0.012%
93	14.040	4041	4043	4047	rVB5	2036	1152	0.14%	0.018%
94	14.069	4047	4052	4053	rBV4	1103	825	0.10%	0.013%
95	14.374	4142	4147	4150	rVB6	1090	1129	0.14%	0.018%
96	14.400	4150	4155	4158	rBV5	1449	1401	0.17%	0.022%
97	14.468	4172	4176	4179	rBV5	1713	897	0.11%	0.014%
98	14.487	4179	4182	4184	rBV4	963	578	0.07%	0.009%
99	15.046	4353	4356	4360	rBV5	1239	1025	0.12%	0.016%
100	16.056	4668	4670	4672	rBV2	2216	1307	0.16%	0.020%




Sum of corrected areas: 6422840

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033452.D
Acq On : 18 Dec 2023 13:06
Operator : SY/MD
Sample : 05794-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

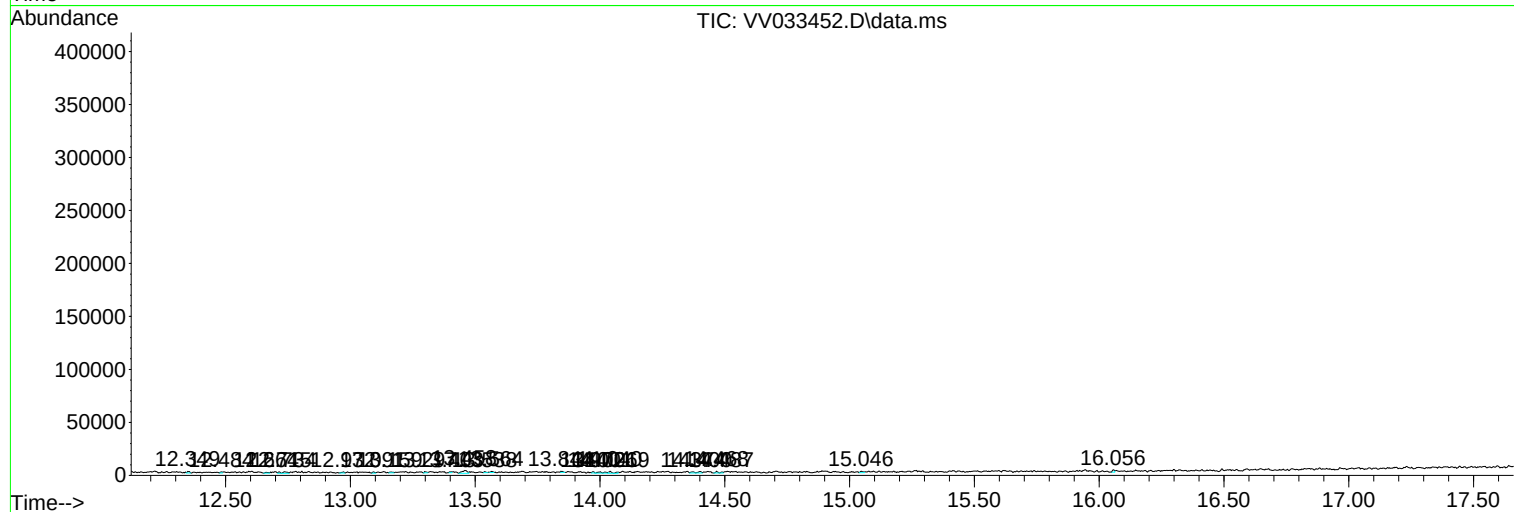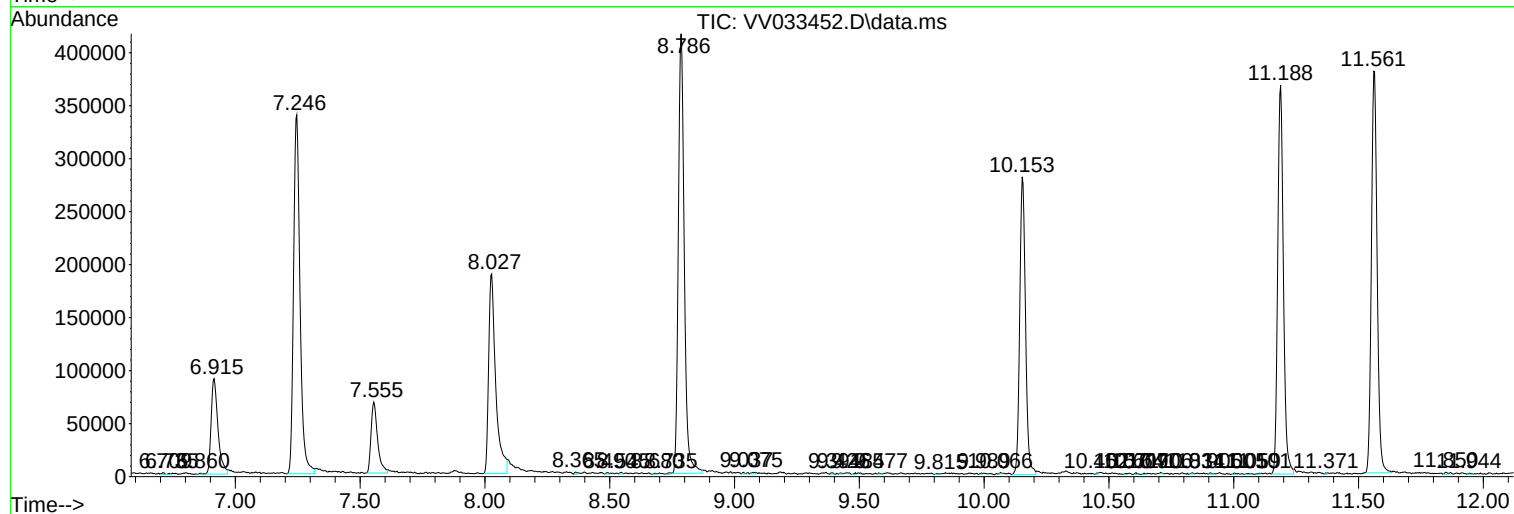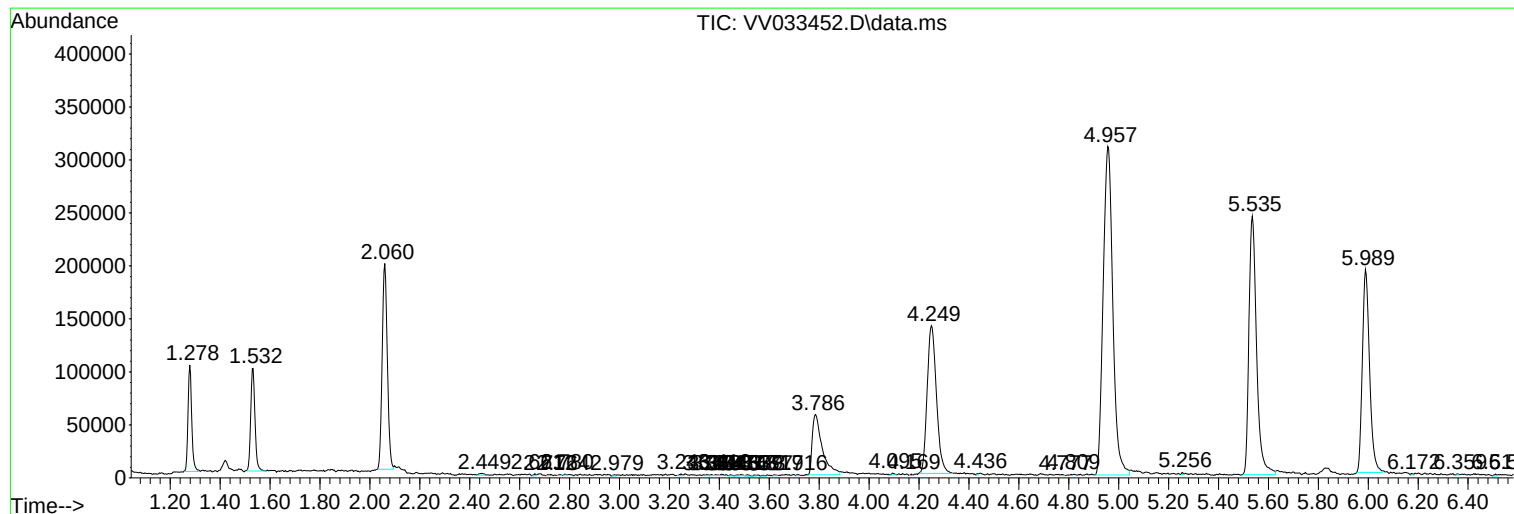

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033452.D
Acq On : 18 Dec 2023 13:06
Operator : SY/MD
Sample : 05794-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033452.D
Acq On : 18 Dec 2023 13:06
Operator : SY/MD
Sample : 05794-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc