

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
 Data File : VV033453.D
 Acq On : 18 Dec 2023 13:30
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	92880	97119	12.23%	1.576%
2	1.529	146	152	163	rBV	91334	108737	13.69%	1.764%
3	2.059	308	317	329	rBV	187050	266716	33.58%	4.327%
4	2.416	424	428	432	rBV6	1446	1365	0.17%	0.022%
5	2.445	432	437	439	rBV5	1906	1509	0.19%	0.024%
6	2.494	451	452	455	rVB3	1356	524	0.07%	0.009%
7	2.510	455	457	460	rBV4	1262	865	0.11%	0.014%
8	2.593	480	483	484	rBV4	1607	698	0.09%	0.011%
9	2.648	499	500	504	rVB4	1253	719	0.09%	0.012%
10	2.670	504	507	508	rBV2	1095	655	0.08%	0.011%
11	2.719	520	522	526	rVB4	1536	702	0.09%	0.011%
12	2.764	531	536	538	rBV5	1220	1080	0.14%	0.018%
13	2.776	538	540	542	rBV2	1185	653	0.08%	0.011%
14	2.831	553	557	559	rBV3	959	717	0.09%	0.012%
15	2.963	595	598	602	rVB5	1110	560	0.07%	0.009%
16	2.998	607	609	613	rVB4	1636	898	0.11%	0.015%
17	3.034	616	620	622	rBV4	895	658	0.08%	0.011%
18	3.117	642	646	647	rBV3	1005	514	0.06%	0.008%
19	3.249	684	687	690	rVB3	1286	918	0.12%	0.015%
20	3.265	690	692	694	rBV3	1021	554	0.07%	0.009%
21	3.281	694	697	698	rBV2	906	570	0.07%	0.009%
22	3.342	715	716	719	rVV3	985	593	0.07%	0.010%
23	3.358	719	721	725	rVV3	1679	763	0.10%	0.012%
24	3.413	736	738	741	rVB3	1462	766	0.10%	0.012%
25	3.445	741	748	751	rBV7	1055	1201	0.15%	0.019%
26	3.468	751	755	756	rBV3	1125	845	0.11%	0.014%
27	3.596	793	795	798	rBV4	1027	699	0.09%	0.011%
28	3.641	807	809	811	rVB3	1661	657	0.08%	0.011%
29	3.786	844	854	874	rBV	56347	151121	19.03%	2.452%
30	4.249	985	998	1026	rBV	134653	342655	43.15%	5.559%
31	4.378	1035	1038	1043	rBV7	1376	1288	0.16%	0.021%
32	4.490	1071	1073	1075	rBV2	1470	675	0.08%	0.011%
33	4.635	1116	1118	1121	rBV4	1289	815	0.10%	0.013%
34	4.686	1128	1134	1137	rBV7	1137	1024	0.13%	0.017%
35	4.847	1178	1184	1186	rBV4	1105	928	0.12%	0.015%
36	4.956	1203	1218	1247	rBV3	296531	794170	100.00%	12.885%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033453.D
 Acq On : 18 Dec 2023 13:30
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	5.317	1327	1330	1332	rVB5	1115	680	0.09%	0.011%
38	5.365	1343	1345	1348	rBV3	1127	524	0.07%	0.009%
39	5.535	1387	1398	1424	rBV	230500	479510	60.38%	7.780%
40	5.989	1527	1539	1562	rBV	182325	379162	47.74%	6.152%
41	6.268	1623	1626	1630	rBV6	1715	1114	0.14%	0.018%
42	6.419	1669	1673	1677	rBV6	1623	1681	0.21%	0.027%
43	6.474	1688	1690	1695	rVB5	1360	863	0.11%	0.014%
44	6.500	1695	1698	1700	rBV3	929	583	0.07%	0.009%
45	6.577	1718	1722	1725	rBV6	1138	879	0.11%	0.014%
46	6.706	1760	1762	1764	rVB3	1215	516	0.06%	0.008%
47	6.825	1796	1799	1802	rBV4	1147	794	0.10%	0.013%
48	6.915	1817	1827	1851	rBV2	87895	166912	21.02%	2.708%
49	7.095	1881	1883	1887	rBV5	1042	712	0.09%	0.012%
50	7.246	1919	1930	1955	rBV	319279	579825	73.01%	9.407%
51	7.554	2018	2026	2046	rBV2	64109	116872	14.72%	1.896%
52	7.796	2099	2101	2104	rBV4	970	631	0.08%	0.010%
53	8.027	2163	2173	2201	rBV	188406	376191	47.37%	6.104%
54	8.545	2330	2334	2335	rBV2	1672	1047	0.13%	0.017%
55	8.590	2347	2348	2352	rVB3	1237	527	0.07%	0.009%
56	8.673	2372	2374	2377	rBV4	1170	617	0.08%	0.010%
57	8.718	2386	2388	2390	rBV2	1061	527	0.07%	0.009%
58	8.786	2397	2409	2430	rBV	395591	652033	82.10%	10.579%
59	9.175	2528	2530	2534	rBV4	1007	783	0.10%	0.013%
60	9.387	2594	2596	2599	rBV4	1274	783	0.10%	0.013%
61	9.535	2638	2642	2645	rBV5	1310	1199	0.15%	0.019%
62	9.586	2654	2658	2659	rBV3	1196	860	0.11%	0.014%
63	9.641	2673	2675	2678	rBV3	1315	815	0.10%	0.013%
64	9.934	2764	2766	2768	rBV3	1084	622	0.08%	0.010%
65	9.950	2770	2771	2774	rVB3	1461	636	0.08%	0.010%
66	9.982	2774	2781	2782	rBV6	1467	1382	0.17%	0.022%
67	10.152	2820	2834	2856	rBV	271945	444308	55.95%	7.209%
68	10.326	2881	2888	2892	rBV9	2799	3728	0.47%	0.060%
69	10.400	2908	2911	2912	rBV	1095	542	0.07%	0.009%
70	10.474	2930	2934	2939	rBV8	1445	1218	0.15%	0.020%
71	10.609	2975	2976	2981	rVB4	899	554	0.07%	0.009%
72	10.747	3017	3019	3026	rVB6	1378	1159	0.15%	0.019%
73	10.792	3029	3033	3036	rBV4	1098	1012	0.13%	0.016%
74	10.863	3053	3055	3058	rVB4	1370	692	0.09%	0.011%
75	10.898	3064	3066	3069	rBV3	1246	926	0.12%	0.015%
76	10.937	3076	3078	3081	rBV4	1129	730	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121823\
 Data File : VW033453.D
 Acq On : 18 Dec 2023 13:30
 Operator : SY/MD
 Sample : 05802-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	11.104	3128	3130	3132	rBV3	1489	894	0.11%	0.015%
78	11.188	3145	3156	3173	rBV	352218	554181	69.78%	8.991%
79	11.564	3261	3273	3289	rBV	357769	579083	72.92%	9.395%
80	11.712	3315	3319	3321	rBV5	1447	939	0.12%	0.015%
81	11.815	3347	3351	3355	rBV6	1536	1468	0.18%	0.024%
82	12.123	3445	3447	3452	rVB5	1396	985	0.12%	0.016%
83	12.670	3613	3617	3621	rVB5	946	738	0.09%	0.012%
84	12.734	3636	3637	3640	rVB3	1102	602	0.08%	0.010%
85	12.911	3690	3692	3695	rVB4	1469	748	0.09%	0.012%
86	13.300	3811	3813	3816	rBV4	1222	674	0.08%	0.011%
87	13.503	3873	3876	3881	rVB4	1841	1558	0.20%	0.025%
88	13.583	3894	3901	3906	rBV8	1215	1679	0.21%	0.027%
89	13.773	3957	3960	3962	rBV4	906	518	0.07%	0.008%
90	13.802	3967	3969	3973	rBV5	889	625	0.08%	0.010%
91	14.278	4115	4117	4123	rVB7	1302	1104	0.14%	0.018%
92	14.307	4124	4126	4130	rVB4	1609	806	0.10%	0.013%
93	14.329	4130	4133	4136	rBV5	1099	764	0.10%	0.012%
94	14.493	4181	4184	4185	rBV3	943	652	0.08%	0.011%
95	14.850	4290	4295	4299	rBV8	2236	2348	0.30%	0.038%
96	15.165	4391	4393	4396	rBV4	904	590	0.07%	0.010%
97	15.188	4396	4400	4401	rBV3	1041	834	0.11%	0.014%
98	15.258	4420	4422	4424	rBV3	1345	508	0.06%	0.008%
99	15.358	4450	4453	4456	rBV3	1719	1211	0.15%	0.020%
100	15.580	4519	4522	4524	rBV5	1457	908	0.11%	0.015%




Sum of corrected areas: 6163497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033453.D
Acq On : 18 Dec 2023 13:30
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

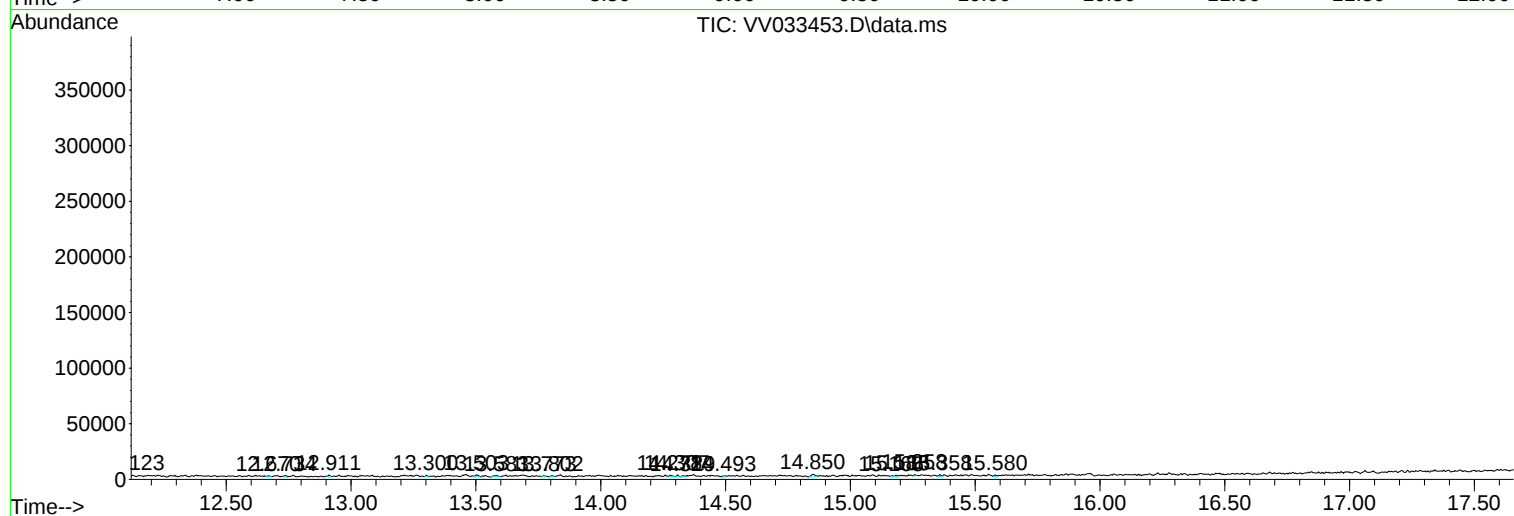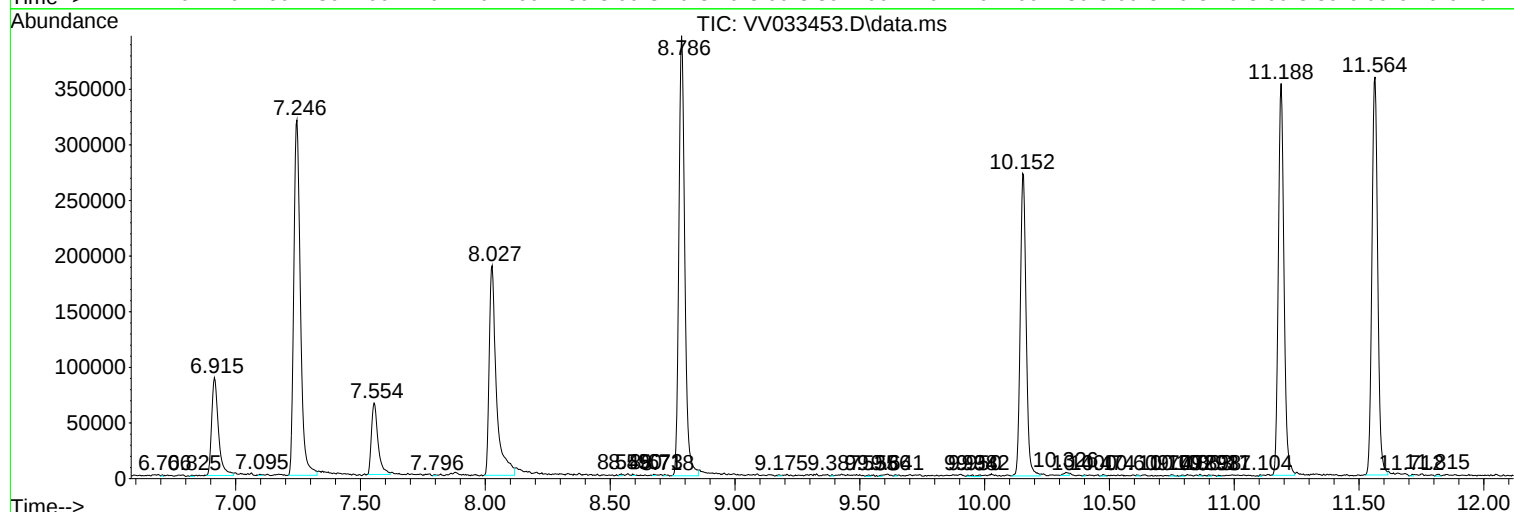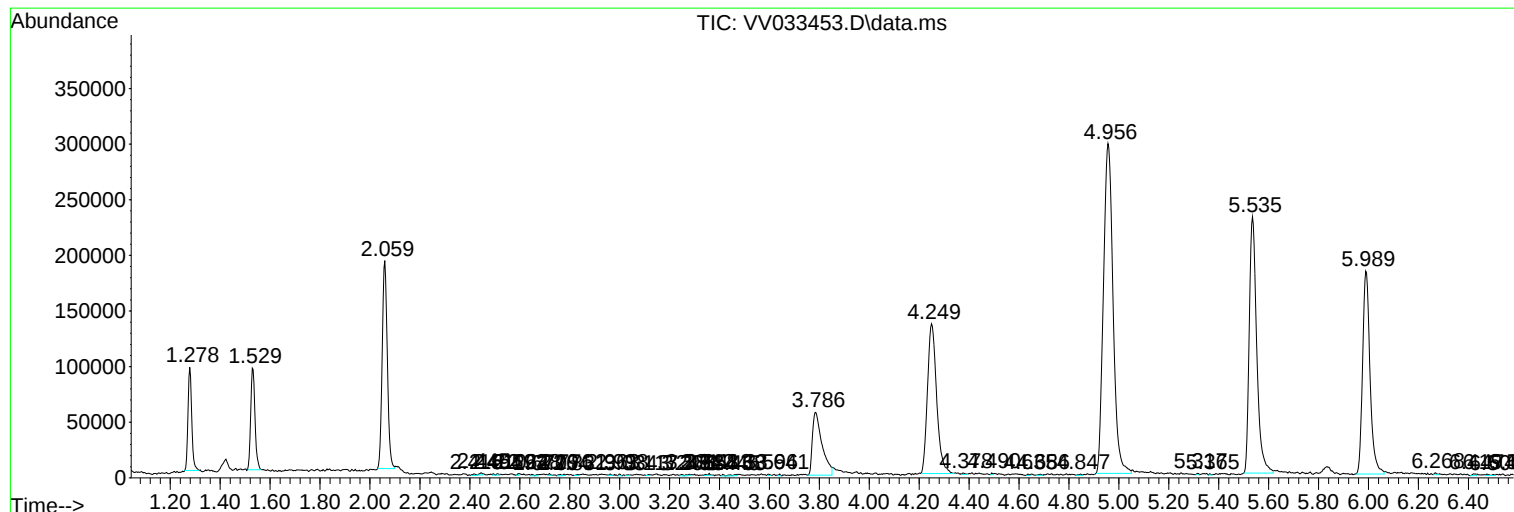

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033453.D
Acq On : 18 Dec 2023 13:30
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033453.D
Acq On : 18 Dec 2023 13:30
Operator : SY/MD
Sample : 05802-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------