
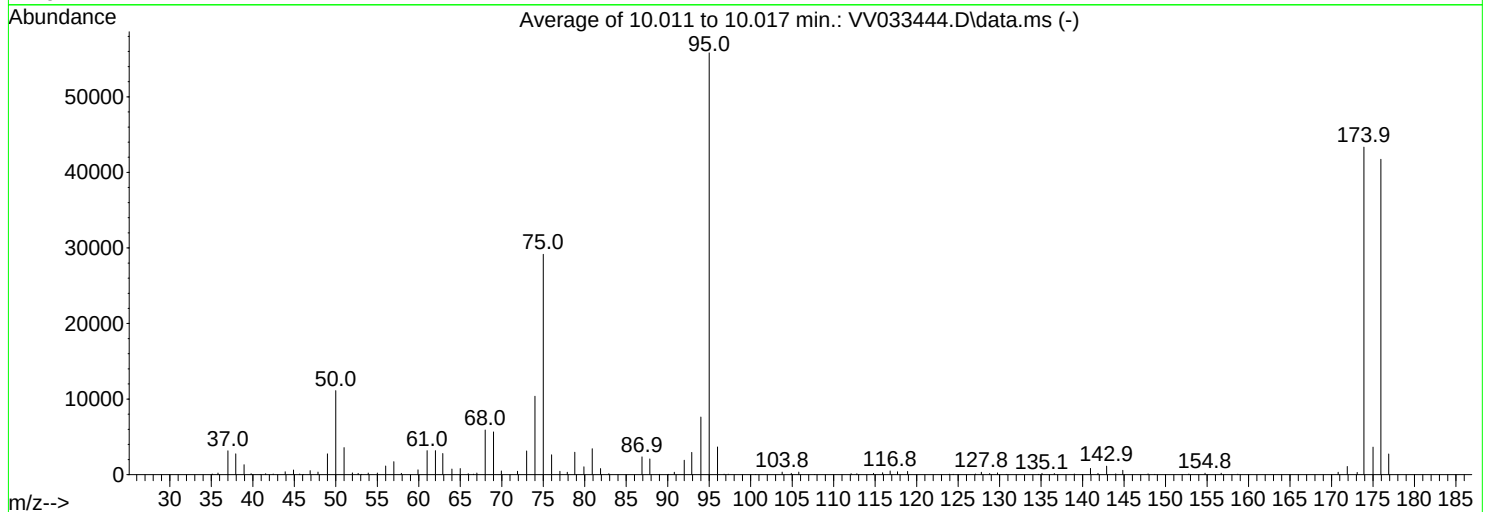


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121823\
Data File : VV033444.D
Acq On : 18 Dec 2023 08:53
Operator : SY/MD
Sample : BFB248
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB248

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis
Last Update : Wed Dec 20 00:24:21 2023

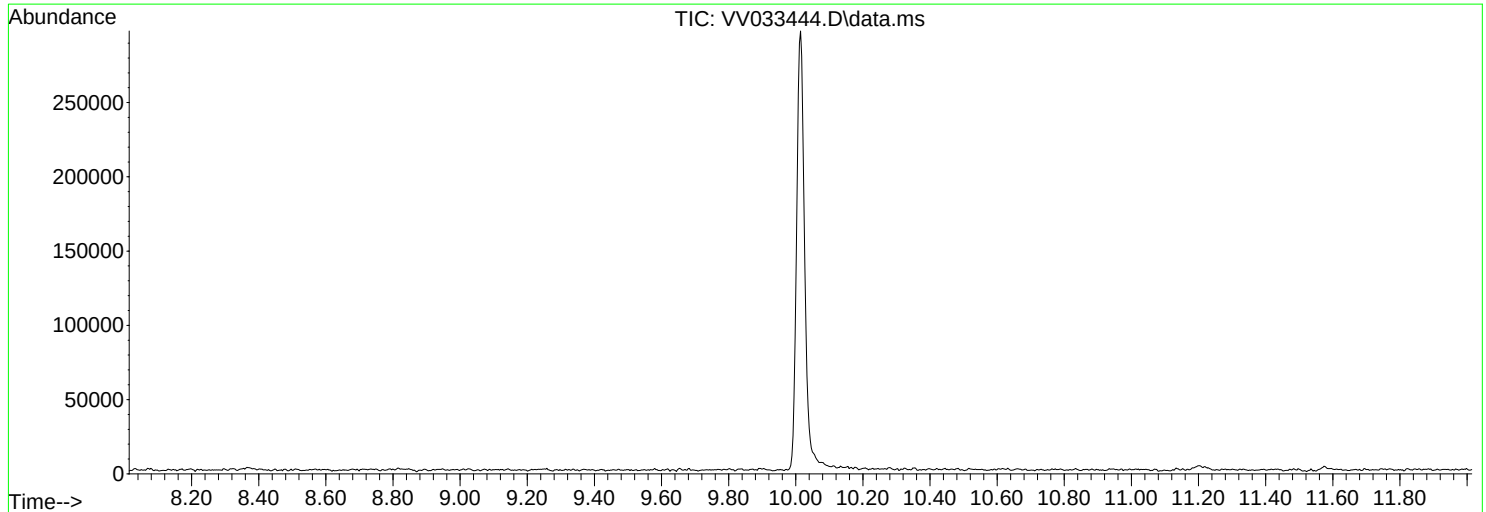

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	11113	PASS
75	95	30	80	52.2	29160	PASS
95	95	100	100	100.0	55819	PASS
96	95	5	9	6.6	3668	PASS
173	174	0.00	2	0.7	303	PASS
174	95	50	120	77.7	43355	PASS
175	174	5	9	8.4	3649	PASS
176	174	95	105	96.3	41744	PASS
177	176	5	10	6.6	2742	PASS

m/z	Abundance
35.70	139.0
36.00	147.0
37.00	156.0
37.80	188.0
38.60	137.0
39.80	216.0
40.90	110.0
43.10	167.0
43.90	433.0
44.90	105.0
46.20	114.0
47.00	114.0
47.80	117.0
51.30	159.0
52.30	114.0
62.90	109.0
116.30	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
35.80	529.0
37.00	3400.0
38.00	2941.0
39.00	1330.0
39.90	365.0
40.90	108.0
41.60	140.0
43.00	183.0
44.00	884.0
44.90	781.0
46.10	171.0
46.90	761.0
47.90	456.0
49.00	2884.0
50.00	11219.0
51.00	3729.0
52.00	215.0
52.70	182.0
53.90	211.0
55.00	202.0
56.00	1100.0
57.00	1819.0
57.90	180.0
59.90	728.0
61.00	3138.0
62.00	3266.0
63.00	2920.0
64.00	721.0
65.00	760.0
65.90	133.0
66.90	234.0
68.00	5852.0
69.00	5650.0
70.00	506.0
71.90	446.0
73.00	3176.0
74.00	10343.0
75.00	29224.0
76.00	2652.0
77.00	450.0
77.90	281.0
78.80	2981.0
79.90	921.0
80.90	3576.0
81.90	802.0
82.90	156.0
86.90	2191.0
87.80	2080.0
90.10	103.0
90.80	331.0
92.00	1935.0
92.90	3151.0
94.00	7644.0
95.00	55160.0
96.00	4005.0
96.80	113.0
103.80	409.0
104.90	151.0
105.80	361.0
112.10	132.0
112.80	146.0
114.80	162.0
115.90	301.0
116.80	514.0
117.70	407.0
119.00	470.0
124.00	108.0
127.80	299.0
128.80	119.0
129.70	186.0
130.80	108.0
135.10	215.0
136.50	182.0
141.00	815.0
141.80	150.0
142.90	1263.0
144.00	113.0
144.80	621.0
147.90	156.0
154.80	194.0
156.70	144.0
158.70	101.0
170.80	335.0
171.90	1020.0
173.10	909.0
173.90	42896.0
175.00	3517.0
176.00	41136.0
176.90	2937.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
35.10	145.0
35.80	484.0
37.00	3408.0
38.00	3026.0
39.00	1336.0
39.90	347.0
40.90	113.0
41.50	141.0
42.50	101.0
43.00	172.0
43.90	840.0
44.90	755.0
45.70	123.0
46.10	128.0
46.90	664.0
47.90	464.0
49.00	2819.0
50.00	11419.0
51.00	3701.0
52.00	238.0
52.70	188.0
53.90	240.0
55.00	224.0
56.00	1170.0
57.00	1742.0
57.90	181.0
59.90	642.0
61.00	3244.0
62.00	3214.0
63.00	2950.0
64.00	777.0
65.00	840.0
66.00	123.0
67.00	206.0
68.00	6071.0
69.00	5824.0
69.90	481.0
71.90	445.0
73.00	3234.0
74.00	10665.0
75.00	30104.0
76.00	2707.0
77.00	473.0
77.90	310.0
78.80	3023.0
79.90	1085.0
80.90	3511.0
81.90	861.0
82.90	145.0
86.90	2391.0
87.90	2152.0
90.80	314.0
92.00	1958.0
92.90	3046.0
94.00	7851.0
95.00	57704.0
96.00	3710.0
96.80	109.0
97.30	107.0
103.80	344.0
104.90	177.0
105.80	342.0
112.10	134.0
112.80	158.0
114.80	181.0
115.90	249.0
116.70	490.0
117.70	407.0
118.90	424.0
123.90	116.0
127.10	115.0
127.80	348.0
128.80	138.0
129.70	244.0
135.10	176.0
136.60	165.0
139.00	109.0
140.90	897.0
141.90	179.0
142.90	1152.0
144.00	104.0
144.80	610.0
147.90	135.0
152.80	111.0
154.70	187.0
156.70	197.0
158.70	103.0
170.80	329.0
171.90	1141.0
173.90	44776.0
175.00	3707.0
175.90	42936.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

176.90

2849.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
35.10	136.0
35.80	475.0
37.00	3106.0
38.00	2851.0
38.90	1282.0
39.80	293.0
40.90	157.0
41.50	128.0
42.40	132.0
43.00	131.0
43.90	723.0
44.90	633.0
45.60	144.0
46.10	121.0
46.90	537.0
47.90	450.0
49.00	2581.0
50.00	10701.0
51.00	3327.0
52.00	258.0
52.80	119.0
53.10	118.0
53.90	188.0
55.00	221.0
56.00	1163.0
57.00	1612.0
57.90	168.0
59.90	530.0
61.00	3141.0
62.00	3055.0
62.90	2839.0
64.00	727.0
65.00	798.0
66.00	115.0
66.60	173.0
67.10	193.0
68.00	5781.0
69.00	5481.0
69.90	464.0
71.90	431.0
73.00	3019.0
74.00	10113.0
75.00	28152.0
76.00	2529.0
77.00	419.0
77.90	386.0
78.80	2892.0
79.90	1130.0
80.90	3186.0
81.90	744.0
82.90	116.0
86.90	2460.0
87.90	1999.0
89.00	108.0
90.80	287.0
92.00	1794.0
92.90	2652.0
94.00	7395.0
95.00	54592.0
96.00	3288.0
97.30	117.0
100.60	100.0
103.80	286.0
104.90	200.0
105.80	312.0
107.70	100.0
112.10	118.0
112.80	112.0
114.80	145.0
115.90	188.0
116.90	465.0
117.70	351.0
118.80	401.0
124.40	101.0
127.10	134.0
127.80	341.0
128.80	163.0
129.80	287.0
134.70	142.0
135.20	110.0
136.70	115.0
139.00	131.0
140.90	762.0
141.90	160.0
142.90	985.0
144.00	104.0
144.90	514.0
148.70	108.0
152.80	142.0
154.70	170.0
156.70	208.0
170.80	309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

171.90	1104.0
173.90	42392.0
175.00	3722.0
175.90	41160.0
176.90	2441.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248