

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (QT Reviewed)


Data File : VV009048.D
Acq On : 19 Dec 2018 13:13
Operator : SY/MD
Sample : J6419-17
Misc : 5.95G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 02:11:41 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 01:58:47 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
BF045

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:10 PM

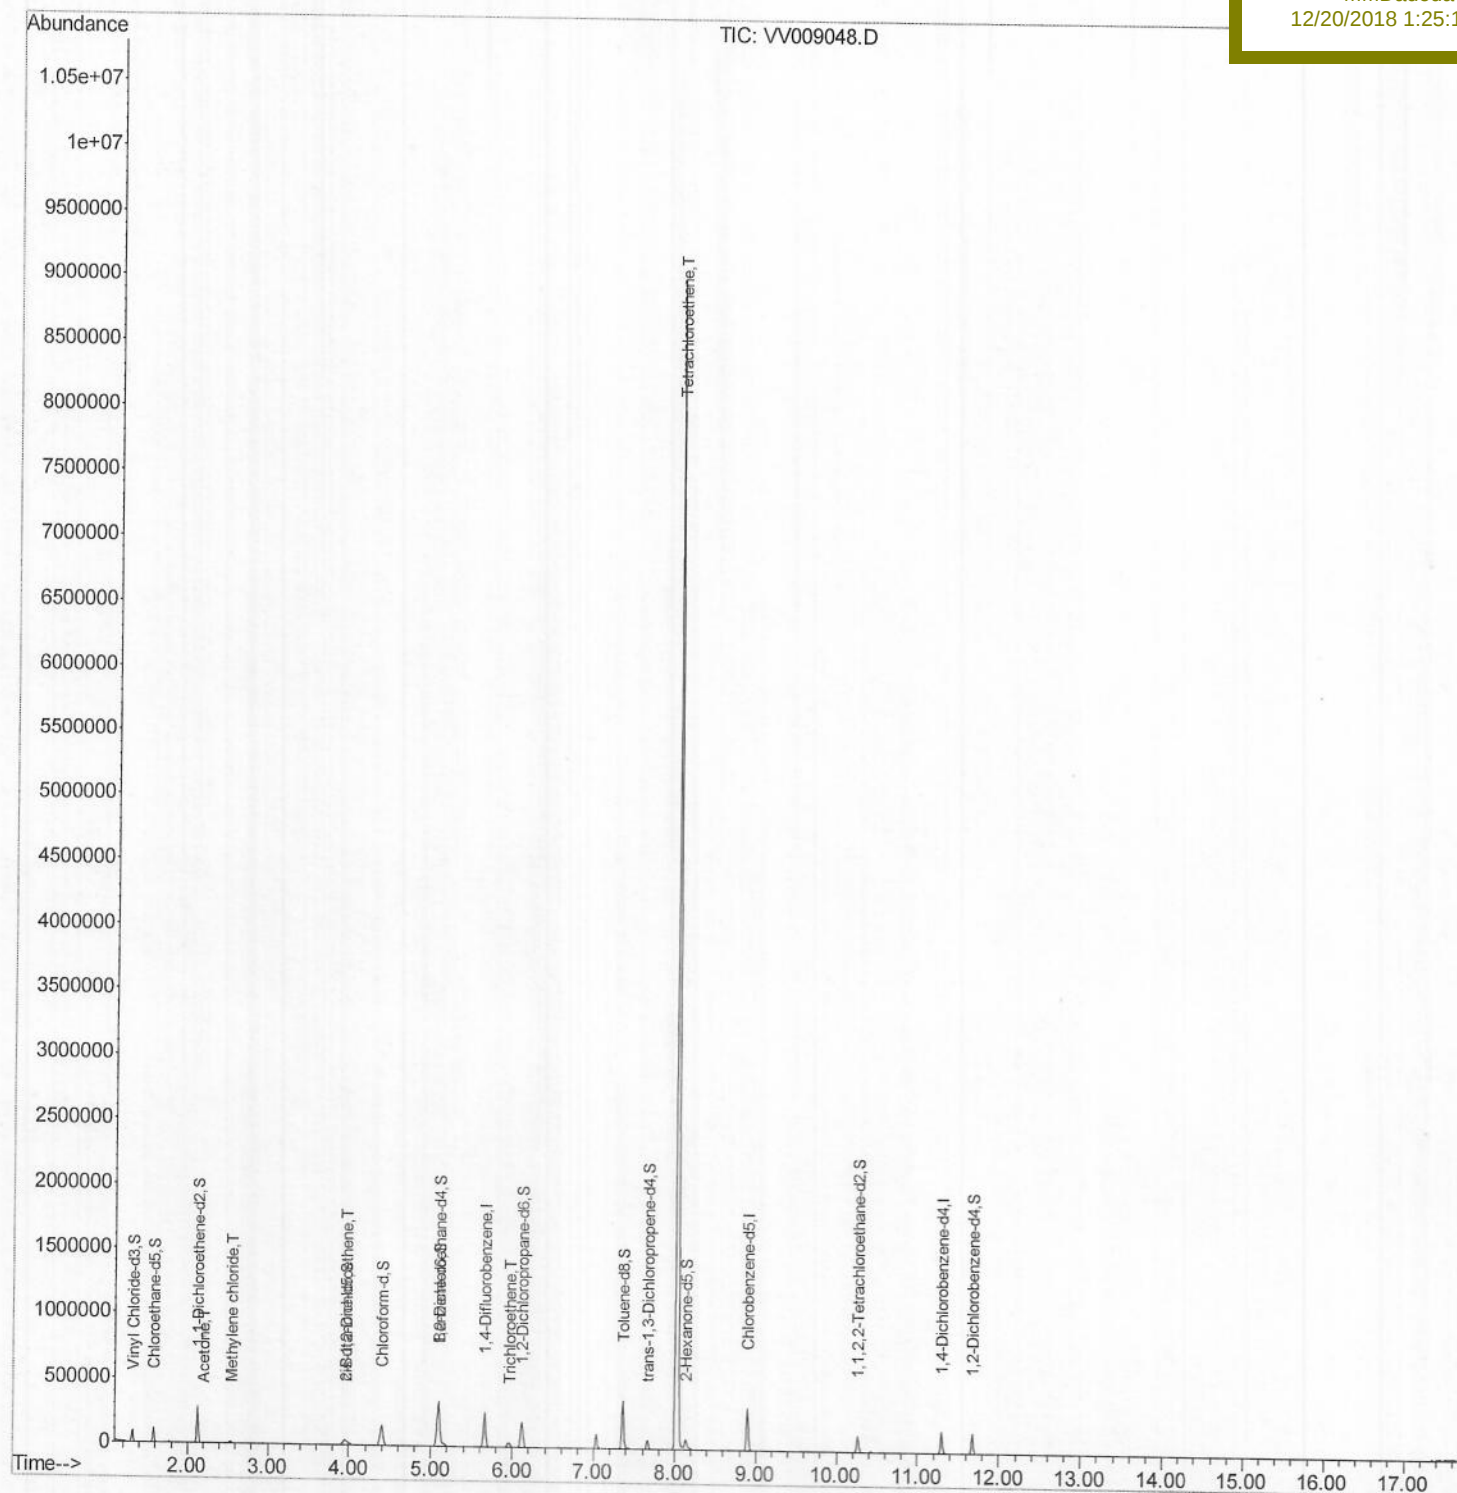

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (Qedit)

Data File : VV009048.D

Acq On : 19 Dec 2018 13:13

Operator : SY/MD

Sample : J6419-17

Misc : 5.95G/10ML/MSVOA_V/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 02:01:44 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M

Quant Title : VOC Analysis

QLast Update : Thu Dec 20 01:58:47 2018

Response via : Initial Calibration

Instrument :




MSVOA_V

ClientSampleId :

BF045

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:10 PM

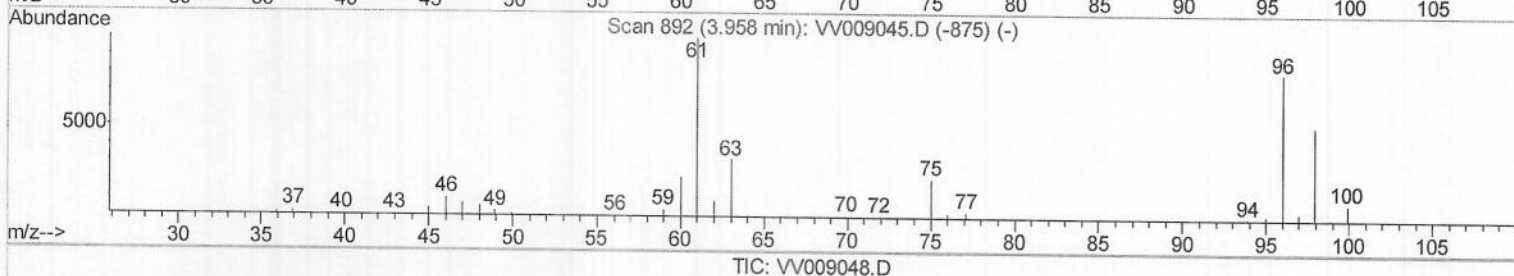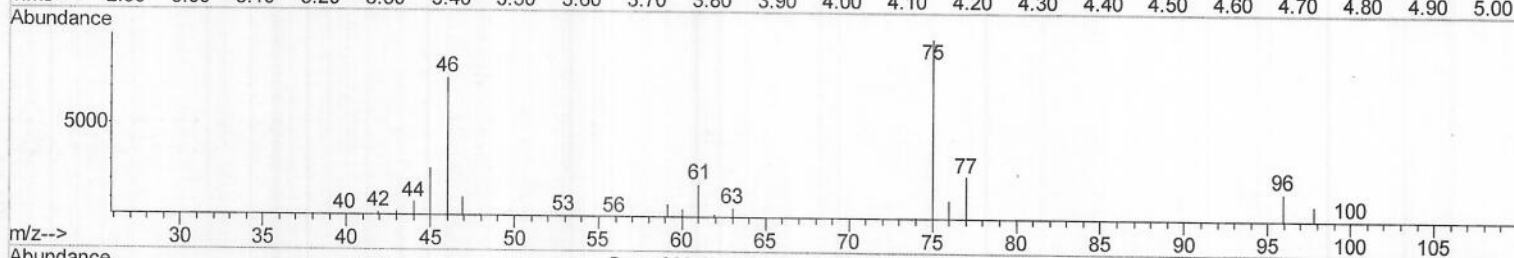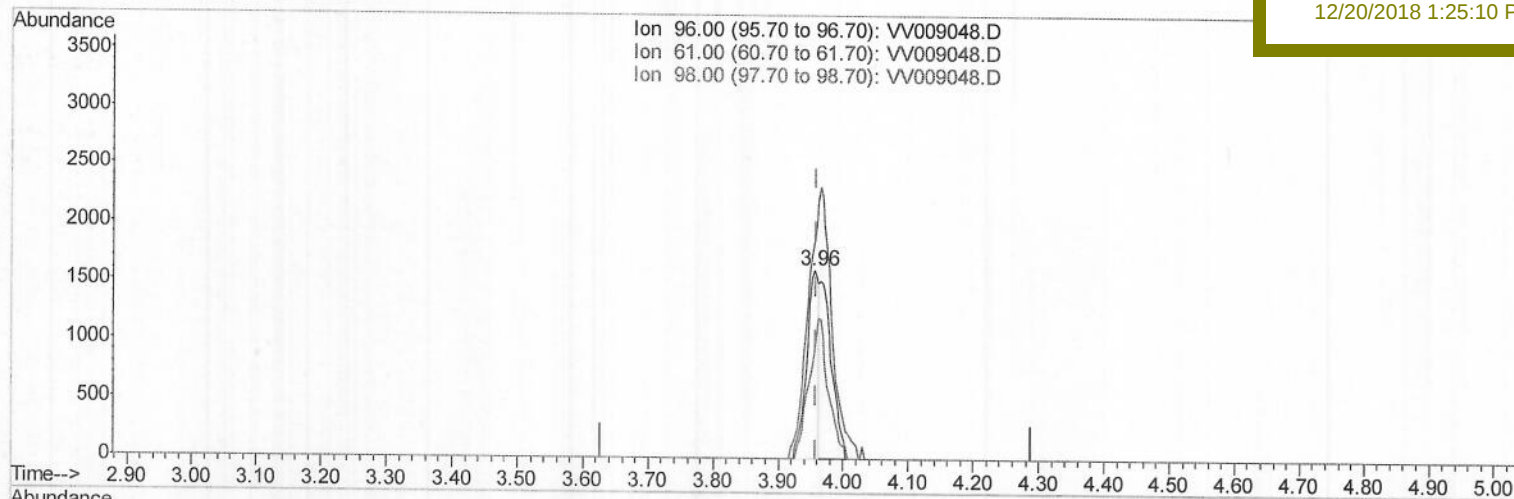

(22) cis-1,2-Dichloroethene (T)

3.955min (-0.003) 0.60ug/L

response 2044

Ion	Exp%	Act%
96.00	100	100
61.00	123.10	115.40
98.00	65.10	57.70
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (Qedit)




Data File : VV009048.D
Acq On : 19 Dec 2018 13:13
Operator : SY/MD
Sample : J6419-17
Misc : 5.95G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 02:01:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 01:58:47 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
BF045

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:10 PM

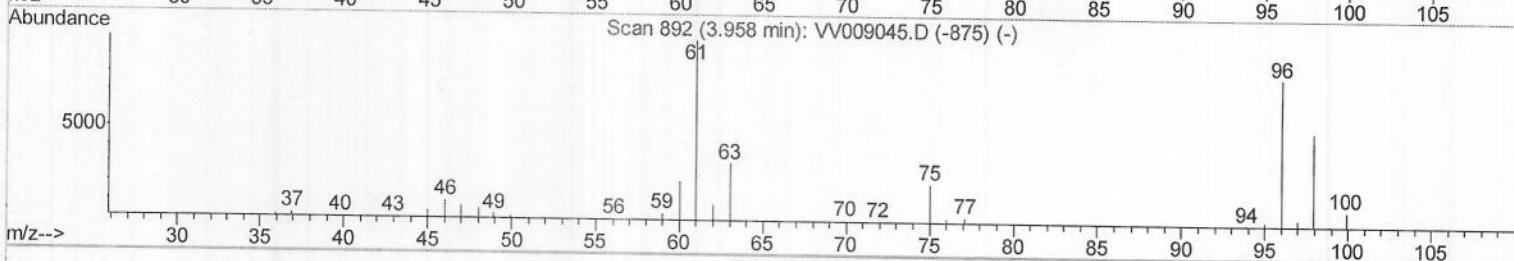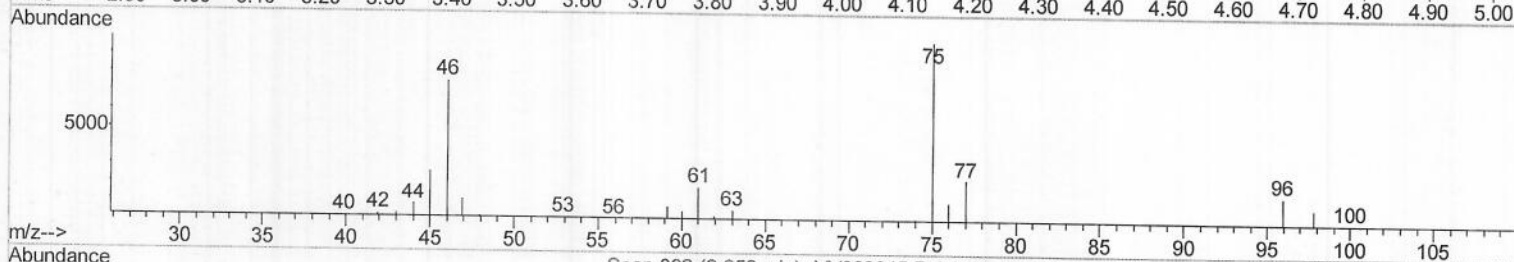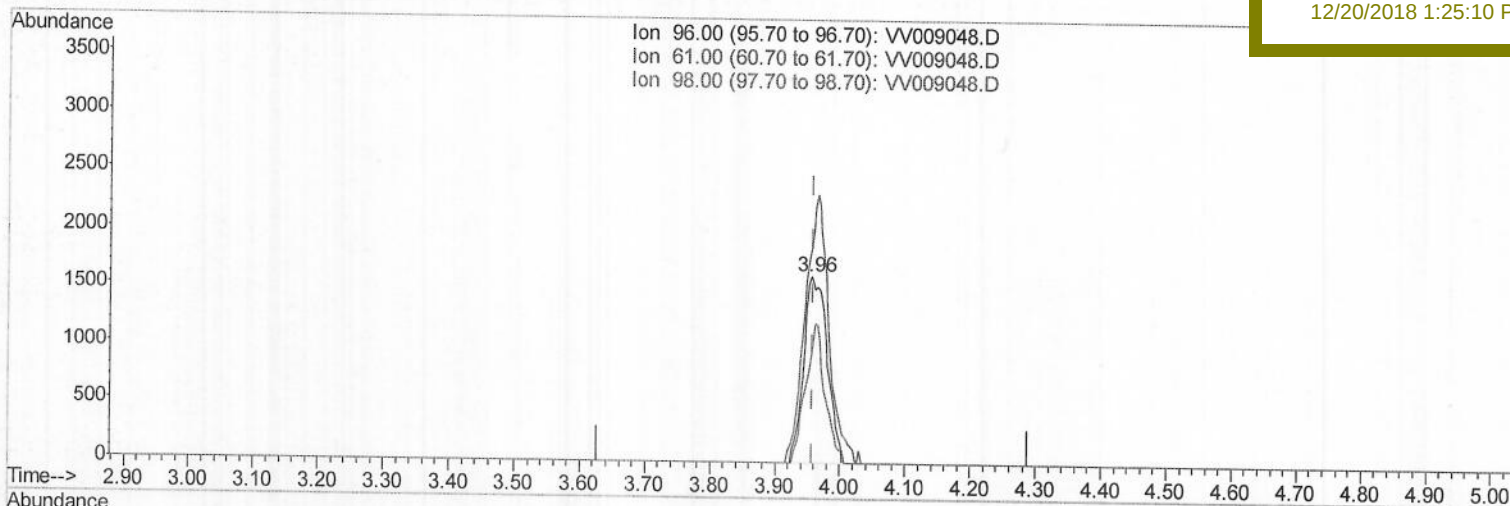

TIC: VV009048.D

(22) cis-1,2-Dichloroethene (T)

3.955min (-0.003) 1.17ug/L m

response 3979

Ion	Exp%	Act%
96.00	100	100
61.00	123.10	115.40
98.00	65.10	57.70
0.00	0.00	0.00

SY
12/28/18

Data File : VV009048.D
Acq On : 19 Dec 2018 13:13
Operator : SY/MD
Sample : J6419-17
Misc : 5.95G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
BF045

Quant Time: Dec 20 02:11:41 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 01:58:47 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:10 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	233835	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	181515	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	45460	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	57116	23.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.40%
7) Chloroethane-d5	1.58	69	63759	35.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	142.68%
10) 1,1-Dichloroethene-d2	2.13	63	155597	25.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	102.88%
20) 2-Butanone-d5	3.94	46	32718	37.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.28%
24) Chloroform-d	4.40	84	157651	28.04	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	112.16%
26) 1,2-Dichloroethane-d4	5.08	65	92793	30.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	121.00%
29) Benzene-d6	5.10	84	305252	30.11	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	120.44%
33) 1,2-Dichloropropane-d6	6.12	67	93492	32.94	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	131.76%#
37) Toluene-d8	7.36	98	250344	26.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.72%
38) trans-1,3-Dichloropropene-	7.66	79	37735	30.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	121.04%
39) 2-Hexanone-d5	8.14	63	21073	40.53	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.06%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	57782	24.27	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.08%
61) 1,2-Dichlorobenzene-d4	11.68	152	42003	24.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.48%

Target Compounds

					Qvalue
13) Acetone	2.20	43	3489	2.688	ug/L 100
16) Methylene chloride	2.54	84	5597	1.421	ug/L 90
22) cis-1,2-Dichloroethene	3.96	96	3979m	1.172	ug/L
35) Trichloroethene	5.96	95	8746	2.668	ug/L 95
47) Tetrachloroethene	8.02	164	2017847	756.793	ug/L 98

SY
12/28/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed