

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (QT Reviewed)

Data File : VV009058.D

Acq On : 19 Dec 2018 18:22

Operator : SY/MD

Sample : J6468-07

Misc : 5.01G/10ML/MSVOA_V/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 03:44:27 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M

Quant Title : VOC Analysis


QLast Update : Thu Dec 20 01:58:47 2018

Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampled :
C0JG5

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:39 PM

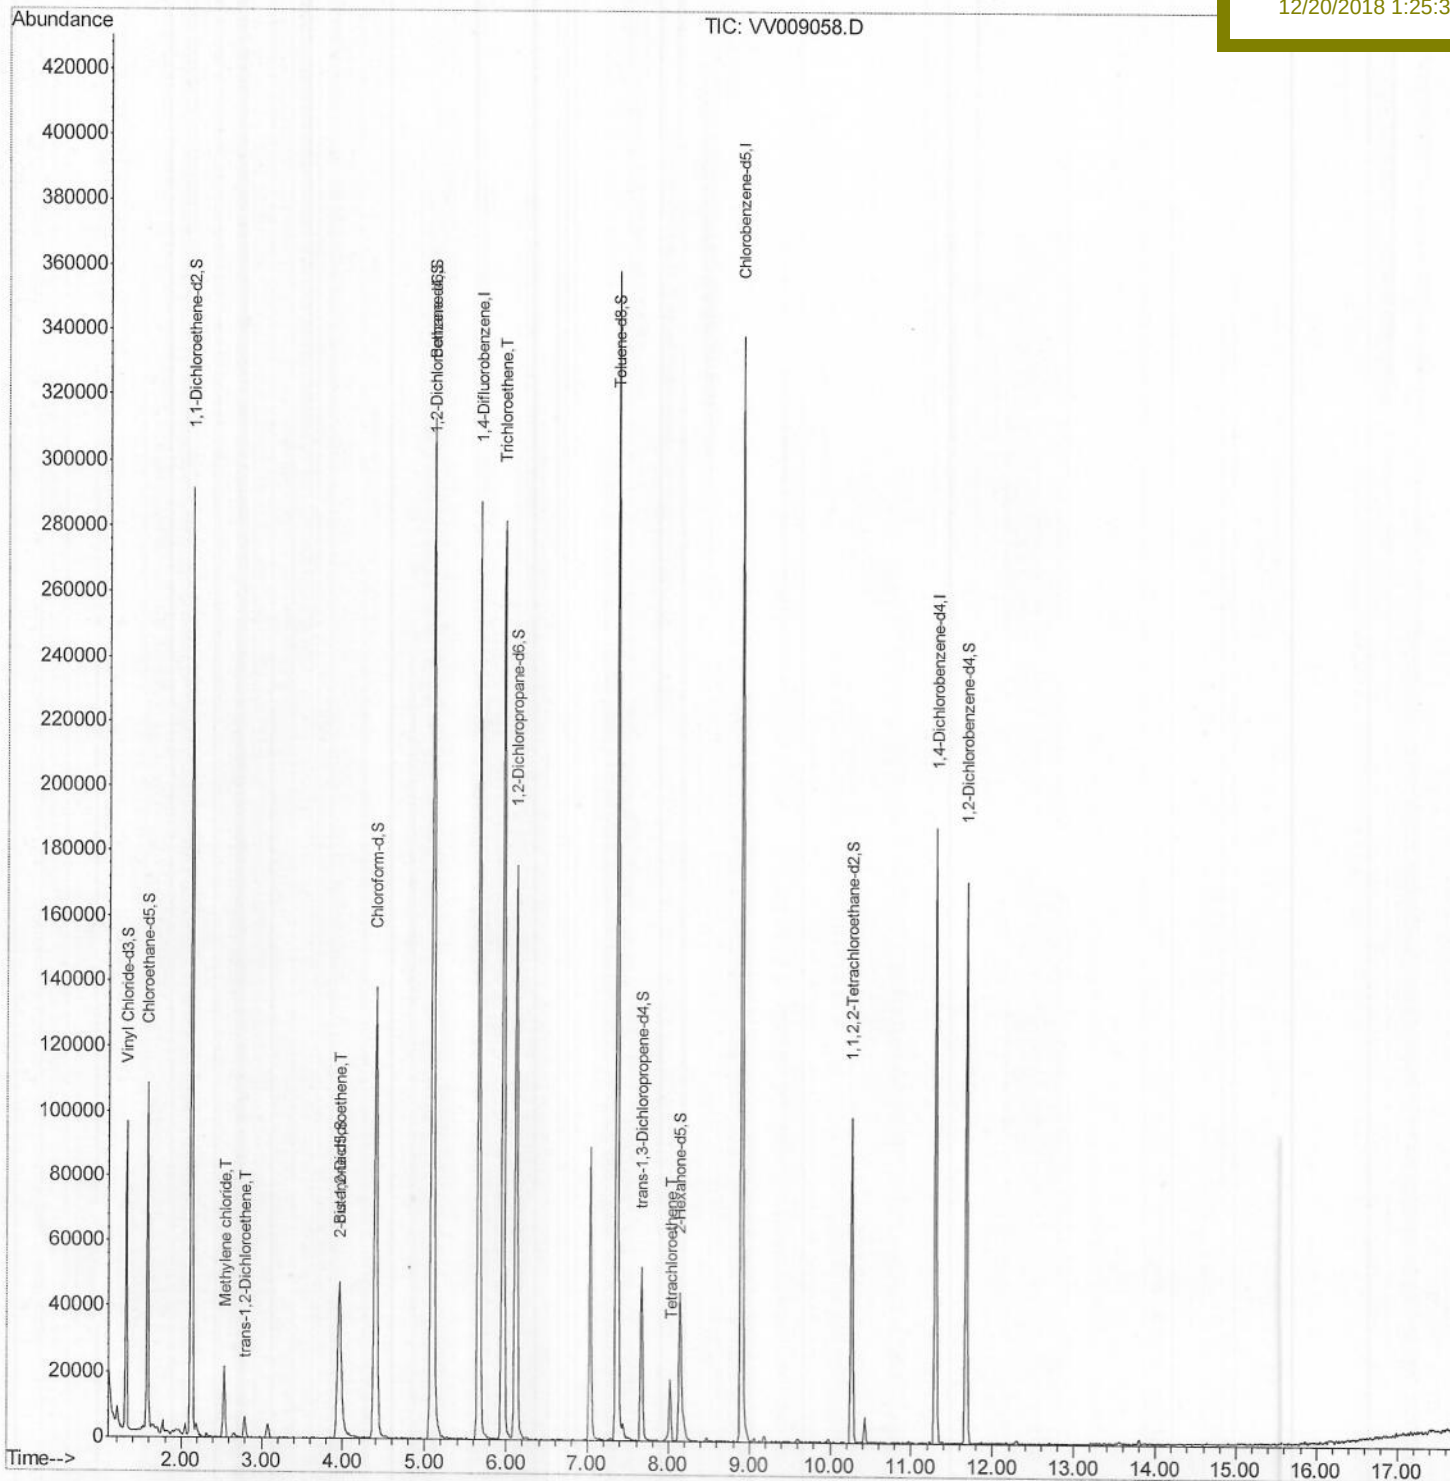

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (Qedit)




Data File : VV009058.D
Acq On : 19 Dec 2018 18:22
Operator : SY/MD
Sample : J6468-07
Misc : 5.01G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 02:04:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 01:58:47 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0JG5

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:39 PM

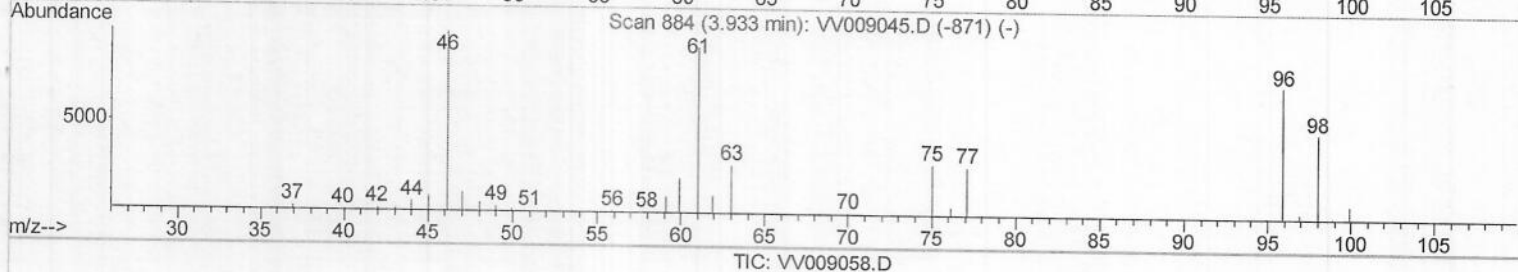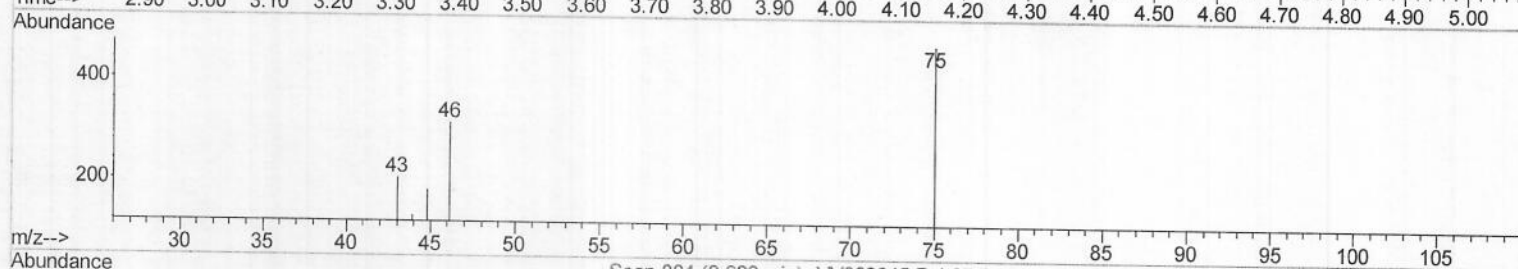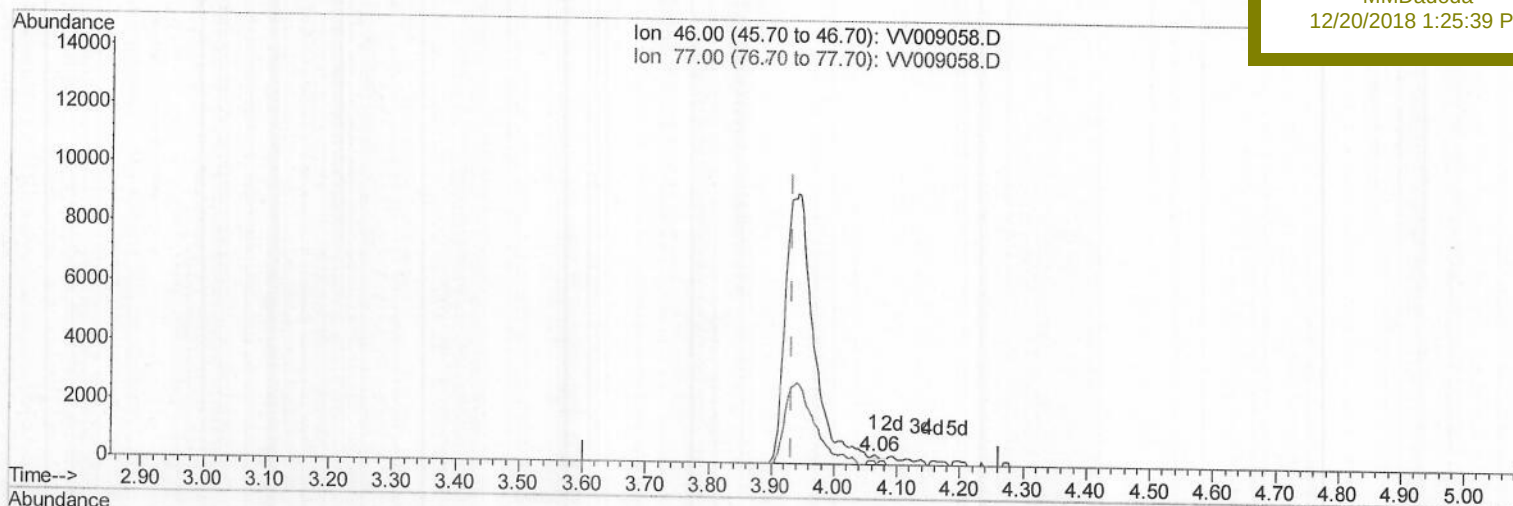

(20) 2-Butanone-d5 (S)

4.064min (+0.132) 0.08ug/L

response 76

Ion	Exp%	Act%
46.00	100	100
77.00	28.30	121.05#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (Qedit)




Data File : VV009058.D
Acq On : 19 Dec 2018 18:22
Operator : SY/MD
Sample : J6468-07
Misc : 5.01G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 02:04:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 01:58:47 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0JG5

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:39 PM

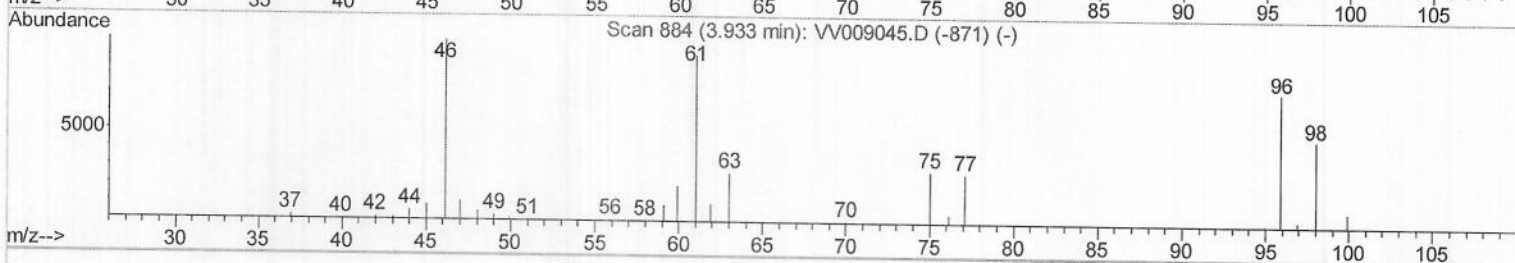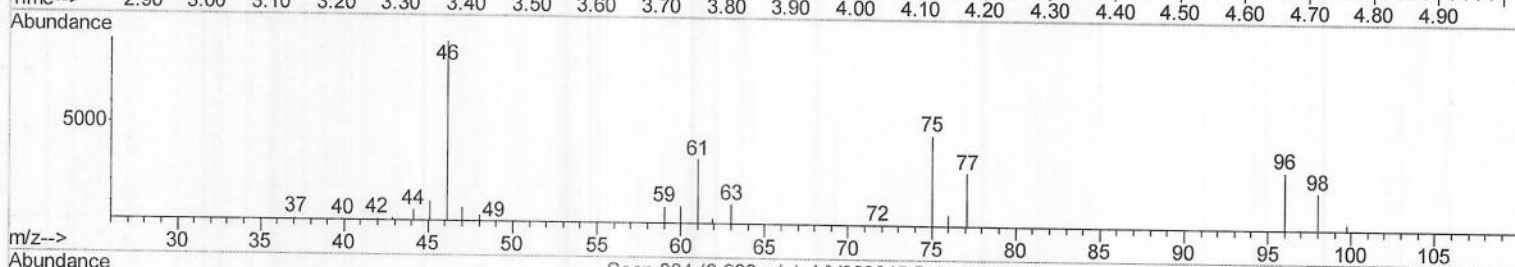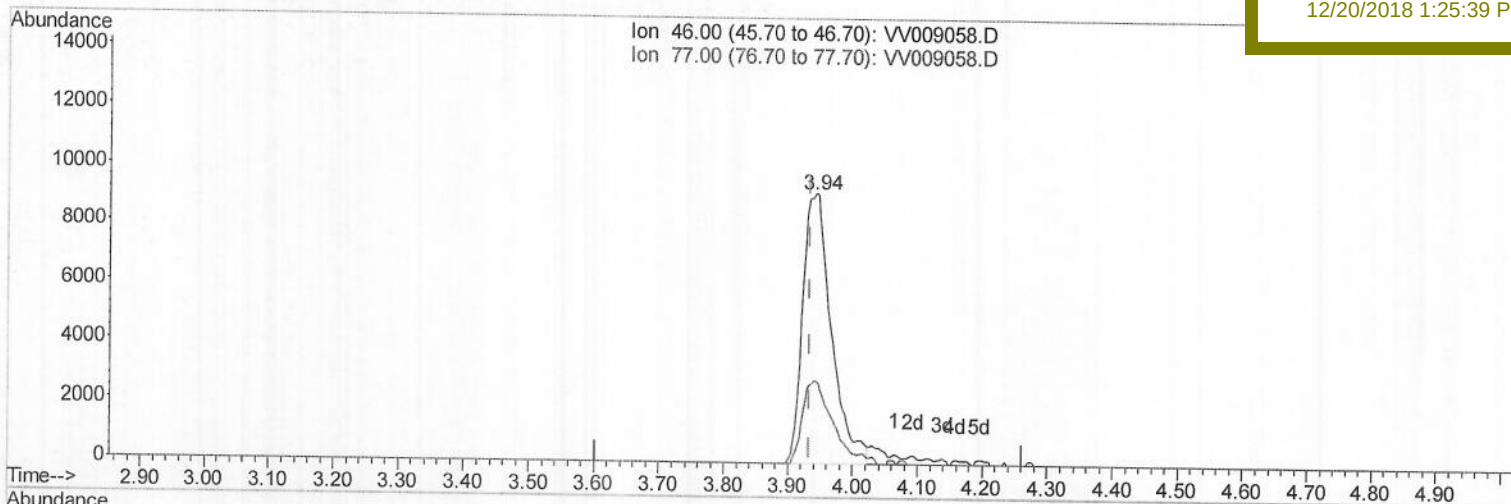

TIC: VV009058.D

(20) 2-Butanone-d5 (S)

3.942min (+0.009) 29.23ug/L m

response 28082

Ion Exp% Act%

46.00 100 100

77.00 28.30 0.33#

0.00 0.00 0.00

0.00 0.00 0.00

SY
12/28/18

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (QT Reviewed)

Data File : VV009058.D
Acq On : 19 Dec 2018 18:22
Operator : SY/MD
Sample : J6468-07
Misc : 5.01G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
C0JG5

Quant Time: Dec 20 03:44:27 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 01:58:47 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:39 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	255016	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	192890	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	53622	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58049	22.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.00%
7) Chloroethane-d5	1.58	69	62993	32.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	129.24%
10) 1,1-Dichloroethene-d2	2.13	63	160742	24.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	97.44%
20) 2-Butanone-d5	3.94	46	28082m	29.23	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.46%
24) Chloroform-d	4.40	84	144811	23.62	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.48%
26) 1,2-Dichloroethane-d4	5.08	65	77380	23.13	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.52%
29) Benzene-d6	5.10	84	288843	26.81	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.24%
33) 1,2-Dichloropropane-d6	6.12	67	86296	28.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.44%
37) Toluene-d8	7.36	98	245678	24.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.56%
38) trans-1,3-Dichloropropene-	7.67	79	30128	22.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.96%
39) 2-Hexanone-d5	8.14	63	16350	29.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.18%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	47045	18.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.36%
61) 1,2-Dichlorobenzene-d4	11.68	152	46960	23.34	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.36%

Target Compounds

					Qvalue
16) Methylene chloride	2.54	84	9608	2.237	ug/L 87
18) trans-1,2-Dichloroethene	2.79	96	2406	0.677	ug/L 86
22) cis-1,2-Dichloroethene	3.96	96	17157	4.632	ug/L 98
35) Trichloroethene	5.96	95	97338	27.938	ug/L 99
47) Tetrachloroethene	8.02	164	4068	1.436	ug/L 86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SY
12/28/18