

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (QT Reviewed)


Data File : VV009074.D
Acq On : 20 Dec 2018 02:52
Operator : SY/MD
Sample : J6468-09
Misc : 3.98G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 04:40:24 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 03:44:50 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampled :
C0JG7

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:53 PM

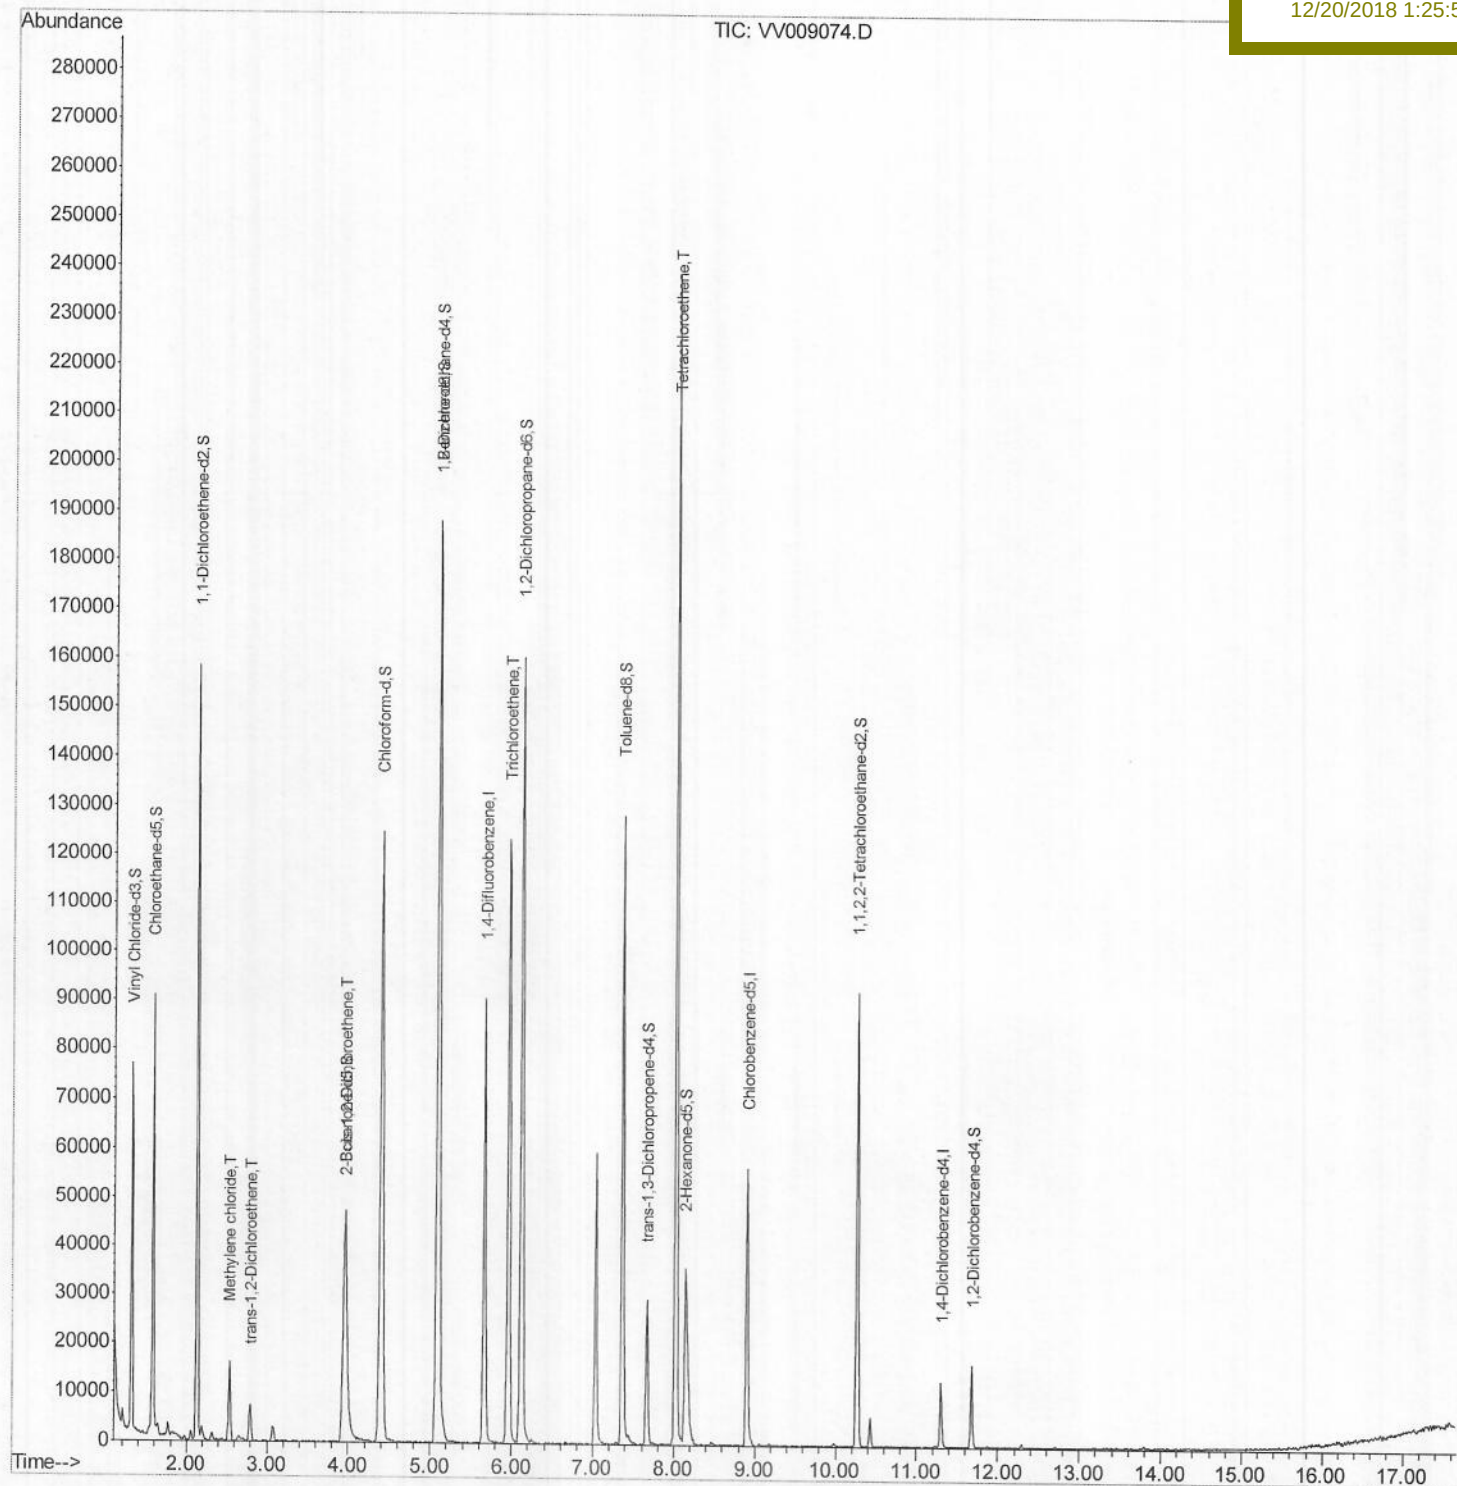

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (Qedit)


Data File : VV009074.D
Acq On : 20 Dec 2018 02:52
Operator : SY/MD
Sample : J6468-09
Misc : 3.98G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 04:39:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 03:44:50 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0JG7

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:53 PM

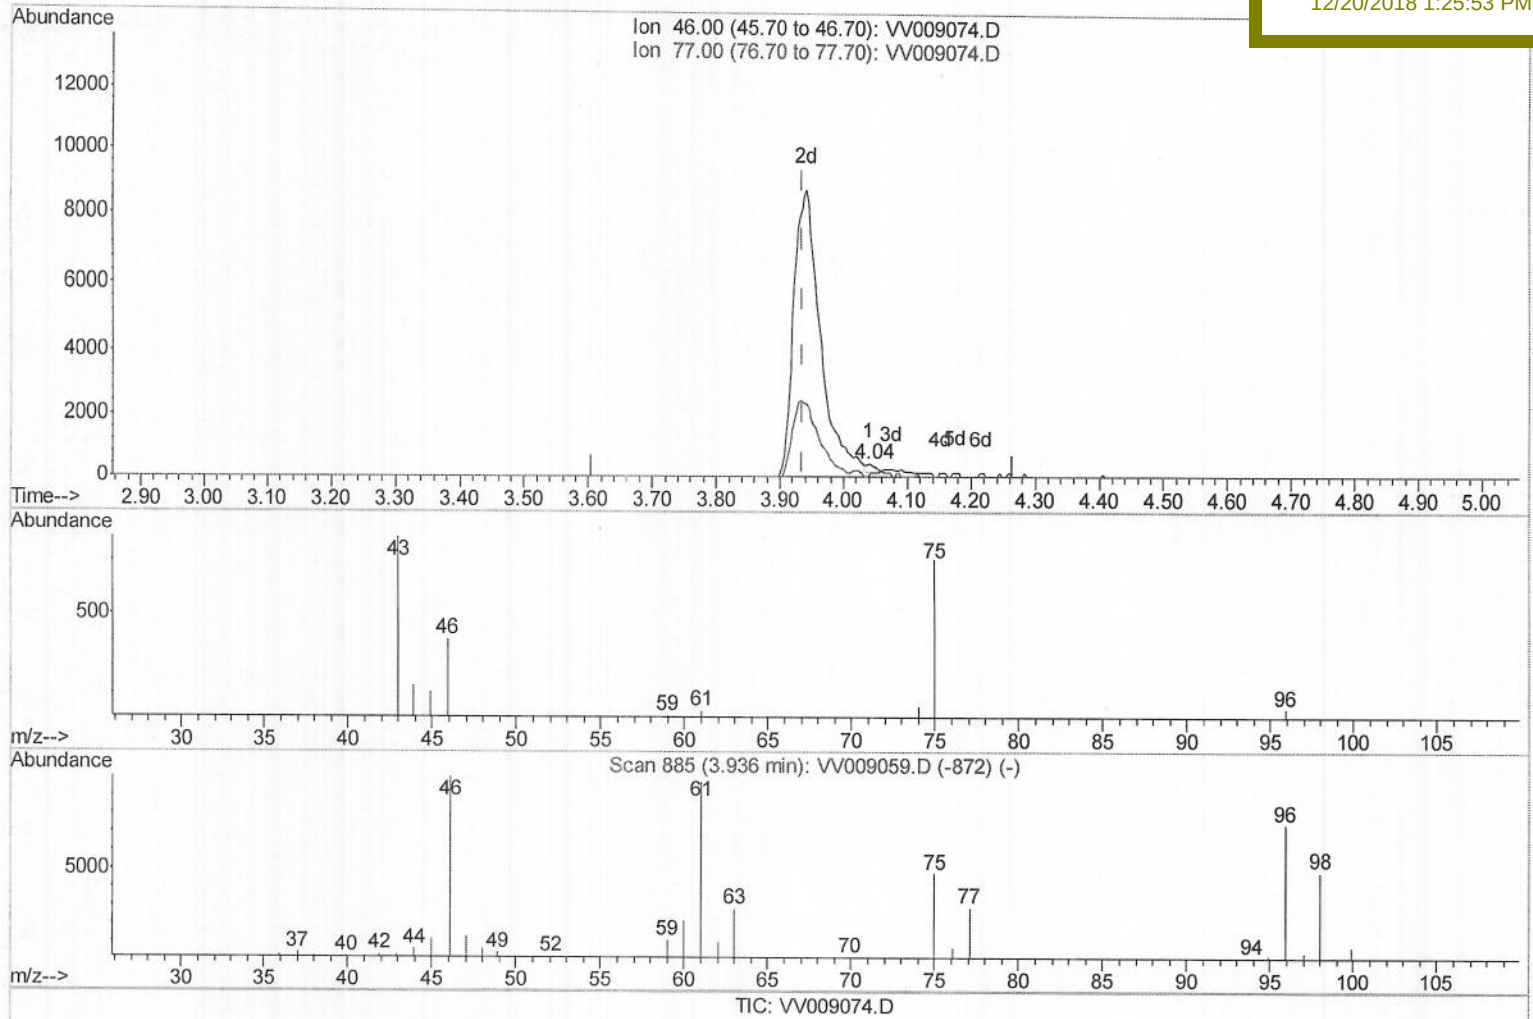

(20) 2-Butanone-d5 (S)

4.039min (+0.103) 0.80ug/L

response 245

Ion	Exp%	Act%
46.00	100	100
77.00	28.30	25.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (Qedit)




Data File : VV009074.D
Acq On : 20 Dec 2018 02:52
Operator : SY/MD
Sample : J6468-09
Misc : 3.98G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 04:39:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 03:44:50 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
Client Sampled :
C0JG7

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:53 PM

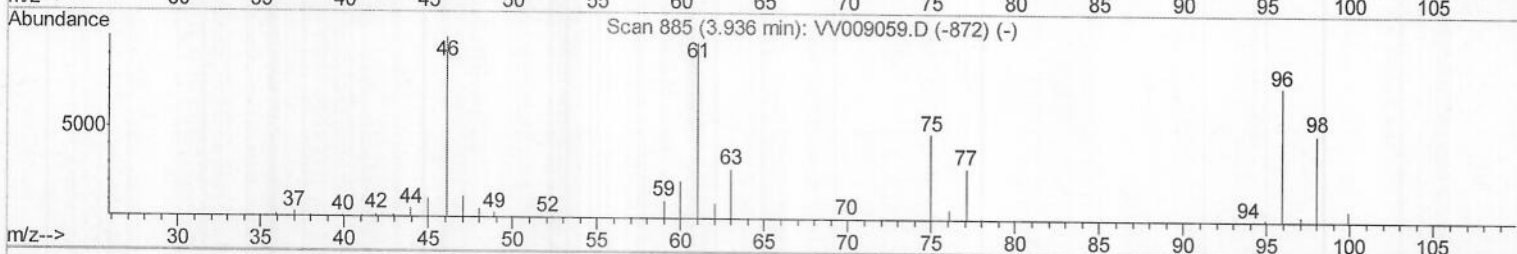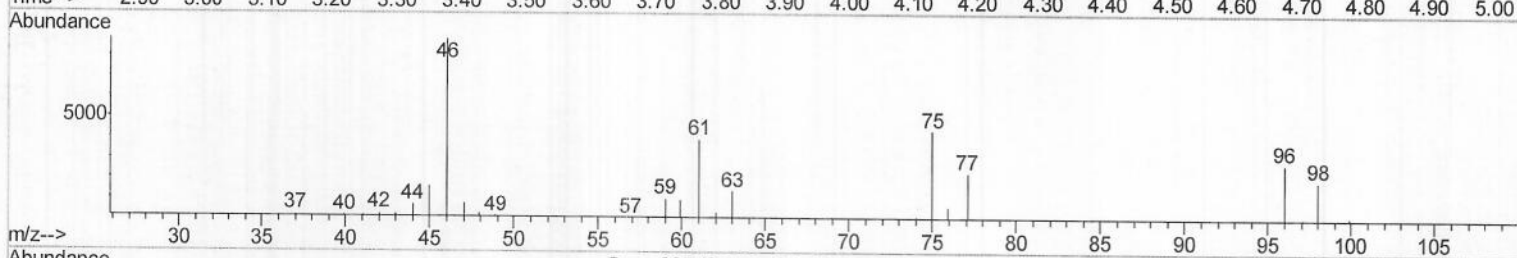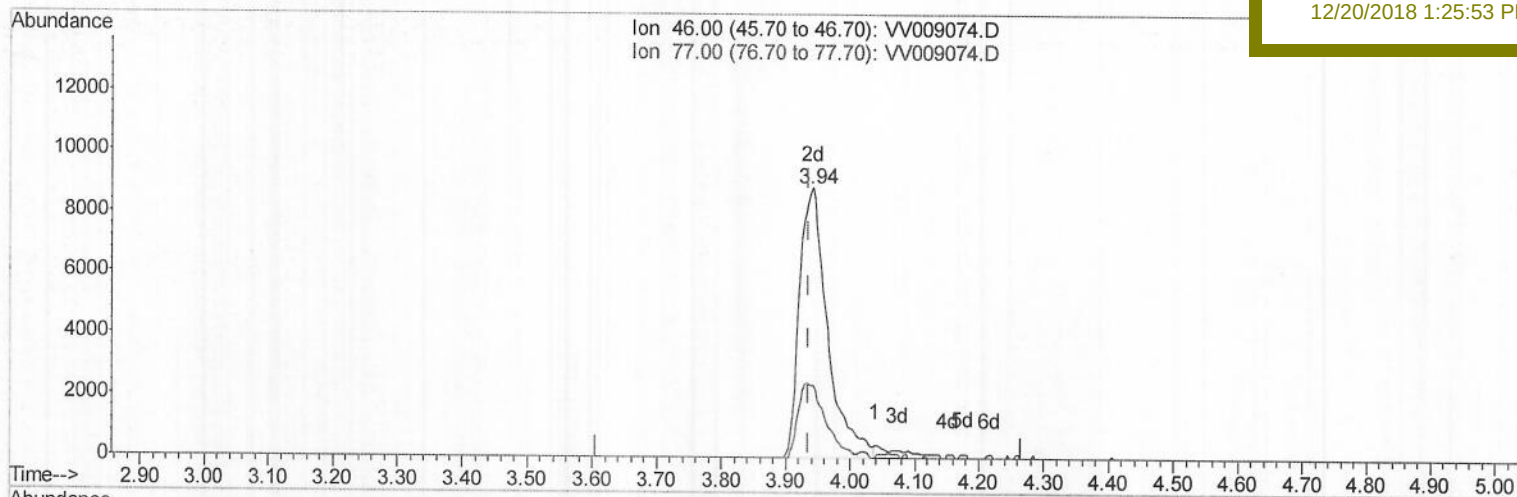

TIC: VV009074.D

(20) 2-Butanone-d5 (S)

3.942min (+0.006) 87.07ug/L m

response 26539

Ion	Exp%	Act%
46.00	100	100
77.00	28.30	0.24#
0.00	0.00	0.00
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121918\
Quantitation Report (QT Reviewed)

Data File : VV009074.D
Acq On : 20 Dec 2018 02:52
Operator : SY/MD
Sample : J6468-09
Misc : 3.98G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 04:40:24 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 20 03:44:50 2018
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0JG7

Manual Integrations
APPROVED

MMDadoda
12/20/2018 1:25:53 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	80899	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	33865	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	3923	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	46836	55.95	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	223.80%#	
7) Chloroethane-d5	1.58	69	52589	85.03	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	340.12%#	
10) 1,1-Dichloroethene-d2	2.13	63	83670	39.97	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	159.88%#	
20) 2-Butanone-d5	3.94	46	26539m	87.07	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	174.14%#	
24) Chloroform-d	4.40	84	132428	68.09	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	272.36%#	
26) 1,2-Dichloroethane-d4	5.08	65	72462	68.28	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	273.12%#	
29) Benzene-d6	5.10	84	151799	80.26	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	321.04%#	
33) 1,2-Dichloropropane-d6	6.12	67	79316	149.79	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	599.16%#	
37) Toluene-d8	7.36	98	90374	51.63	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	206.52%#	
38) trans-1,3-Dichloropropene-	7.67	79	17404	74.81	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	299.24%#	
39) 2-Hexanone-d5	8.14	63	12365	127.47	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	254.94%#	
48) 1,1,2,2-Tetrachloroethane-	10.26	84	44710	100.66	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	402.64%#	
61) 1,2-Dichlorobenzene-d4	11.68	152	4999	33.95	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	135.80%#	

Target Compounds

					Qvalue
16) Methylene chloride	2.53	84	6807	4.997 ug/L	96
18) trans-1,2-Dichloroethene	2.79	96	3162	2.806 ug/L	100
22) cis-1,2-Dichloroethene	3.96	96	17232	14.666 ug/L	94
35) Trichloroethene	5.96	95	42246	69.065 ug/L	99
47) Tetrachloroethene	8.02	164	54451	109.460 ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SY
12/28/18