


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121918\
Data File : VV009044.D
Acq On : 19 Dec 2018 09:01
Operator : SY/MD
Sample : BFB63
Misc : 5.00 g/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Title : VOC Analysis
Last Update : Fri Dec 21 01:30:11 2018

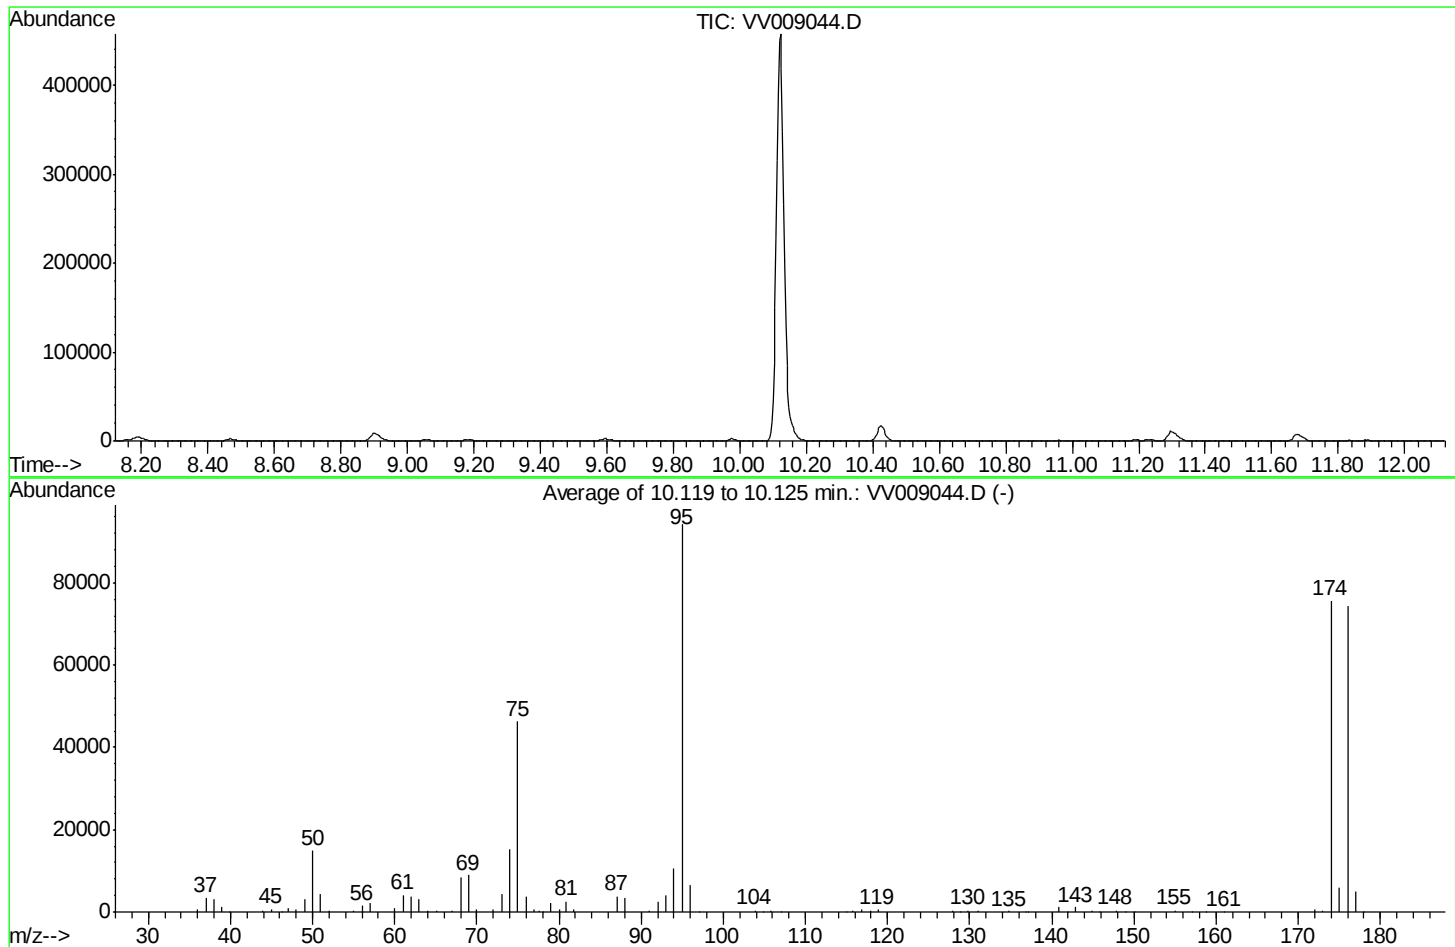

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	14868	PASS
75	95	30	80	49.1	46264	PASS
95	95	100	100	100.0	94200	PASS
96	95	5	9	6.8	6427	PASS
173	174	0.00	2	0.6	426	PASS
174	95	50	120	80.2	75586	PASS
175	174	5	9	7.9	6003	PASS
176	174	95	101	98.6	74493	PASS
177	176	5	9	6.7	4988	PASS

m/z	Abundance
43.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	668.0
37.00	3624.0
38.00	3335.0
39.00	1215.0
39.90	131.0
43.90	473.0
45.00	661.0
46.20	114.0
47.10	1095.0
47.90	546.0
49.00	3537.0
50.00	15336.0
51.00	4694.0
52.00	190.0
55.10	258.0
56.00	1513.0
57.00	2313.0
60.00	922.0
61.00	4141.0
62.00	3809.0
63.00	3272.0
64.00	345.0
65.00	312.0
67.00	293.0
68.00	8574.0
69.00	8928.0
70.00	701.0
72.00	482.0
73.00	4306.0
74.00	15741.0
75.00	47160.0
76.10	4046.0
76.90	472.0
77.70	353.0
78.90	2428.0
80.00	674.0
80.90	2774.0
81.80	584.0
87.00	4048.0
87.90	3561.0
91.00	357.0
92.00	2675.0
93.00	4019.0
94.00	10790.0
95.00	97056.0
96.00	6561.0
97.00	112.0
103.90	445.0
104.80	160.0
105.80	397.0
107.00	121.0
115.80	330.0
116.90	506.0
117.90	423.0
118.80	530.0
127.90	339.0
128.80	144.0
129.90	437.0
131.00	198.0
134.80	201.0
137.10	250.0
140.90	1162.0
141.90	185.0
142.90	1047.0
144.90	179.0
145.90	159.0
147.80	305.0
154.90	271.0
157.00	151.0
160.90	132.0
172.00	752.0
173.00	1279.0
174.00	74888.0
175.00	6171.0
176.00	74216.0
177.00	5008.0
177.90	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	670.0
37.00	3688.0
38.00	3161.0
39.00	1256.0
39.80	141.0
43.90	450.0
45.00	682.0
46.20	102.0
47.00	926.0
47.90	592.0
49.00	3316.0
50.00	15421.0
51.00	4604.0
52.00	184.0
55.00	211.0
56.00	1539.0
57.00	2242.0
60.00	887.0
61.00	4241.0
62.00	3861.0
63.00	3204.0
64.00	366.0
65.00	299.0
66.90	263.0
68.00	8818.0
69.00	9191.0
70.00	664.0
71.90	505.0
73.00	4535.0
74.00	15825.0
75.00	47832.0
76.00	3943.0
76.90	522.0
77.60	362.0
78.10	217.0
78.90	2330.0
80.00	682.0
80.90	2593.0
81.80	570.0
87.00	3858.0
88.00	3516.0
91.00	360.0
92.00	2580.0
93.00	4101.0
94.00	11121.0
95.00	97592.0
96.00	6669.0
97.00	123.0
103.90	499.0
104.80	124.0
105.80	427.0
107.00	131.0
115.00	111.0
115.80	290.0
116.90	533.0
117.90	432.0
118.80	557.0
127.90	382.0
128.90	182.0
129.90	415.0
131.00	230.0
134.80	218.0
136.80	242.0
140.90	1140.0
142.00	166.0
142.90	1155.0
144.90	209.0
145.80	163.0
147.90	367.0
149.00	124.0
155.00	357.0
157.10	154.0
158.80	152.0
161.00	134.0
172.00	709.0
174.00	78176.0
175.00	6272.0
176.00	77336.0
177.00	5230.0
177.90	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	620.0
37.00	3410.0
38.00	2786.0
39.00	1181.0
39.80	132.0
43.90	444.0
45.00	605.0
47.00	732.0
48.00	546.0
49.00	2818.0
50.00	13847.0
51.00	4062.0
52.10	171.0
55.00	182.0
56.00	1308.0
57.00	2049.0
60.00	853.0
61.00	3925.0
62.00	3608.0
63.00	2884.0
64.00	302.0
65.10	294.0
66.90	223.0
68.00	8042.0
69.00	8546.0
70.00	528.0
71.90	481.0
73.00	4219.0
74.00	14255.0
75.00	43800.0
76.00	3517.0
76.90	477.0
77.60	295.0
78.10	196.0
78.90	2236.0
80.00	647.0
80.90	2186.0
81.90	515.0
87.00	3322.0
88.00	2962.0
90.90	316.0
92.10	2282.0
93.00	3676.0
94.00	10317.0
95.00	87952.0
96.00	6051.0
97.10	127.0
103.90	447.0
105.80	386.0
107.00	102.0
115.00	115.0
115.70	236.0
116.90	520.0
117.90	342.0
118.90	522.0
127.90	395.0
129.00	174.0
129.80	352.0
131.00	201.0
134.80	209.0
136.80	232.0
140.90	1016.0
142.10	140.0
142.90	1189.0
144.80	170.0
145.70	137.0
147.90	341.0
149.00	144.0
150.00	115.0
155.00	369.0
157.10	174.0
158.80	163.0
161.00	117.0
172.00	584.0
174.00	73696.0
175.00	5567.0
176.00	71928.0
177.00	4727.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63