


Data File : VV014128.D
Acq On : 19 Dec 2019 10:23
Operator : SY/MD
Sample : VV1219WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Manual Integrations
APPROVED

apatel
12/20/2019 10:49:10 AM

Quant Time: Dec 20 07:25:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 07:12:45 2019
Response via : Initial Calibration

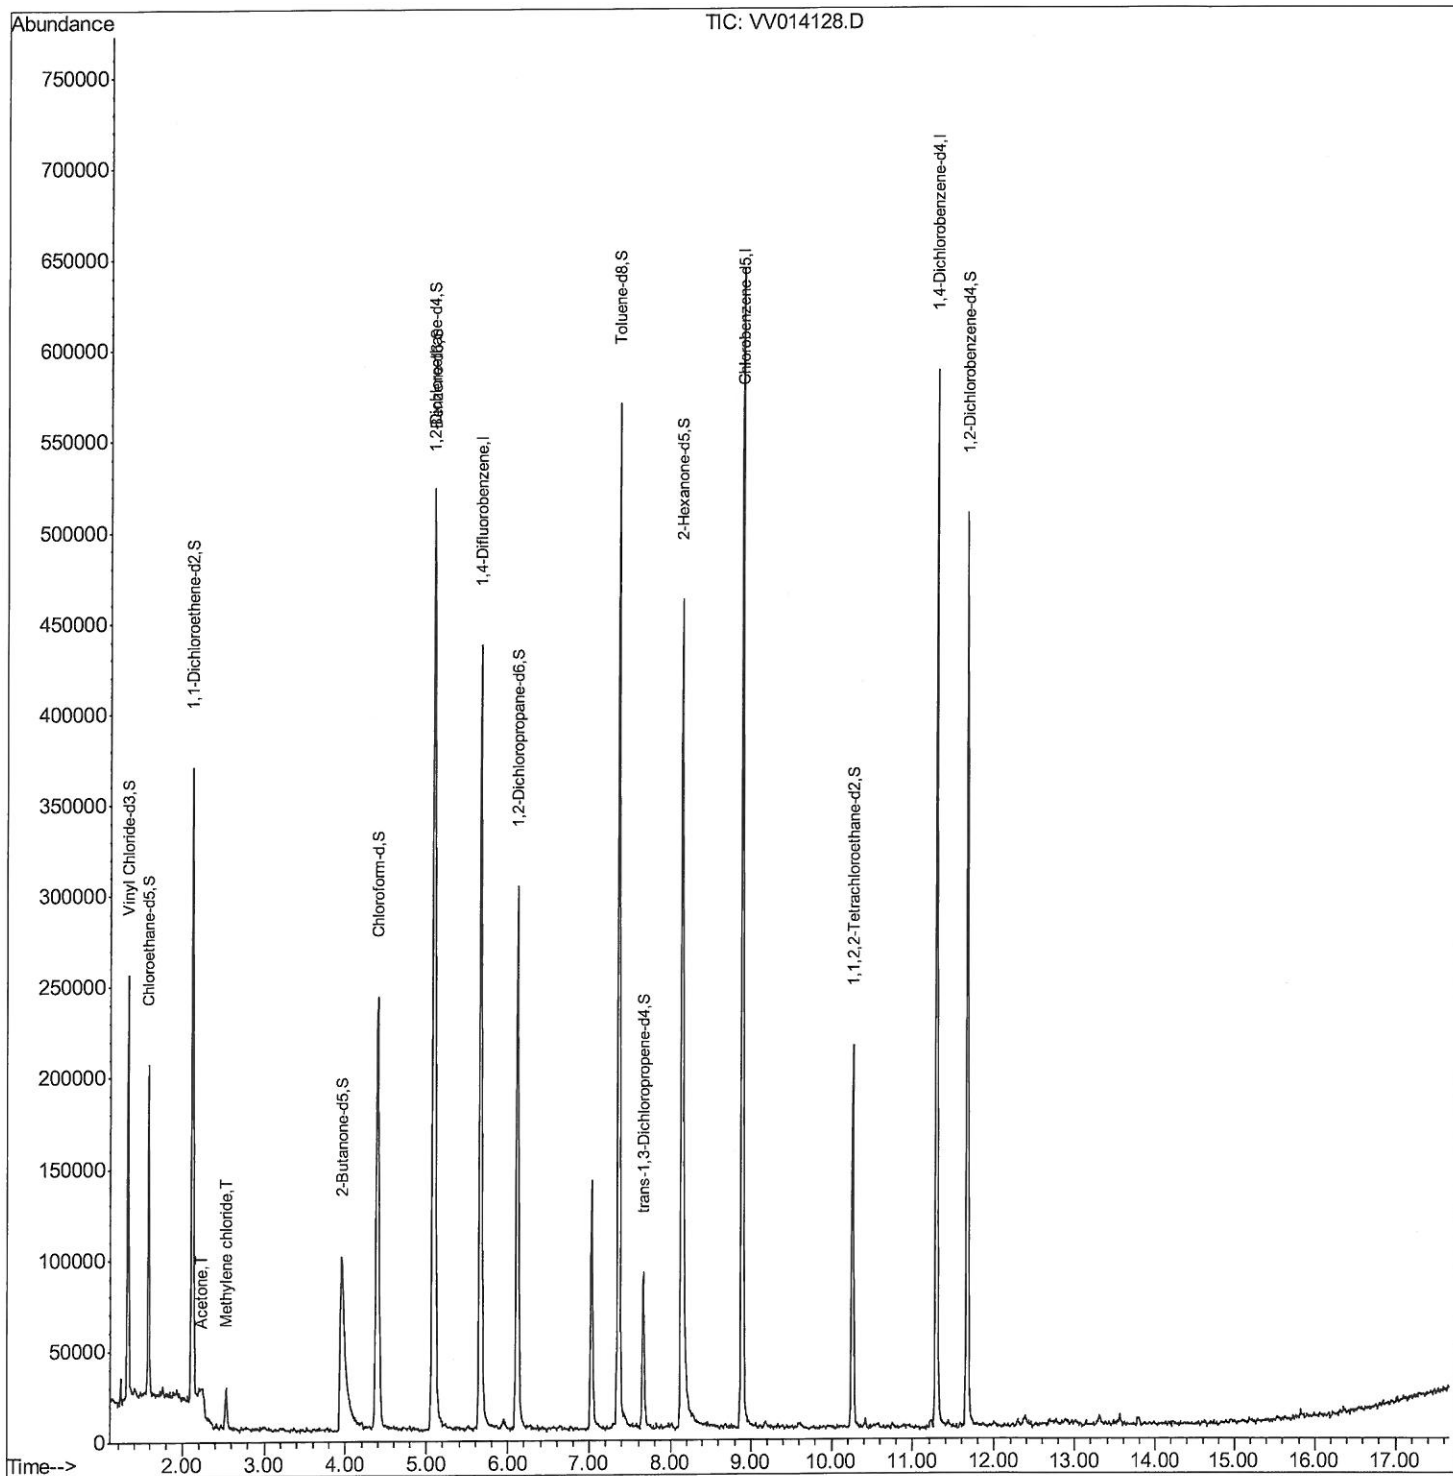

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121919\
Quantitation Report (Qedit)




Data File : VV014128.D
Acq On : 19 Dec 2019 10:23
Operator : SY/MD
Sample : VV1219WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK64

Manual Integrations
APPROVED

apatel
12/20/2019 10:49:10 AM

Quant Time: Dec 20 07:15:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 07:12:45 2019
Response via : Initial Calibration

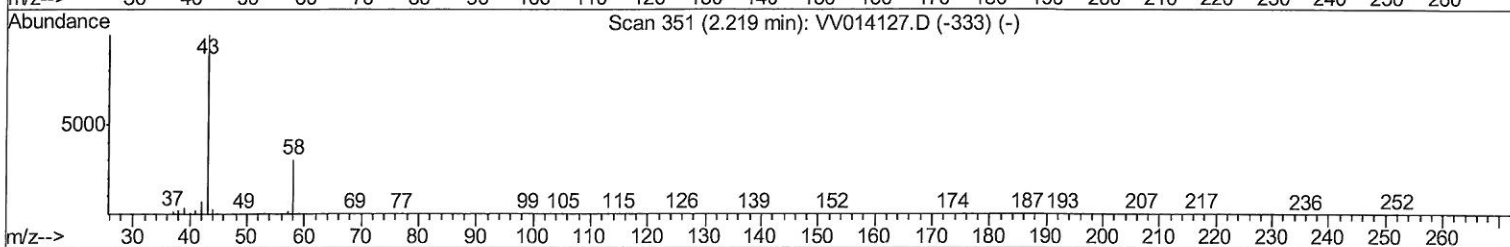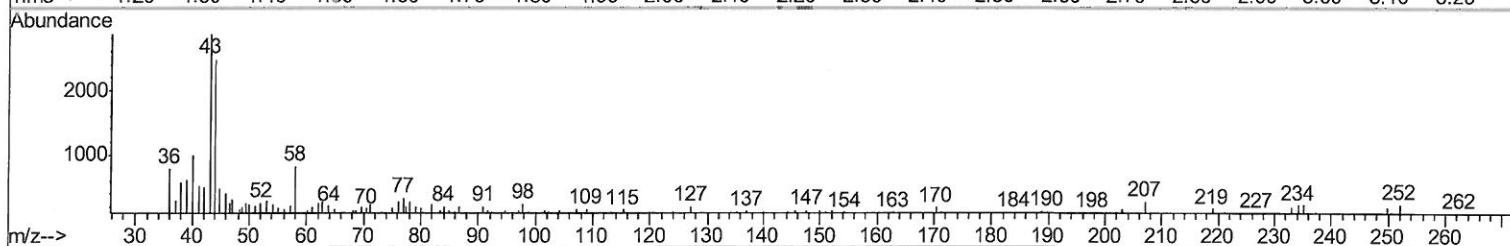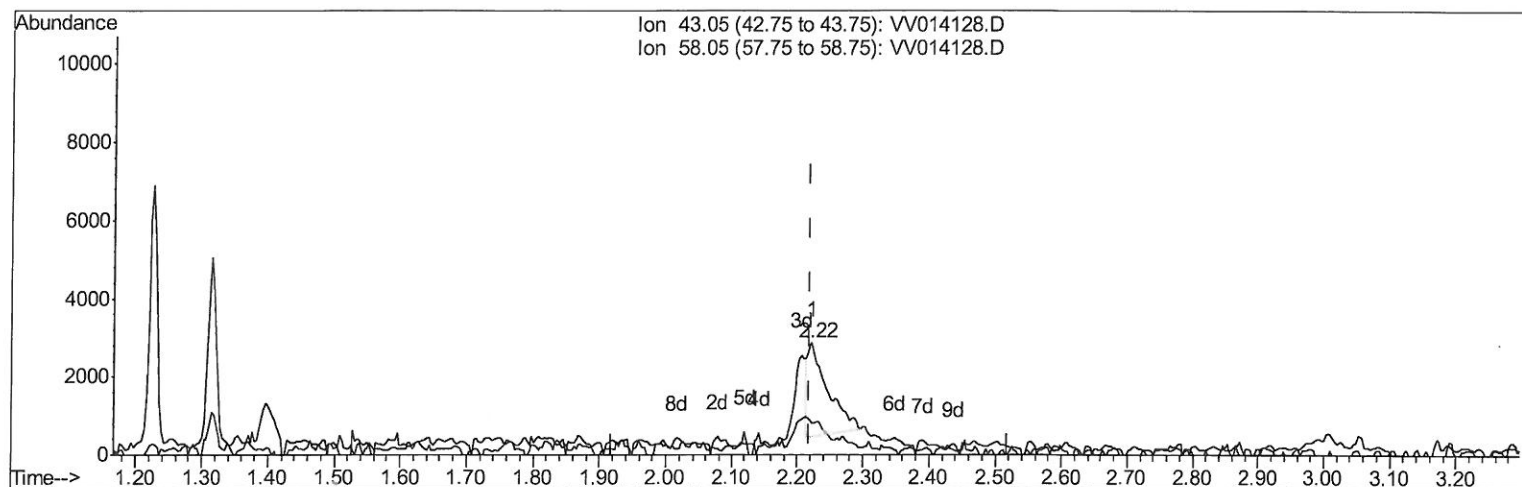

TIC: VV014128.D

(13) Acetone (T)

2.222min (+0.003) 1.56ug/L

response 5114

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	6.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121919\
Quantitation Report (Qedit)




Data File : VV014128.D
Acq On : 19 Dec 2019 10:23
Operator : SY/MD
Sample : VV1219WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Manual Integrations
APPROVED

apatel
12/20/2019 10:49:10 AM

Quant Time: Dec 20 07:15:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 07:12:45 2019
Response via : Initial Calibration

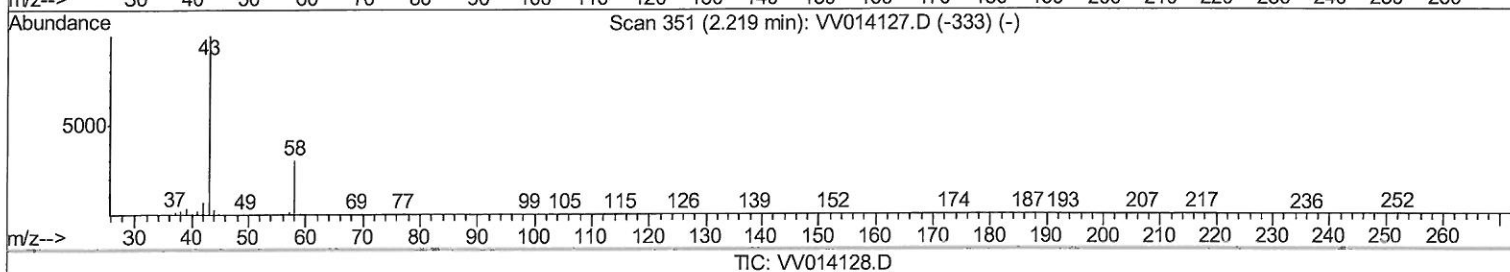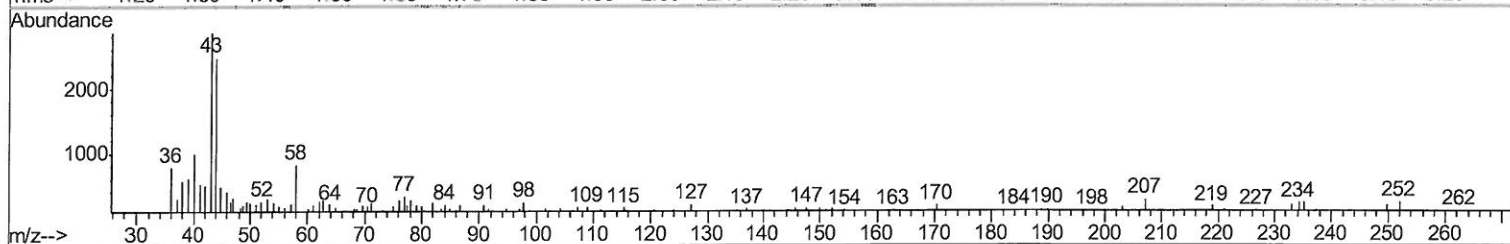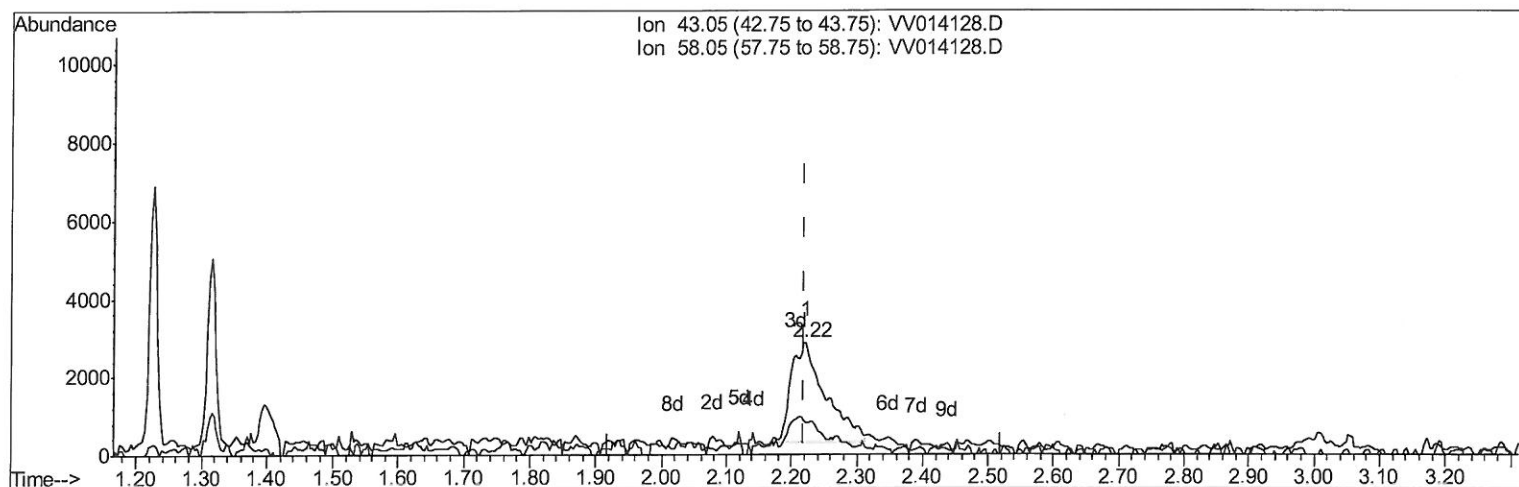

(13) Acetone (T)

2.222min (+0.003) 2.85ug/L m

response 9346

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	3.79
0.00	0.00	0.00
0.00	0.00	0.00

7 mg
12/20/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121919\
Quantitation Report (QT Reviewed)

Data File : VV014128.D
Acq On : 19 Dec 2019 10:23
Operator : SY/MD
Sample : VV1219WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Manual Integrations
APPROVED

apatel
12/20/2019 10:49:10 AM

Quant Time: Dec 20 07:25:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 07:12:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	364369	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	352674	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	154616	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	134517	5.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	119.20%
7) Chloroethane-d5	1.58	69	112204	5.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.20%
11) 1,1-Dichloroethene-d2	2.13	63	176406	4.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.00%
20) 2-Butanone-d5	3.96	46	222771	47.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.04%
24) Chloroform-d	4.40	84	235552	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
26) 1,2-Dichloroethane-d4	5.08	65	116126	5.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.40%
32) Benzene-d6	5.09	84	451529	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.11	67	141827	5.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.60%
41) Toluene-d8	7.36	98	372135	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.66	79	48739	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.13	63	154563	39.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.40%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	101628	5.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	133434	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%

Target Compounds

13) Acetone	2.22	43	9346m	2.851	ug/L	Qvalue
16) Methylene chloride	2.53	84	9678	0.403	ug/L	92

> MD
12/20/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed