


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121919\
Data File : VV014126.D
Acq On : 19 Dec 2019 08:43
Operator : SY/MD
Sample : BFB85
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB85

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Dec 20 07:12:45 2019

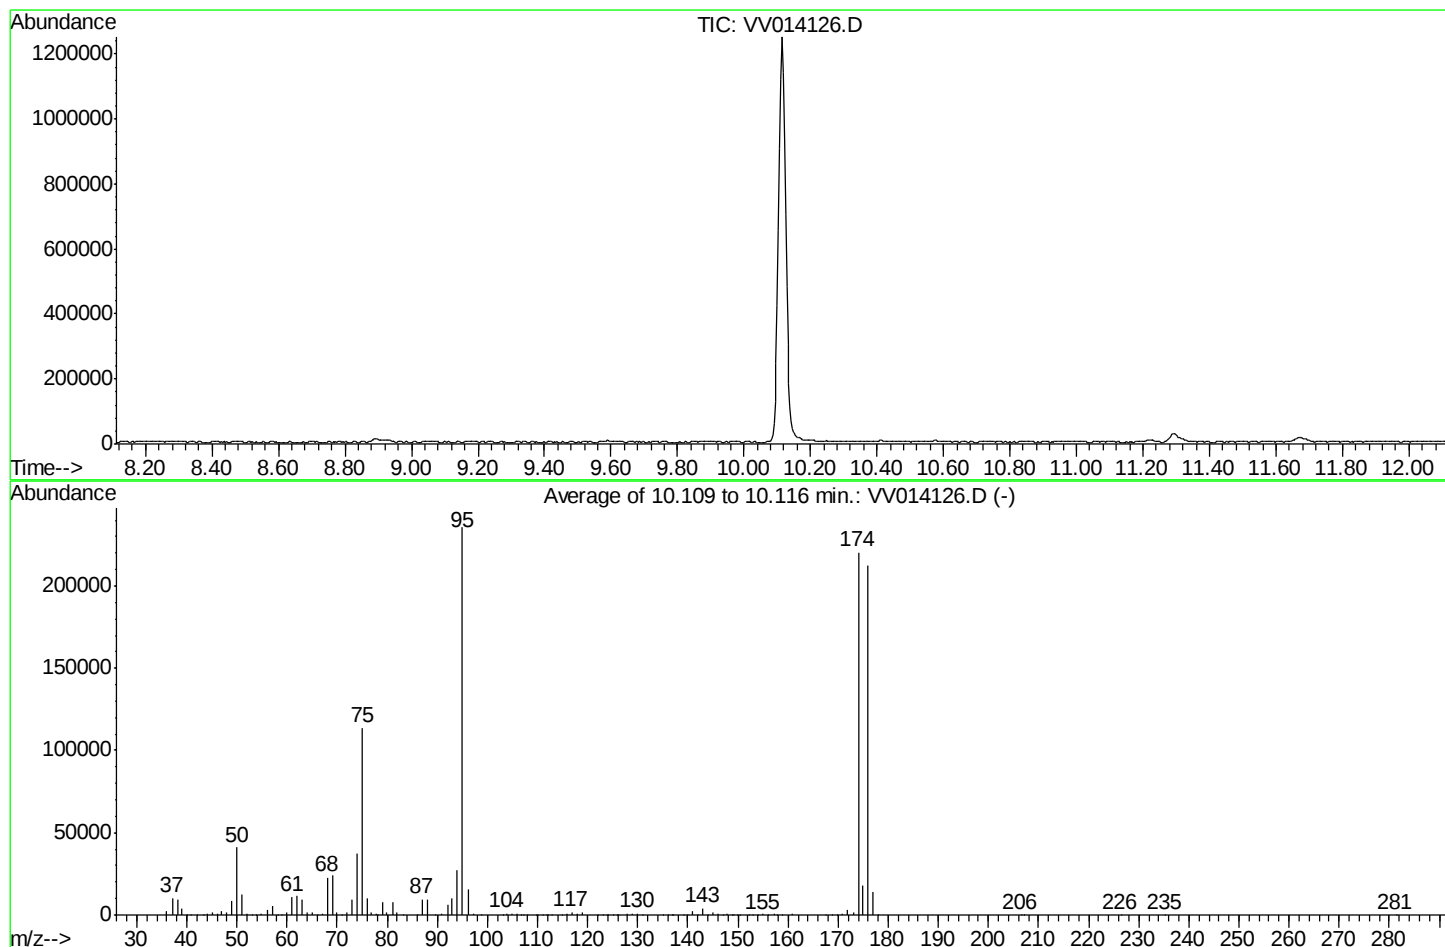

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	40950	PASS
75	95	30	80	48.2	113589	PASS
95	95	100	100	100.0	235605	PASS
96	95	5	9	6.7	15836	PASS
173	174	0.00	2	0.6	1239	PASS
174	95	50	120	93.6	220416	PASS
175	174	5	9	8.0	17712	PASS
176	174	95	101	96.2	212032	PASS
177	176	5	9	6.8	14394	PASS

m/z	Abundance
35.30	174.0
36.00	2249.0
37.10	9958.0
38.10	9015.0
39.10	4102.0
39.90	827.0
40.70	270.0
42.10	128.0
42.80	190.0
44.00	1642.0
45.00	1849.0
46.30	512.0
47.00	2302.0
47.90	1560.0
49.00	7896.0
50.10	38840.0
51.00	12315.0
52.00	643.0
53.00	373.0
53.80	229.0
54.90	644.0
56.10	3240.0
57.10	5407.0
58.00	363.0
60.00	1729.0
61.00	10953.0
62.00	11259.0
63.10	8925.0
64.00	1794.0
64.90	1855.0
66.00	411.0
66.90	602.0
68.00	20616.0
69.00	22800.0
70.00	1768.0
71.00	198.0
72.00	1257.0
73.10	9299.0
74.00	35040.0
75.10	104992.0
76.10	8976.0
76.90	1389.0
77.90	1178.0
79.00	7262.0
80.00	1762.0
81.00	7204.0
81.90	1539.0
83.10	160.0
87.00	8958.0
88.00	8296.0
89.50	117.0
90.90	949.0
92.00	6271.0
93.00	9579.0
94.00	26672.0
95.00	221376.0
96.10	15491.0
97.10	596.0
98.70	118.0
103.10	173.0
103.90	731.0
104.90	424.0
105.90	703.0
106.80	208.0
108.10	164.0
110.10	145.0
111.20	198.0
111.80	143.0
112.80	146.0
115.00	331.0
115.90	760.0
116.80	1639.0
117.90	983.0
118.90	1312.0
123.80	144.0
125.90	116.0
127.80	799.0
128.90	394.0
130.00	1039.0
131.00	387.0
135.10	401.0
136.10	111.0
136.70	351.0
137.10	341.0
139.00	130.0
139.90	351.0
141.00	2177.0
142.00	343.0
143.00	3776.0
144.10	300.0
145.00	1690.0
146.10	497.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

147.80	644.0
148.70	158.0
149.10	145.0
149.90	277.0
150.30	212.0
152.30	213.0
152.80	229.0
153.90	224.0
155.00	633.0
157.10	364.0
158.90	238.0
160.90	382.0
167.50	124.0
168.80	112.0
169.70	128.0
170.90	821.0
172.00	3033.0
173.10	3717.0
174.00	200320.0
175.00	17104.0
176.00	191296.0
177.00	13810.0
178.00	322.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	2537.0
37.10	10761.0
38.10	9755.0
39.00	4238.0
40.00	817.0
42.00	117.0
42.90	199.0
44.10	1736.0
45.10	1964.0
46.30	451.0
47.00	2670.0
48.00	1657.0
49.10	8620.0
50.10	42344.0
51.00	13140.0
52.00	743.0
53.00	398.0
53.80	199.0
54.90	739.0
56.10	3415.0
57.10	5935.0
58.00	368.0
59.00	121.0
60.00	1855.0
61.00	11618.0
62.00	11662.0
63.10	9501.0
64.00	1737.0
65.00	2055.0
66.00	410.0
67.00	741.0
68.00	23664.0
69.00	25056.0
70.00	1803.0
71.00	159.0
72.00	1553.0
73.00	10096.0
74.00	39080.0
75.10	117176.0
76.10	10264.0
76.90	1589.0
77.90	1250.0
79.00	7713.0
80.00	2026.0
81.00	7586.0
82.00	1712.0
83.10	251.0
86.10	398.0
87.00	9723.0
88.00	9112.0
89.50	149.0
90.90	1118.0
92.00	6925.0
93.00	10655.0
94.00	28088.0
95.00	243200.0
96.10	16318.0
97.10	588.0
103.10	137.0
103.90	850.0
104.90	563.0
105.90	731.0
106.70	234.0
108.10	132.0
110.00	109.0
111.10	196.0
111.70	146.0
112.00	153.0
112.90	196.0
114.80	362.0
115.90	816.0
116.80	1819.0
117.90	936.0
119.00	1480.0
123.70	126.0
126.10	133.0
127.90	781.0
128.90	497.0
130.00	1178.0
130.90	391.0
134.90	377.0
136.00	104.0
136.70	436.0
137.10	358.0
139.00	152.0
139.90	316.0
141.00	2446.0
142.10	411.0
143.00	4288.0
145.00	1841.0
146.00	521.0
147.20	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

147.90	696.0
148.90	138.0
149.90	308.0
150.20	283.0
152.20	261.0
152.80	267.0
153.80	277.0
155.00	635.0
156.00	160.0
157.10	449.0
157.80	111.0
158.90	377.0
160.90	456.0
168.80	138.0
170.90	968.0
171.90	3512.0
174.00	227968.0
175.00	18304.0
176.00	218752.0
177.00	14966.0
177.90	367.0
206.50	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	2463.0
37.10	10542.0
38.10	9760.0
39.00	4200.0
40.10	901.0
41.90	153.0
43.30	321.0
44.00	1837.0
45.20	1909.0
46.10	427.0
47.00	2727.0
48.00	1534.0
49.10	8878.0
50.10	42136.0
51.10	12877.0
52.00	796.0
53.10	382.0
53.90	211.0
54.90	707.0
56.10	3164.0
57.10	6170.0
58.00	338.0
58.90	156.0
60.00	1969.0
61.00	11143.0
62.00	11177.0
63.00	9109.0
64.10	1607.0
65.00	2119.0
66.00	381.0
67.10	847.0
68.00	24464.0
69.00	23720.0
70.00	1818.0
71.00	168.0
72.00	1720.0
73.00	9801.0
74.00	39128.0
75.10	118600.0
76.00	10302.0
77.00	1587.0
78.10	1145.0
79.00	7403.0
79.90	2051.0
81.00	7460.0
82.00	1715.0
83.10	330.0
86.10	464.0
87.00	9982.0
88.00	9538.0
89.50	156.0
91.00	1245.0
92.00	6671.0
93.00	10702.0
94.00	27744.0
95.00	242240.0
96.10	15701.0
97.10	484.0
103.00	145.0
103.90	950.0
104.90	540.0
105.90	764.0
106.70	248.0
107.20	187.0
108.00	128.0
109.70	115.0
111.00	225.0
111.60	183.0
112.10	192.0
112.90	199.0
114.80	405.0
115.90	833.0
116.80	1827.0
117.90	803.0
119.00	1563.0
121.90	120.0
123.00	121.0
124.10	100.0
124.70	130.0
125.10	132.0
126.10	165.0
127.90	734.0
128.90	512.0
130.00	1115.0
130.90	343.0
134.80	421.0
136.70	402.0
137.10	355.0
139.00	132.0
139.90	235.0
140.90	2395.0
142.10	404.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

143.00	4532.0
144.90	1773.0
146.00	453.0
147.00	211.0
148.00	650.0
148.80	160.0
149.90	343.0
152.20	217.0
152.90	260.0
153.80	282.0
155.00	639.0
156.00	169.0
157.20	454.0
157.90	125.0
158.90	437.0
160.90	504.0
168.90	128.0
170.90	1032.0
171.90	3533.0
174.00	232960.0
175.00	17728.0
176.00	226048.0
177.00	14407.0
177.90	409.0
206.50	109.0
207.10	175.0
226.40	103.0
235.20	103.0
281.40	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.30	117.0
35.90	160.0
36.30	143.0
36.80	104.0
37.50	159.0
38.20	172.0
38.80	145.0
40.00	803.0
41.00	212.0
41.60	136.0
42.40	170.0
42.80	186.0
44.00	923.0
45.00	156.0
46.70	130.0
49.90	156.0
51.50	105.0
54.40	174.0
55.00	196.0
57.40	113.0
58.20	137.0
65.00	110.0
66.60	141.0
69.30	177.0
71.70	118.0
76.80	102.0
85.90	101.0
87.50	117.0
101.50	152.0
112.50	109.0
115.30	154.0
122.20	113.0
124.80	110.0
137.80	121.0
280.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85