
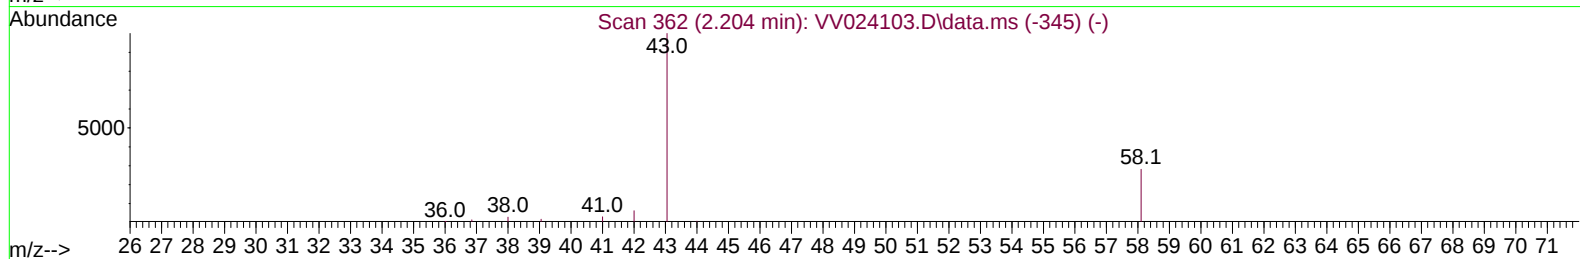
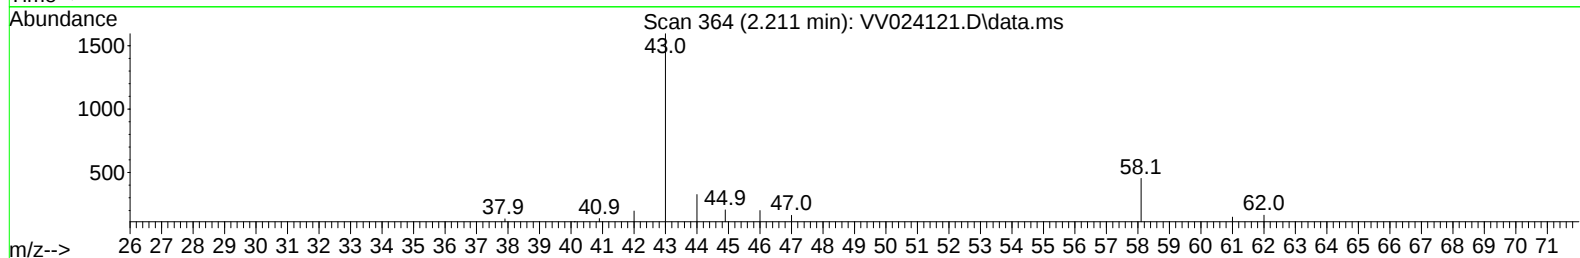


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024121.D
Acq On : 20 Dec 2021 04:35
Operator : SY/MD
Sample : M5148-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Dec 20 05:38:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 04:04:22 2021
Response via : Initial Calibration

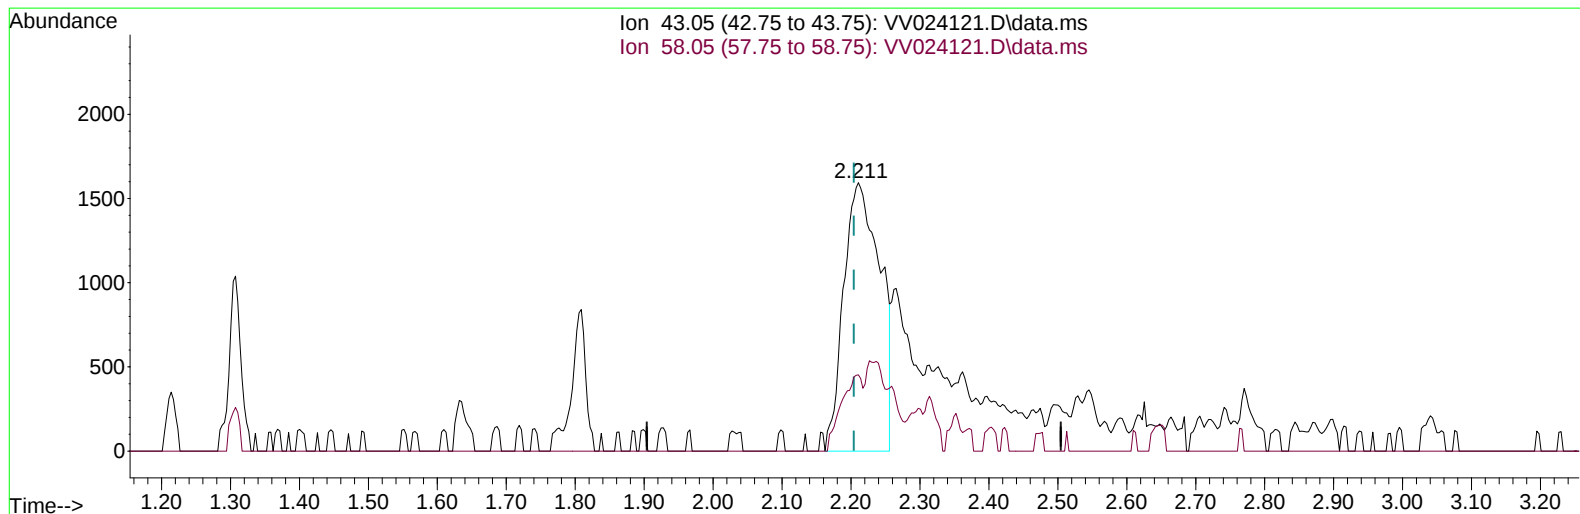

TIC: VV024121.D\data.ms

(13) Acetone (T)

2.211min (+ 0.006) 8.02 ug/L

response 5817

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	16.50
0.00	0.00	0.00
0.00	0.00	0.00