




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024087.D
 Acq On : 19 Dec 2021 14:41
 Operator : SY/MD
 Sample : M5134-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK2

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:36:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

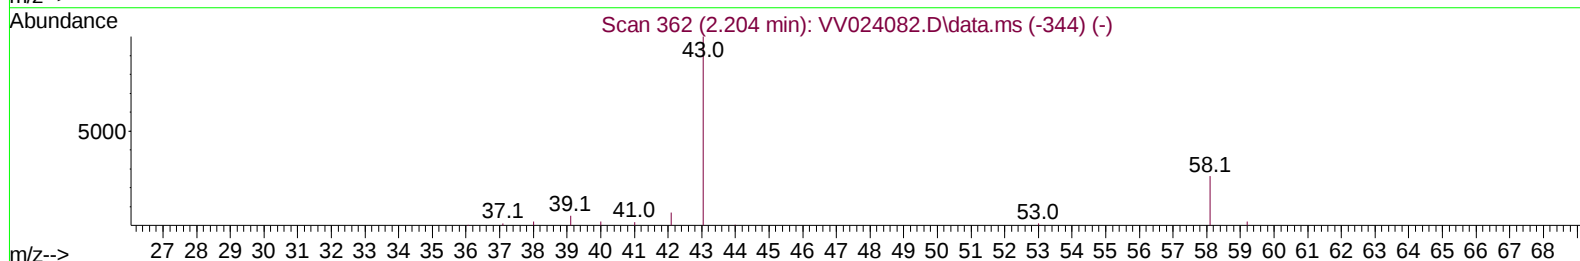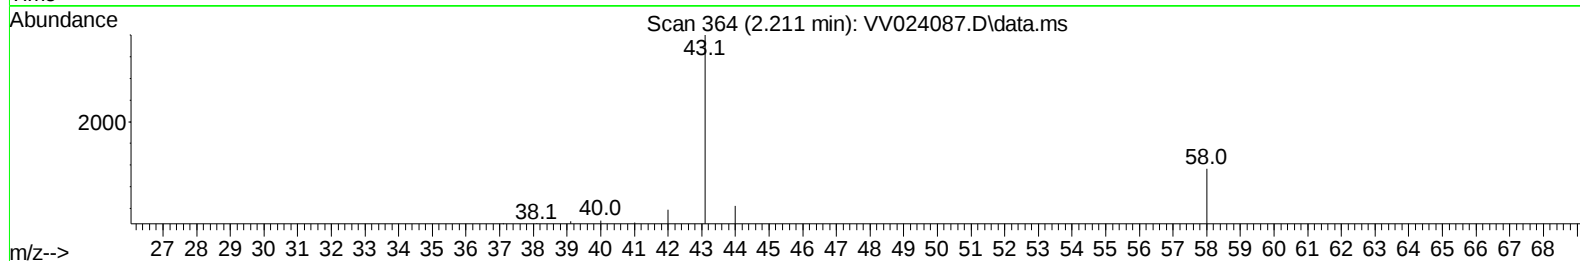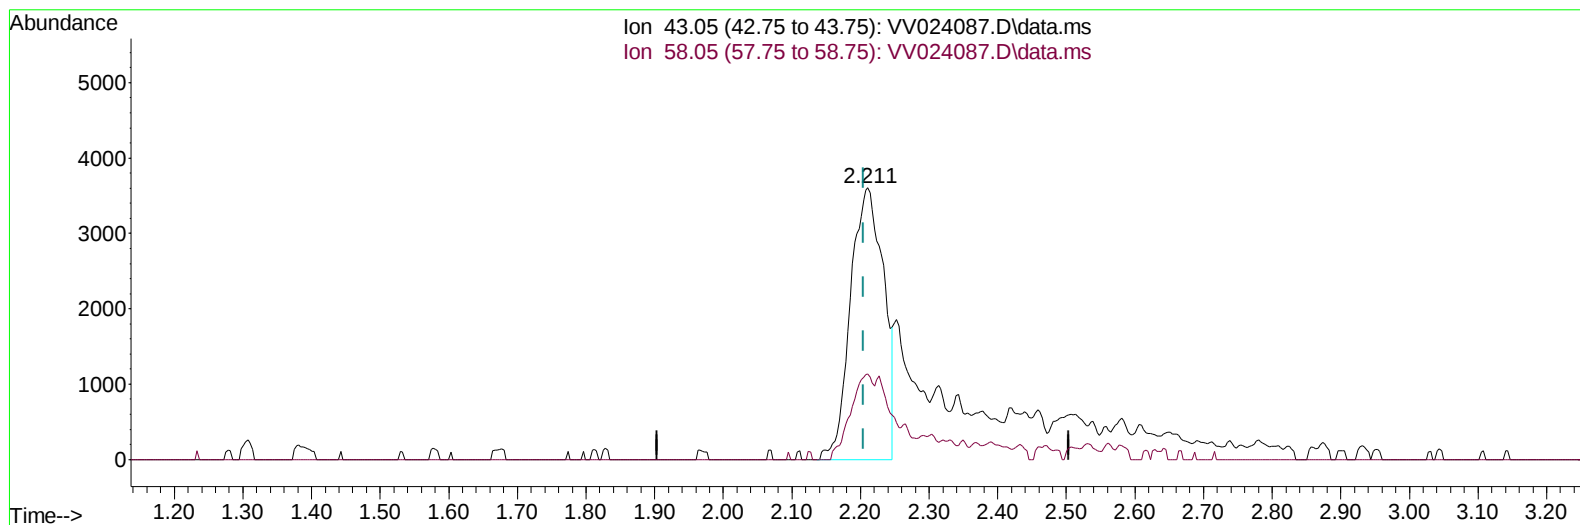

TIC: VV024087.D\data.ms

(13) Acetone (T)

2.211min (+ 0.007) 13.60 ug/L

response 12131

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	21.84
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024087.D
 Acq On : 19 Dec 2021 14:41
 Operator : SY/MD
 Sample : M5134-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK2

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:36:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

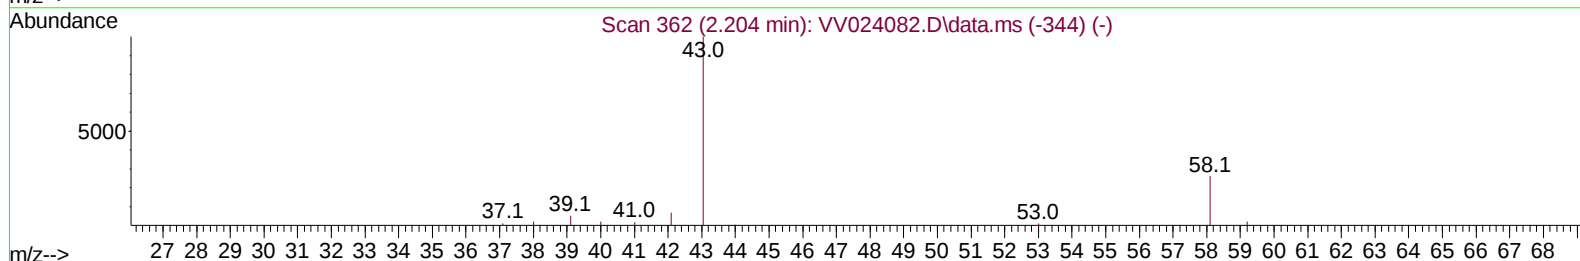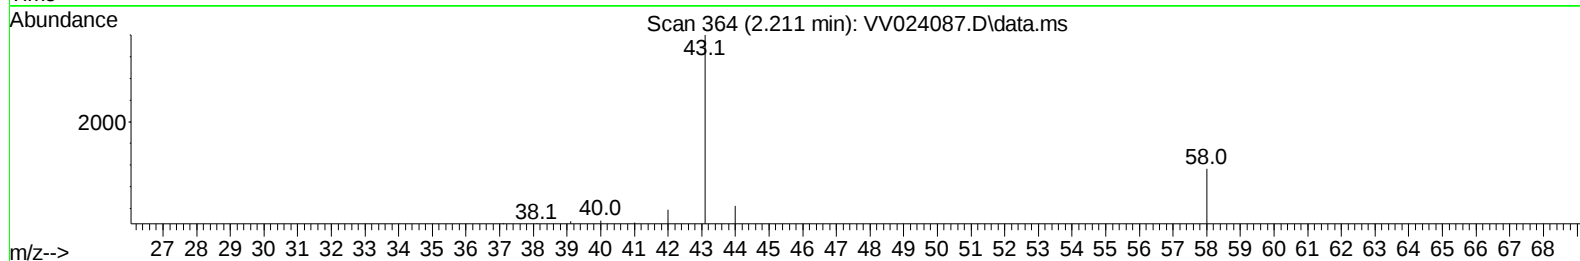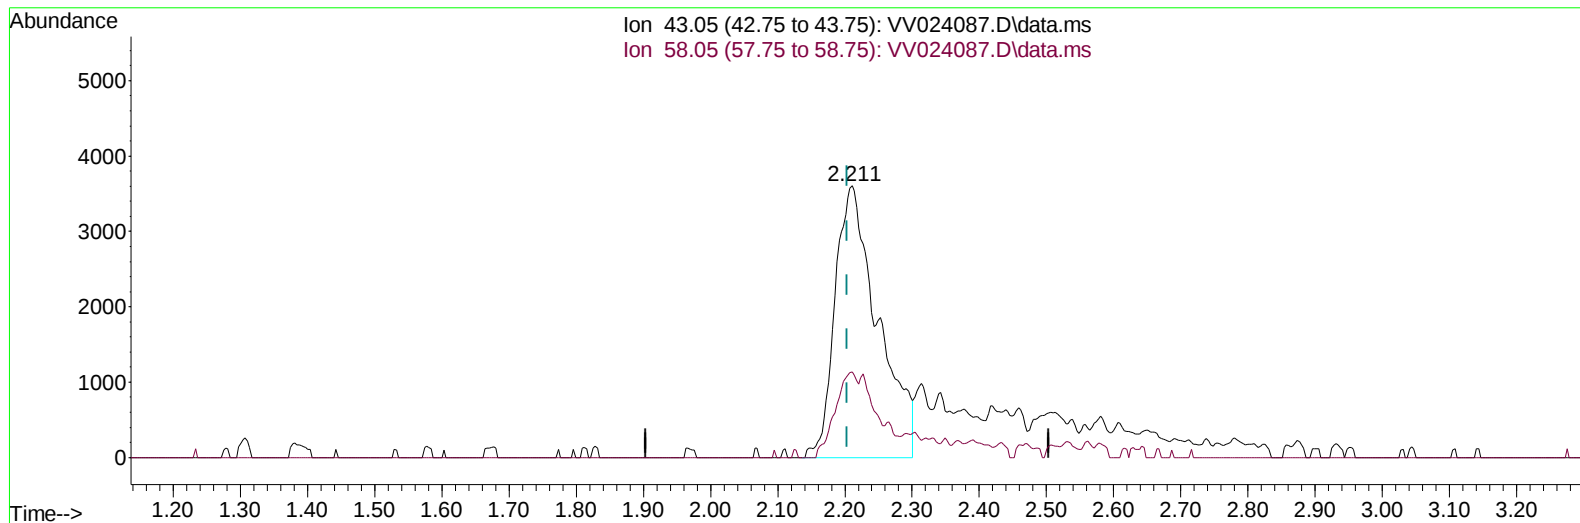

TIC: VV024087.D\data.ms

(13) Acetone (T)

2.211min (+ 0.007) 17.93 ug/L m

response 15997

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	16.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024087.D
 Acq On : 19 Dec 2021 14:41
 Operator : SY/MD
 Sample : M5134-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:36:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

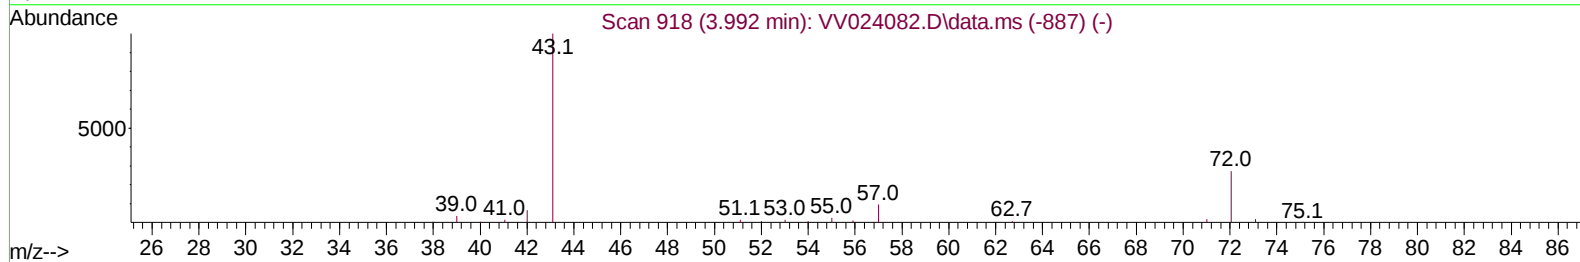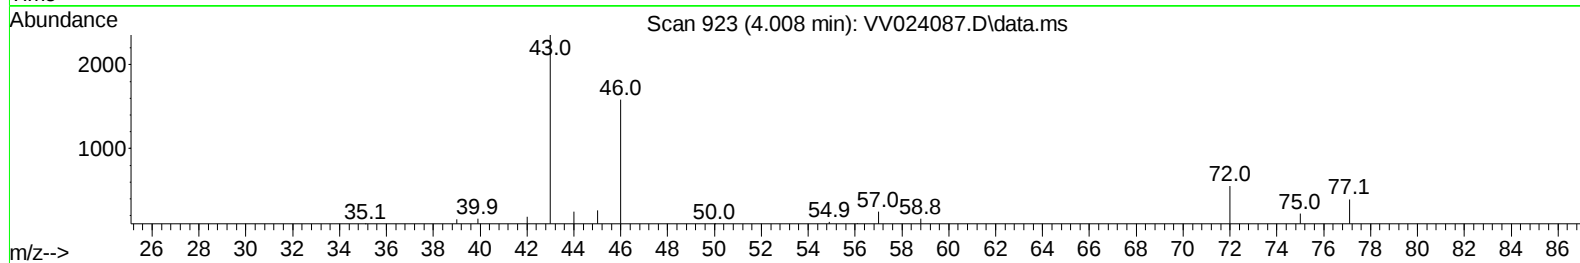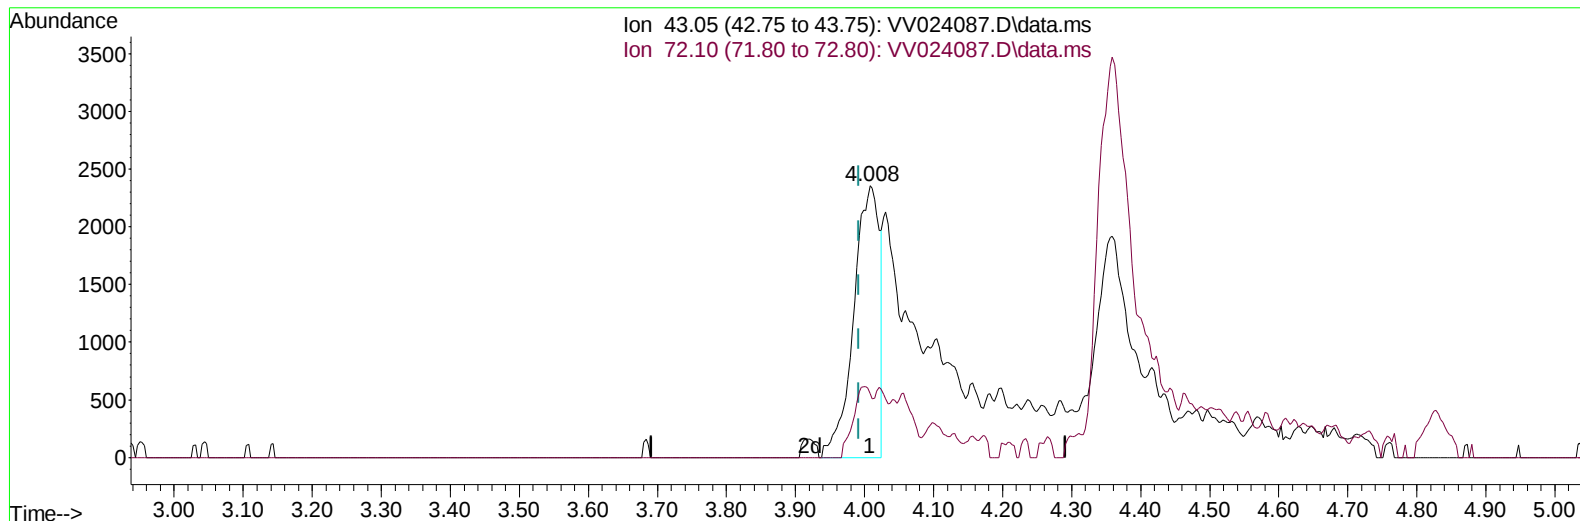

TIC: VV024087.D\data.ms

(21) 2-Butanone (T)

4.008min (+ 0.016) 4.83 ug/L

response 6153

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	22.10	18.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024087.D
 Acq On : 19 Dec 2021 14:41
 Operator : SY/MD
 Sample : M5134-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK2

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:36:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

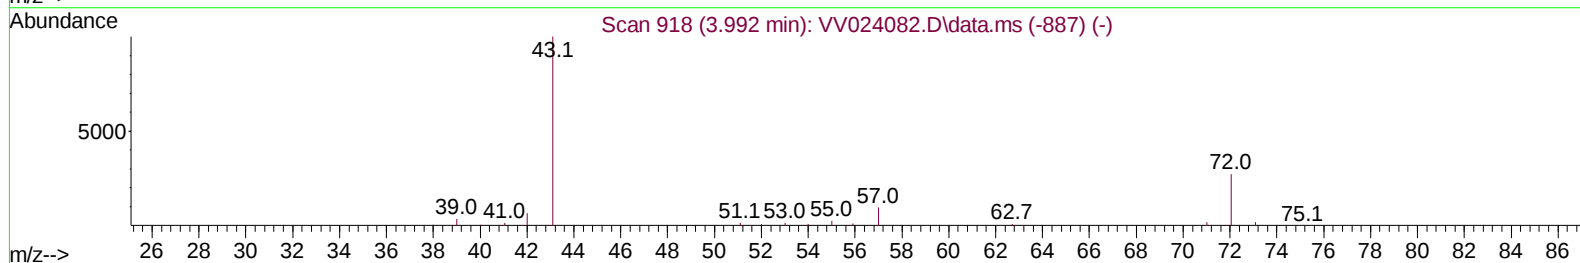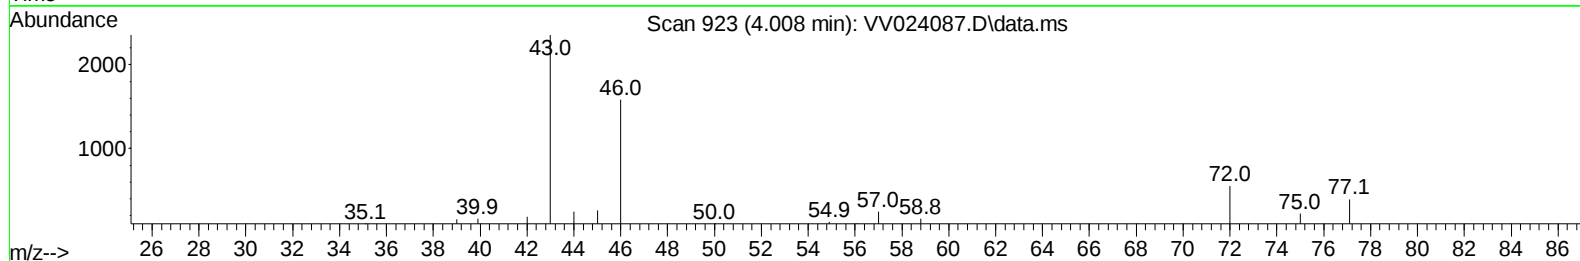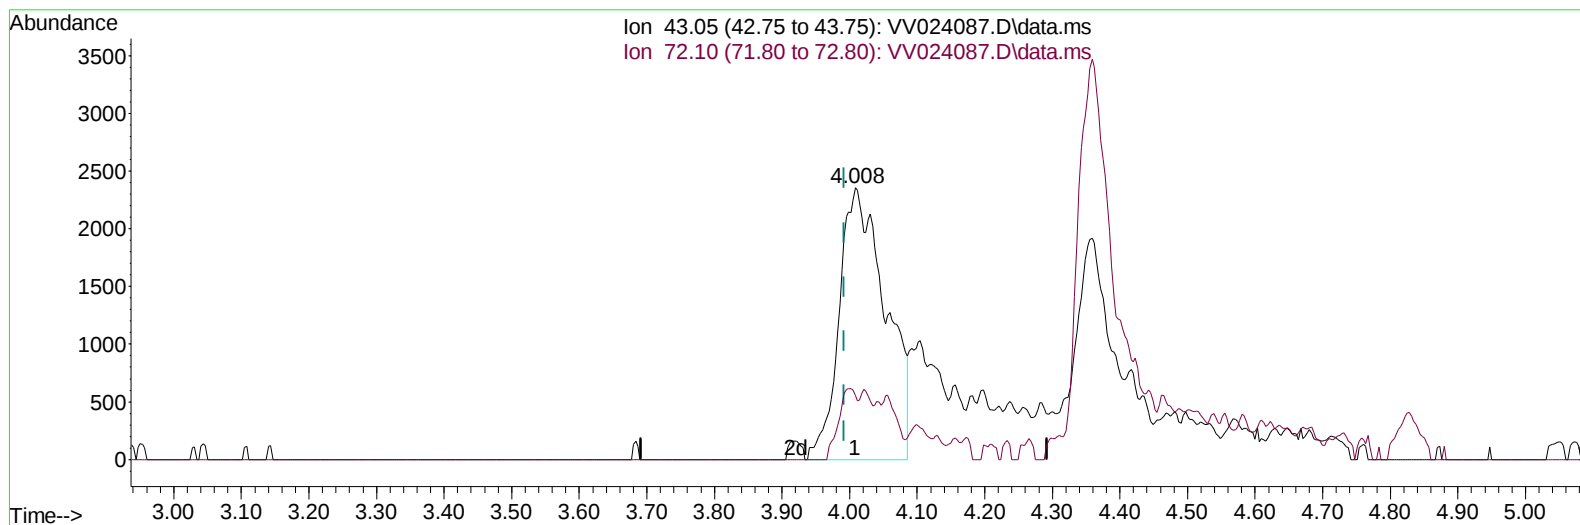

TIC: VV024087.D\data.ms

(21) 2-Butanone (T)

4.008min (+ 0.016) 8.82 ug/L m

response 11245

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	22.10	10.14#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024087.D
 Acq On : 19 Dec 2021 14:41
 Operator : SY/MD
 Sample : M5134-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK2

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:36:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Reviewed By : John Carlone 12/20/2021
 Supervised By : Mahesh Dadoda 12/22/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	106156	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	110104	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57095	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	18965	3.323	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery =	66.400%		
7) Chloroethane-d5	1.568	69	17386	3.651	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery =	73.000%		
11) 1,1-Dichloroethene-d2	2.108	63	30621	2.749	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery =	55.000%#		
20) 2-Butanone-d5	3.921	46	31606	28.348	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery =	56.700%		
24) Chloroform-d	4.349	84	47553	3.679	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	73.600%		
26) 1,2-Dichloroethane-d4	5.034	65	23275	3.867	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	77.400%		
32) Benzene-d6	5.050	84	86982	3.989	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	79.800%		
36) 1,2-Dichloropropane-d6	6.069	67	25649	3.898	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery =	78.000%		
41) Toluene-d8	7.317	98	76956	3.920	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	78.400%		
43) trans-1,3-Dichloroprop...	7.625	79	9161	3.356	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery =	67.200%		
46) 2-Hexanone-d5	8.092	63	32983	26.994	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery =	53.980%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	17279	3.166	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery =	63.400%#		
66) 1,2-Dichlorobenzene-d4	11.625	152	32979	4.324	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery =	86.400%		
Target Compounds						
						Qvalue
13) Acetone	2.211	43	15997m	17.934	ug/L	
21) 2-Butanone	4.008	43	11245m	8.823	ug/L	
31) Carbon tetrachloride	4.828	117	95814	7.076	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024087.D
Acq On : 19 Dec 2021 14:41
Operator : SY/MD
Sample : M5134-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBK2

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:36:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

