




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024094.D
 Acq On : 19 Dec 2021 17:27
 Operator : SY/MD
 Sample : M5134-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:38:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

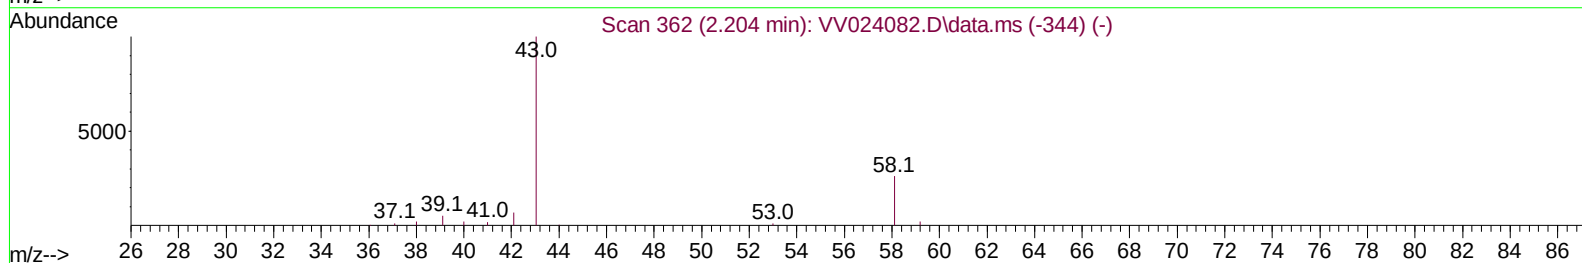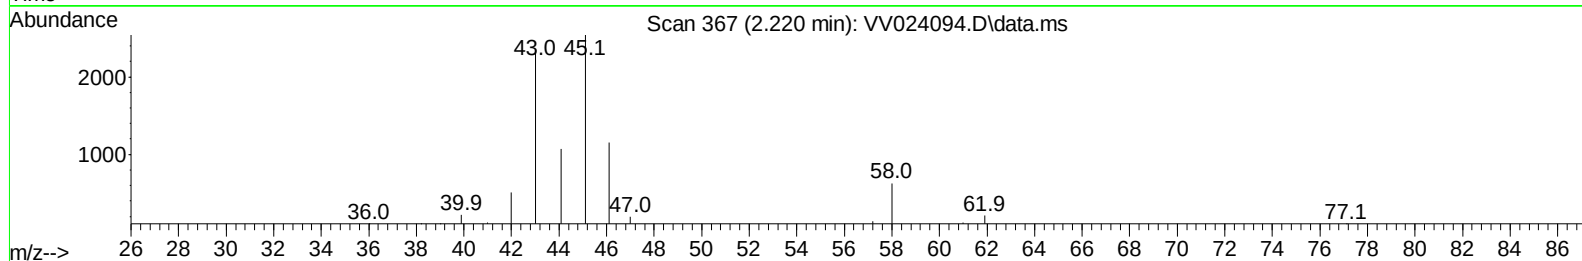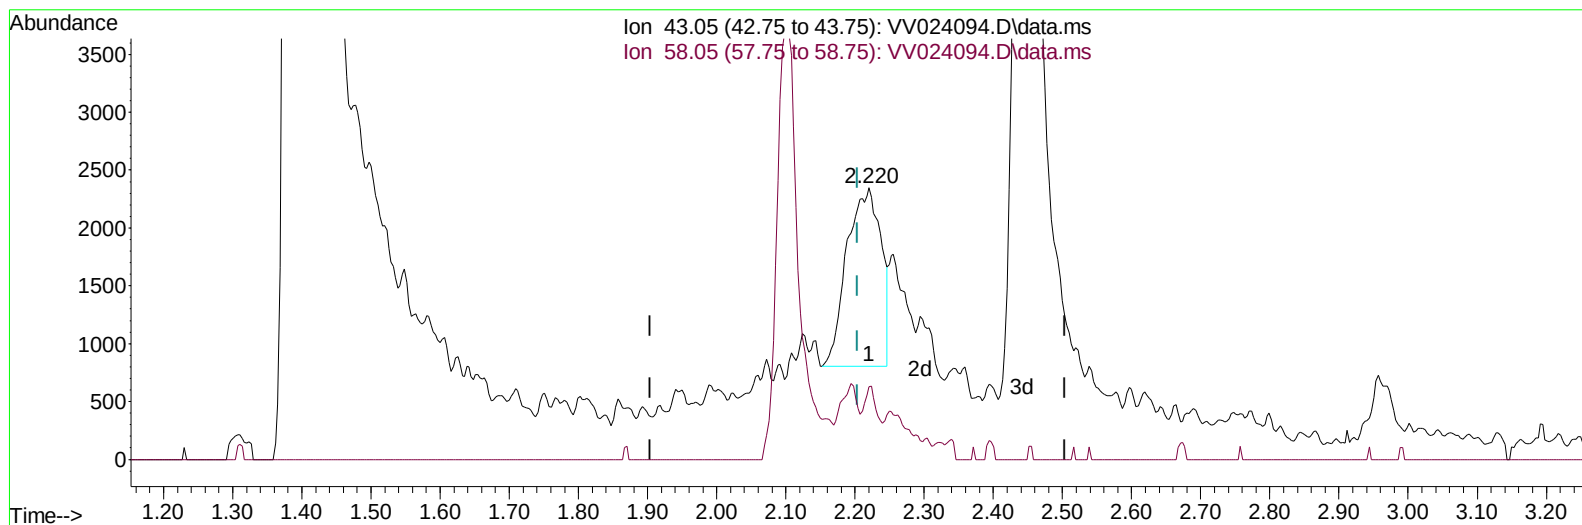

TIC: VV024094.D\data.ms

(13) Acetone (T)

2.220min (+ 0.016) 6.69 ug/L

response 5272

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	13.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024094.D
Acq On : 19 Dec 2021 17:27
Operator : SY/MD
Sample : M5134-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBK7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:38:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

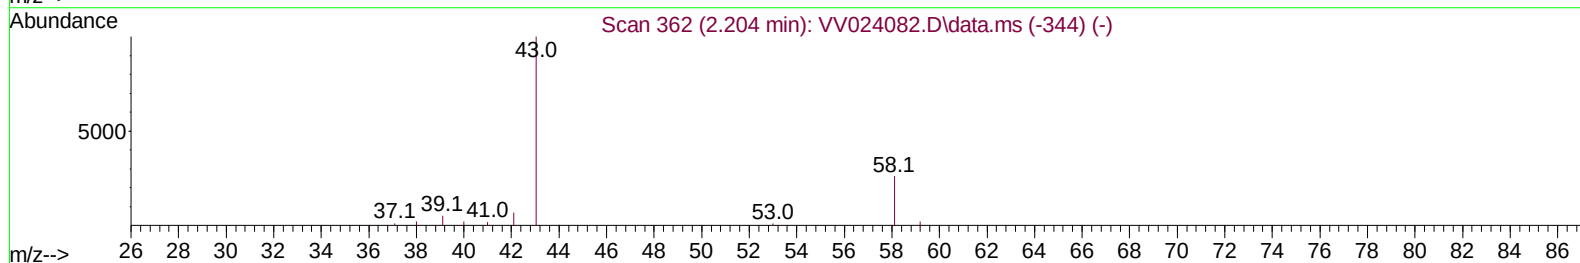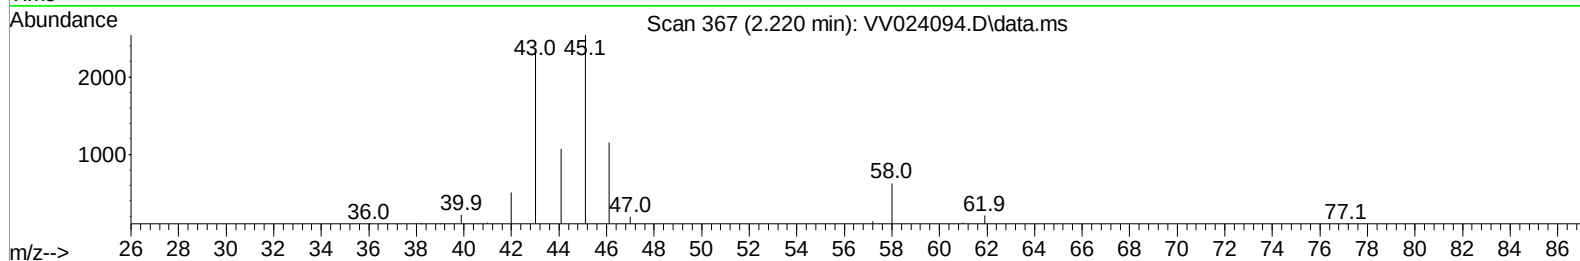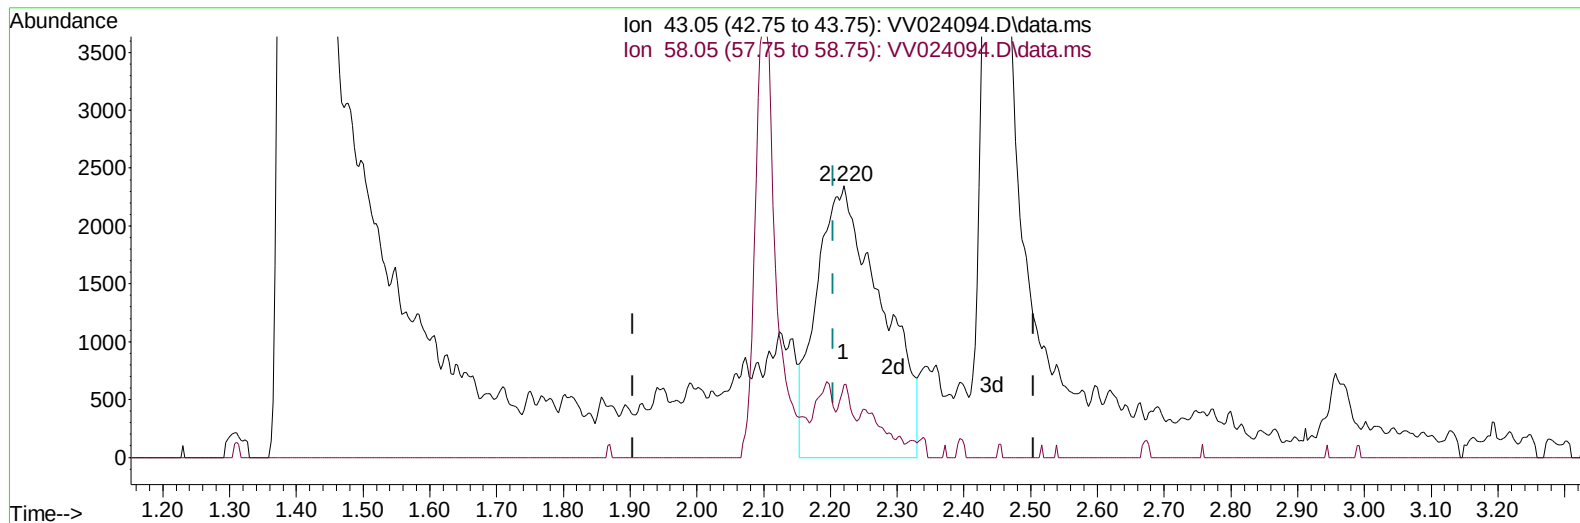

TIC: VV024094.D\data.ms

(13) Acetone (T)

2.220min (+ 0.016) 20.17 ug/L m

response 15882

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	4.42
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024094.D
 Acq On : 19 Dec 2021 17:27
 Operator : SY/MD
 Sample : M5134-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:38:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	93718	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	98376	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60308	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	26916	5.342	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 106.800%			
7) Chloroethane-d5	1.568	69	24163	5.748	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 115.000%			
11) 1,1-Dichloroethene-d2	2.108	63	43766	4.450	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 89.000%			
20) 2-Butanone-d5	3.915	46	46394	47.133	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 94.260%			
24) Chloroform-d	4.349	84	68268	5.982	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 119.600%			
26) 1,2-Dichloroethane-d4	5.034	65	32122	6.045	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 121.000%			
32) Benzene-d6	5.050	84	127262	6.531	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 130.600%#			
36) 1,2-Dichloropropane-d6	6.069	67	37267	6.339	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 126.800%			
41) Toluene-d8	7.317	98	118248	6.741	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 134.800%#			
43) trans-1,3-Dichloroprop...	7.625	79	13477	5.526	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 110.600%			
46) 2-Hexanone-d5	8.092	63	48869	44.763	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 89.520%			
56) 1,1,2,2-Tetrachloroeth...	10.214	84	25764	5.283	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 105.600%			
66) 1,2-Dichlorobenzene-d4	11.625	152	51788	6.429	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 128.600%#			
Target Compounds						
13) Acetone	2.220	43	15882m	20.168	ug/L	
14) Carbon disulfide	2.298	76	4044	0.222	ug/L	99
15) Methyl Acetate	2.442	43	23803	12.470	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024094.D
Acq On : 19 Dec 2021 17:27
Operator : SY/MD
Sample : M5134-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
GBBK7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:38:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

