




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024096.D
 Acq On : 19 Dec 2021 18:15
 Operator : SY/MD
 Sample : M5134-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK9

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:39:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

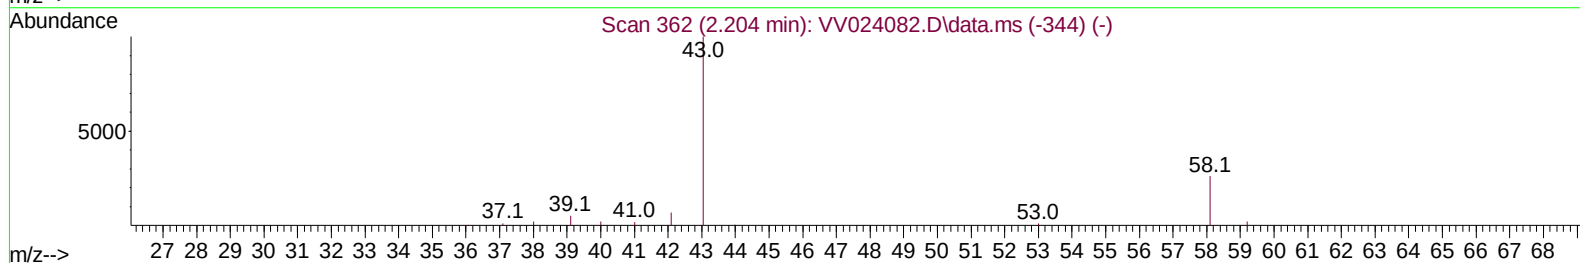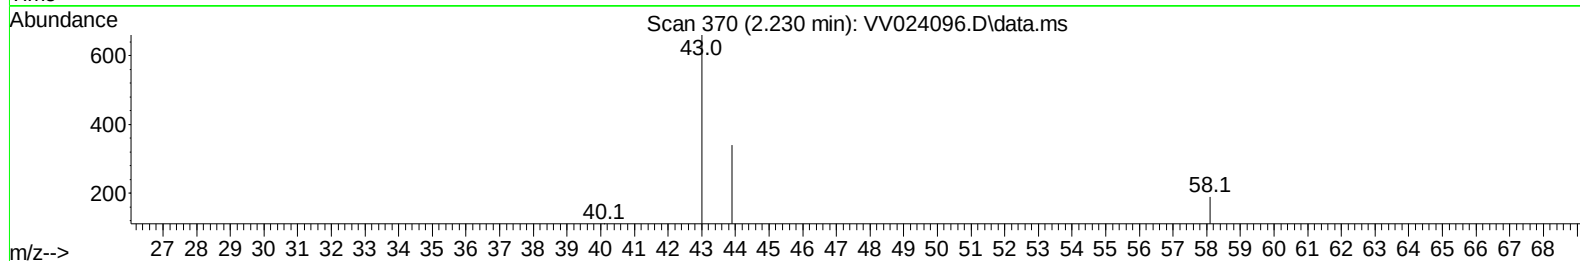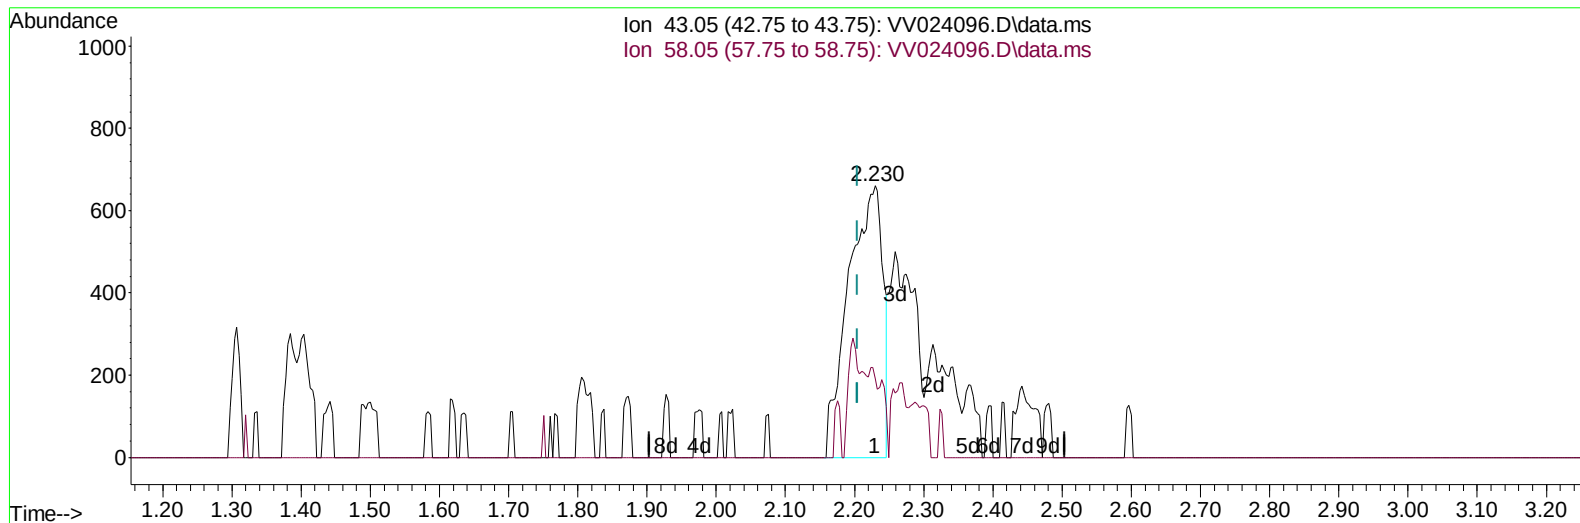

TIC: VV024096.D\data.ms

(13) Acetone (T)

2.230min (+ 0.026) 3.09 ug/L

response 2262

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	20.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024096.D
 Acq On : 19 Dec 2021 18:15
 Operator : SY/MD
 Sample : M5134-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK9

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:39:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

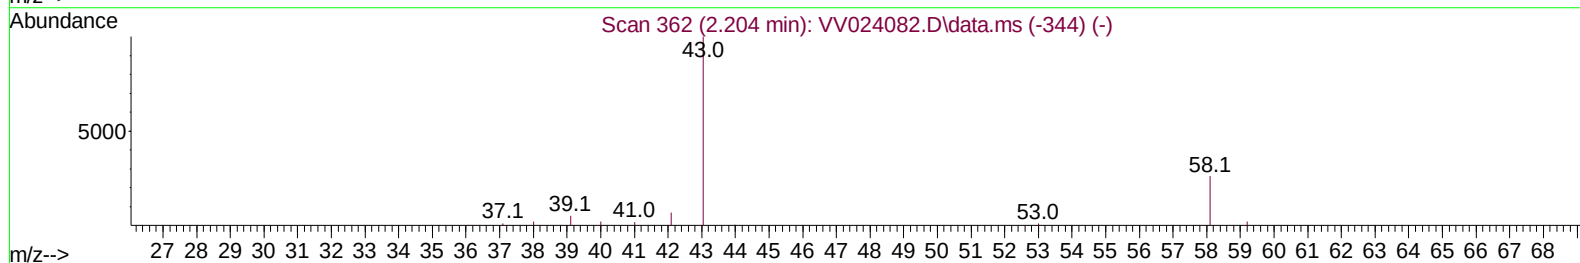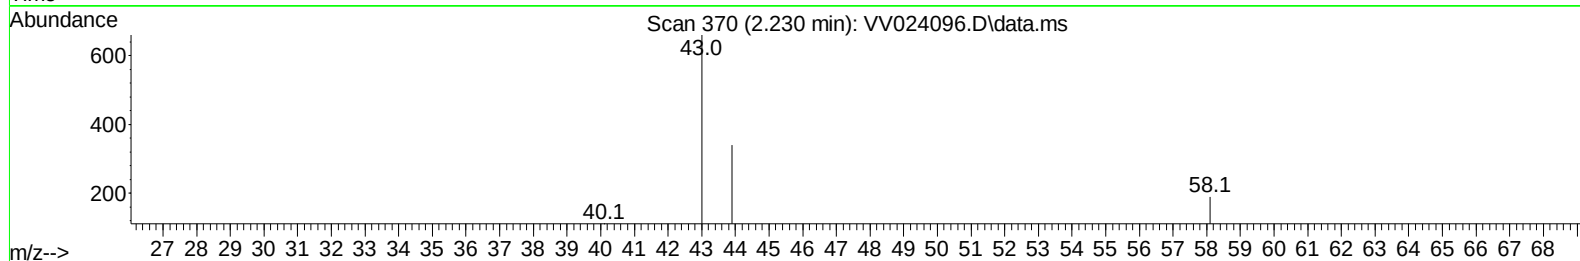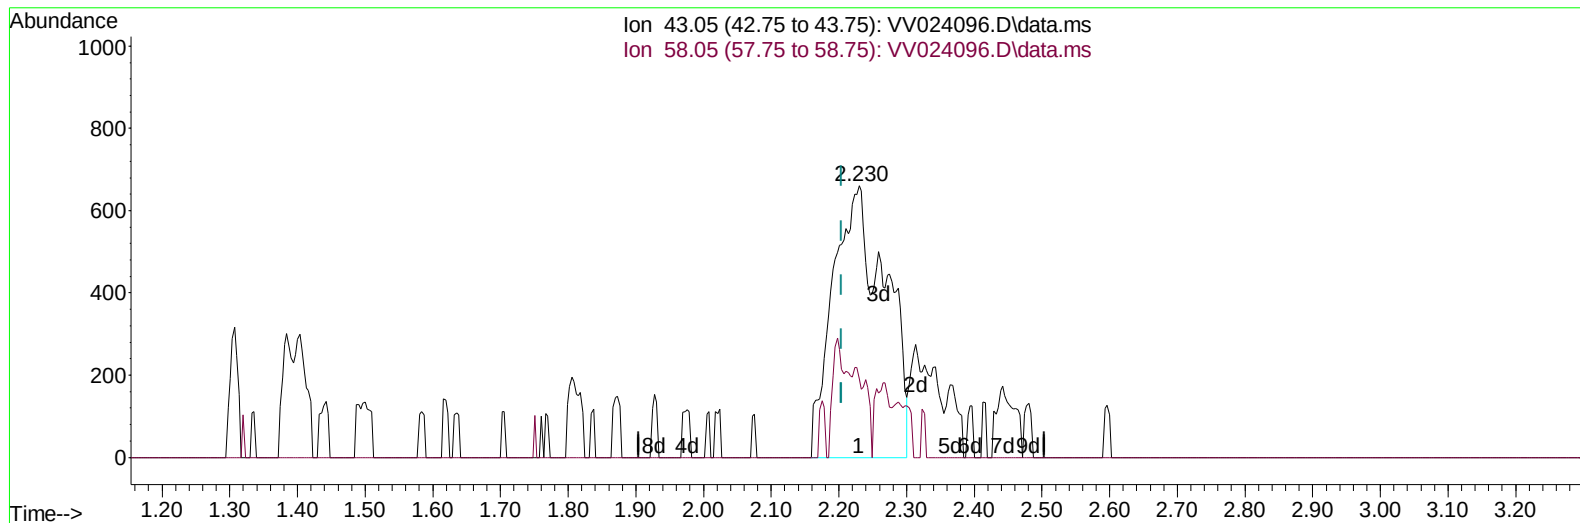

TIC: VV024096.D\data.ms

(13) Acetone (T)

2.230min (+ 0.026) 4.82 ug/L m

response 3523

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	12.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024096.D
 Acq On : 19 Dec 2021 18:15
 Operator : SY/MD
 Sample : M5134-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK9

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 12/20/2021
 Supervised By : Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:39:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	87031	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	92195	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	46661	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	18372	3.927	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	78.600%		
7) Chloroethane-d5	1.568	69	17652	4.522	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	90.400%		
11) 1,1-Dichloroethene-d2	2.108	63	29839	3.267	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	65.400%		
20) 2-Butanone-d5	3.918	46	44707	48.909	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	97.820%		
24) Chloroform-d	4.349	84	47790	4.509	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	90.200%		
26) 1,2-Dichloroethane-d4	5.037	65	24195	4.903	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.000%		
32) Benzene-d6	5.050	84	85785	4.698	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	94.000%		
36) 1,2-Dichloropropane-d6	6.069	67	25731	4.671	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	93.400%		
41) Toluene-d8	7.316	98	74653	4.541	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	90.800%		
43) trans-1,3-Dichloroprop...	7.625	79	9509	4.161	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	83.200%		
46) 2-Hexanone-d5	8.091	63	35421	34.620	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	69.240%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	16791	3.674	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	73.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	30635	4.915	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	98.400%		
Target Compounds						Qvalue
13) Acetone	2.230	43	3523m	4.817	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024096.D
Acq On : 19 Dec 2021 18:15
Operator : SY/MD
Sample : M5134-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
GBBK9

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:39:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

