




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024097.D
 Acq On : 19 Dec 2021 18:38
 Operator : SY/MD
 Sample : M5134-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBLO

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:39:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
 Supervised By :Mahesh Dadoda 12/22/2021

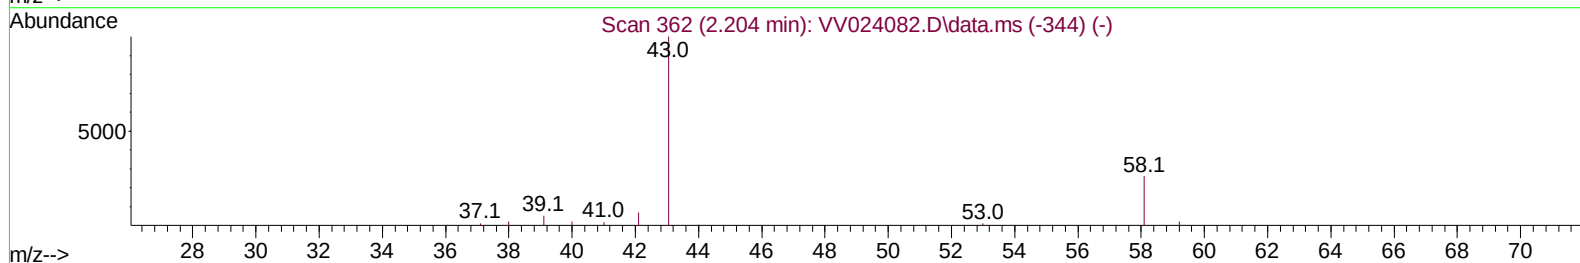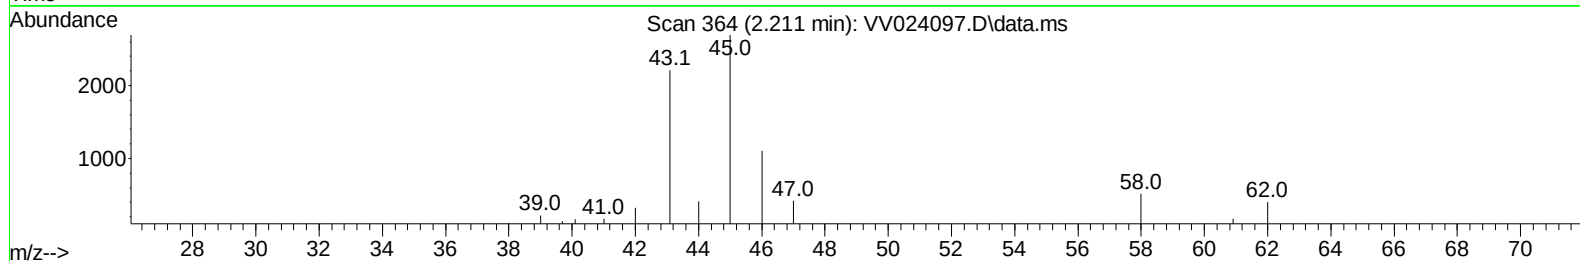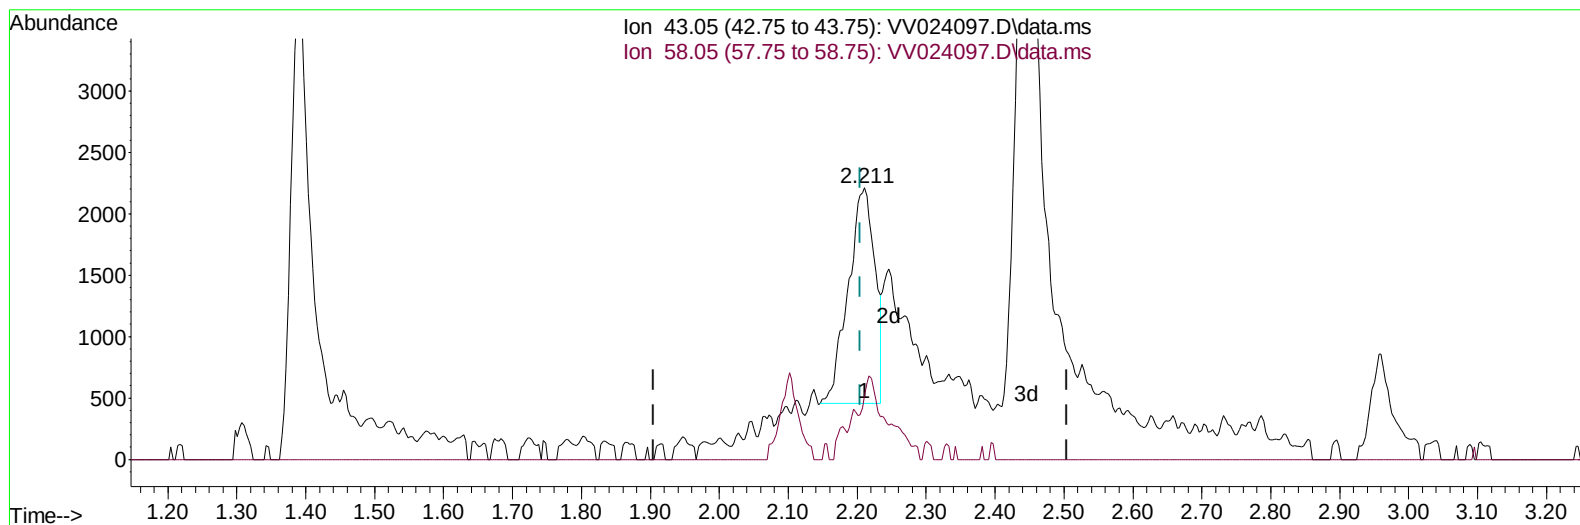

TIC: VV024097.D\data.ms

(13) Acetone (T)

2.211min (+ 0.007) 6.02 ug/L

response 4667

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	36.66
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024097.D
Acq On : 19 Dec 2021 18:38
Operator : SY/MD
Sample : M5134-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBL0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:39:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

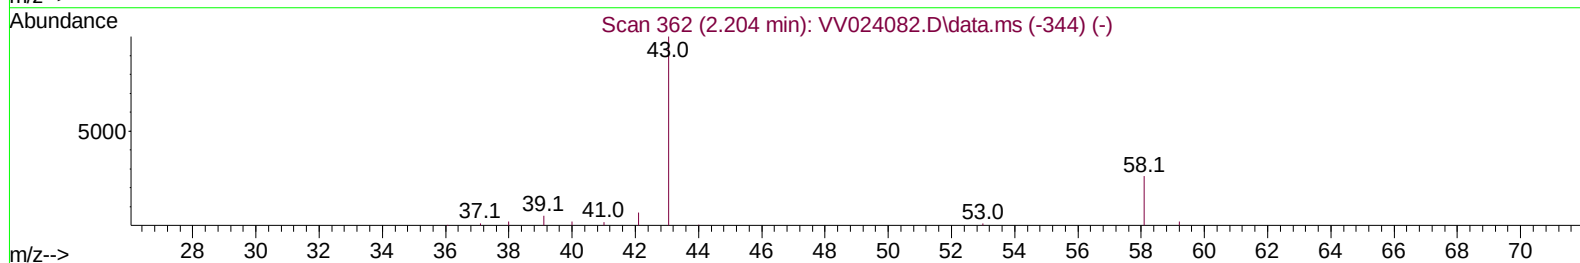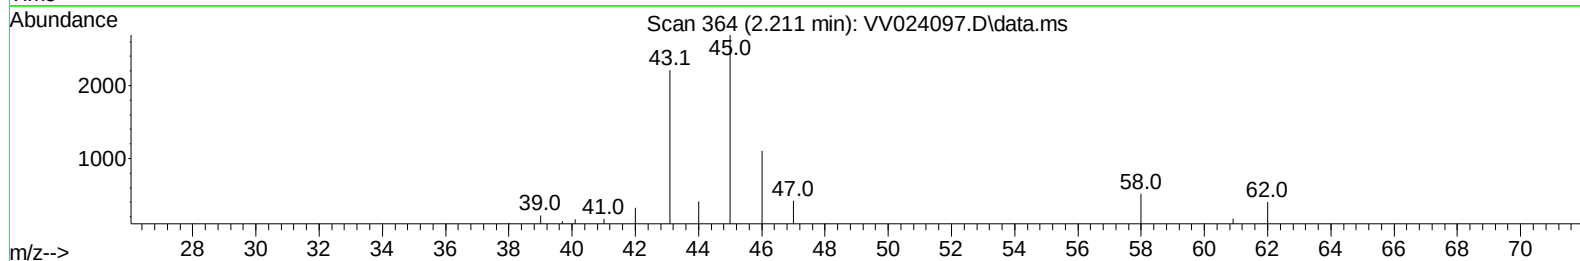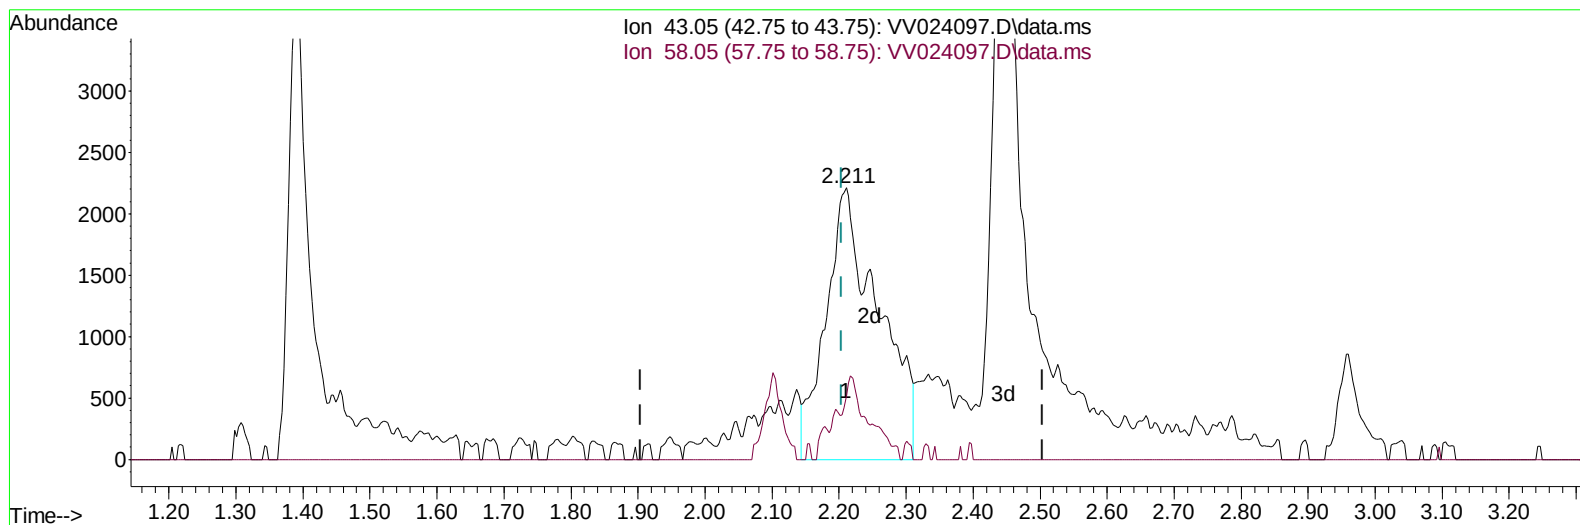

TIC: VV024097.D\data.ms

(13) Acetone (T)

2.211min (+ 0.007) 15.64 ug/L m

response 12136

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	14.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024097.D
 Acq On : 19 Dec 2021 18:38
 Operator : SY/MD
 Sample : M5134-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBLO

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:39:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Reviewed By : John Carlone 12/20/2021
 Supervised By : Mahesh Dadoda 12/22/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	92318	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	93792	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54619	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	18626	3.753	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	75.000%	
7) Chloroethane-d5	1.568	69	17341	4.188	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	83.800%	
11) 1,1-Dichloroethene-d2	2.108	63	29564	3.052	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	61.000%	
20) 2-Butanone-d5	3.915	46	35047	36.146	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	72.300%	
24) Chloroform-d	4.349	84	49148	4.372	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	87.400%	
26) 1,2-Dichloroethane-d4	5.034	65	22408	4.281	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	85.600%	
32) Benzene-d6	5.050	84	85300	4.592	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.800%	
36) 1,2-Dichloropropane-d6	6.069	67	25012	4.463	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	89.200%	
41) Toluene-d8	7.317	98	77105	4.610	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	92.200%	
43) trans-1,3-Dichloroprop...	7.625	79	8855	3.808	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	76.200%	
46) 2-Hexanone-d5	8.092	63	33799	32.472	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	64.940%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	18093	3.892	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	77.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	33656	4.613	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	92.200%	
Target Compounds						
13) Acetone	2.211	43	12136m	15.645	ug/L	
14) Carbon disulfide	2.298	76	2917	0.162	ug/L #	94
15) Methyl Acetate	2.446	43	12861	6.840	ug/L	99
25) Chloroform	4.378	83	48975	3.580	ug/L	97
31) Carbon tetrachloride	4.825	117	9221	0.799	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024097.D
Acq On : 19 Dec 2021 18:38
Operator : SY/MD
Sample : M5134-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBL0

Manual IntegrationsAPPROVED

Quant Time: Dec 20 01:39:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

