

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121921\
 Data File : VW024084.D
 Acq On : 19 Dec 2021 13:00
 Operator : SY/MD
 Sample : M5133-10DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBJ0DL

Quant Time: Dec 20 01:36:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	90231	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	94330	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	48059	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	19404	4.000	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.568	69	17612	4.352	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.000%
11) 1,1-Dichloroethene-d2	2.105	63	31975	3.377	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%
20) 2-Butanone-d5	3.912	46	29880	31.529	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	63.060%
24) Chloroform-d	4.349	84	48139	4.381	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.034	65	24214	4.733	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
32) Benzene-d6	5.050	84	87918	4.706	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
36) 1,2-Dichloropropane-d6	6.069	67	26820	4.758	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%
41) Toluene-d8	7.317	98	77437	4.604	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	7.622	79	9267	3.963	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.091	63	34625	33.076	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	66.160%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	17680	3.781	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	32323	5.035	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds						Qvalue
31) Carbon tetrachloride	4.825	117	37506	3.233	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024084.D
Acq On : 19 Dec 2021 13:00
Operator : SY/MD
Sample : M5133-10DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ0DL


Quant Time: Dec 20 01:36:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

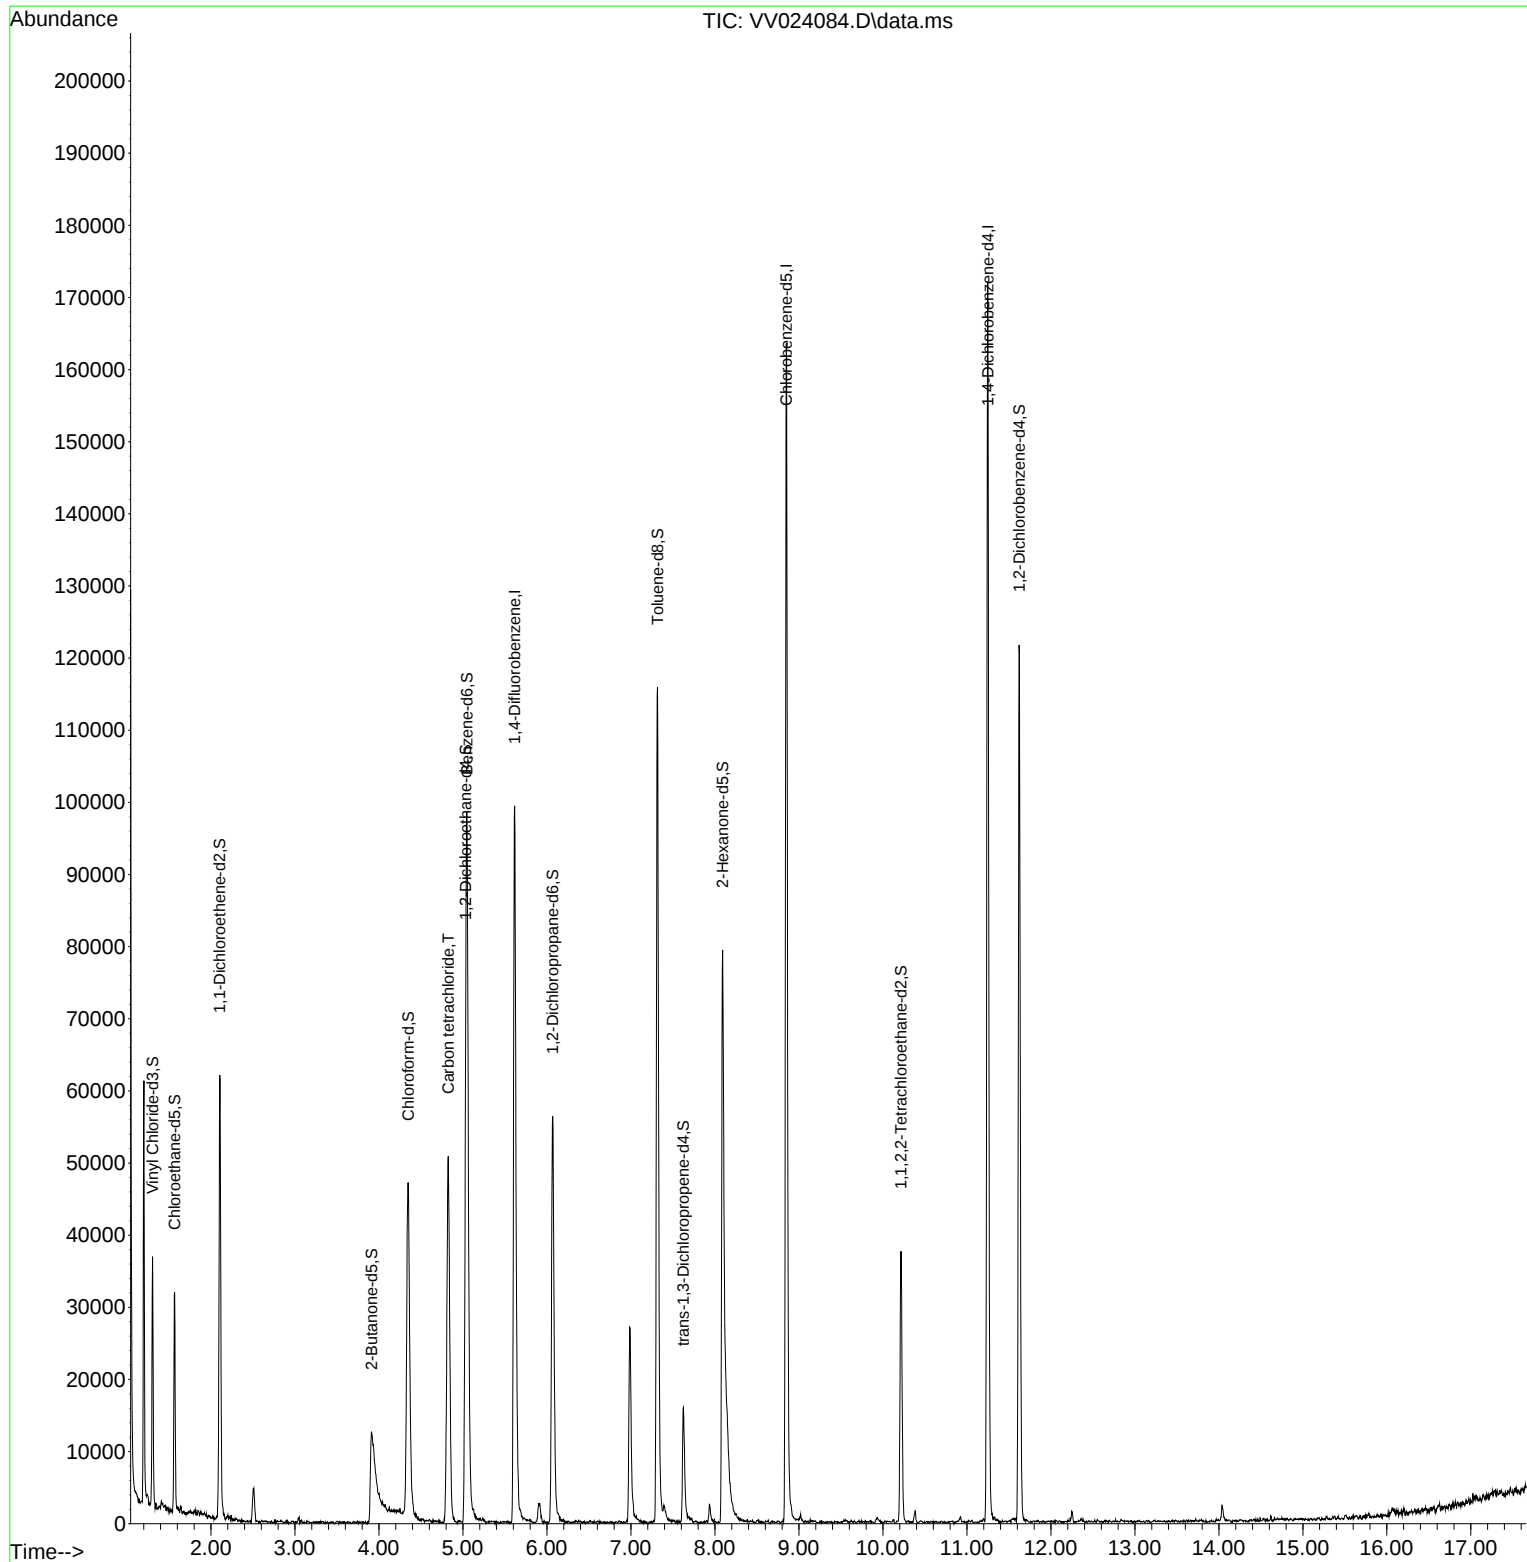

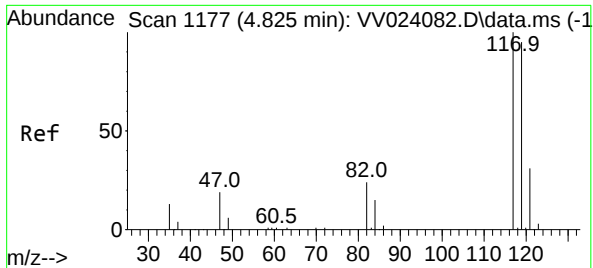

#31
Carbon tetrachloride
Concen: 3.233 ug/L
RT: 4.825 min Scan# 1177
Delta R.T. 0.000 min
Lab File: VV024084.D
Acq: 19 Dec 2021 13:00

Instrument :
MSVOA_V
ClientSampleId :
GBBJ0DL

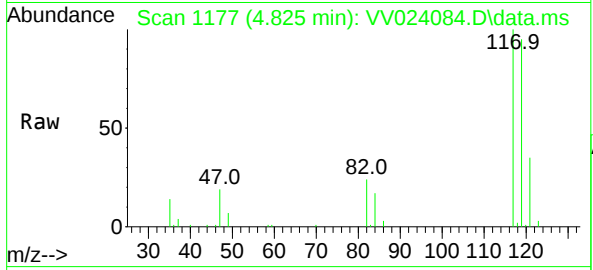

Tgt Ion:117 Resp: 37506
Ion Ratio Lower Upper
117 100
119 94.9 76.6 114.8

