

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121921\
 Data File : VW024097.D
 Acq On : 19 Dec 2021 18:38
 Operator : SY/MD
 Sample : M5134-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBLO

Manual Integrations
 APPROVED

Reviewed By : John Carlone 12/20/2021
 Supervised By : Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:39:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 20 01:35:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	92318	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	93792	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54619	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	18626	3.753	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.000%
7) Chloroethane-d5	1.568	69	17341	4.188	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.800%
11) 1,1-Dichloroethene-d2	2.108	63	29564	3.052	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.000%
20) 2-Butanone-d5	3.915	46	35047	36.146	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.300%
24) Chloroform-d	4.349	84	49148	4.372	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
26) 1,2-Dichloroethane-d4	5.034	65	22408	4.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
32) Benzene-d6	5.050	84	85300	4.592	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
36) 1,2-Dichloropropane-d6	6.069	67	25012	4.463	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.200%
41) Toluene-d8	7.317	98	77105	4.610	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	7.625	79	8855	3.808	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.200%
46) 2-Hexanone-d5	8.092	63	33799	32.472	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	64.940%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	18093	3.892	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	33656	4.613	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.200%
Target Compounds					Qvalue	
13) Acetone	2.211	43	12136m	15.645	ug/L	
14) Carbon disulfide	2.298	76	2917	0.162	ug/L	# 94
15) Methyl Acetate	2.446	43	12861	6.840	ug/L	99
25) Chloroform	4.378	83	48975	3.580	ug/L	97
31) Carbon tetrachloride	4.825	117	9221	0.799	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024097.D
Acq On : 19 Dec 2021 18:38
Operator : SY/MD
Sample : M5134-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
GBBL0

Manual Integrations
APPROVED

Reviewed By : John Carlone 12/20/2021
Supervised By : Mahesh Dadoda 12/22/2021

Quant Time: Dec 20 01:39:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 20 01:35:07 2021
Response via : Initial Calibration

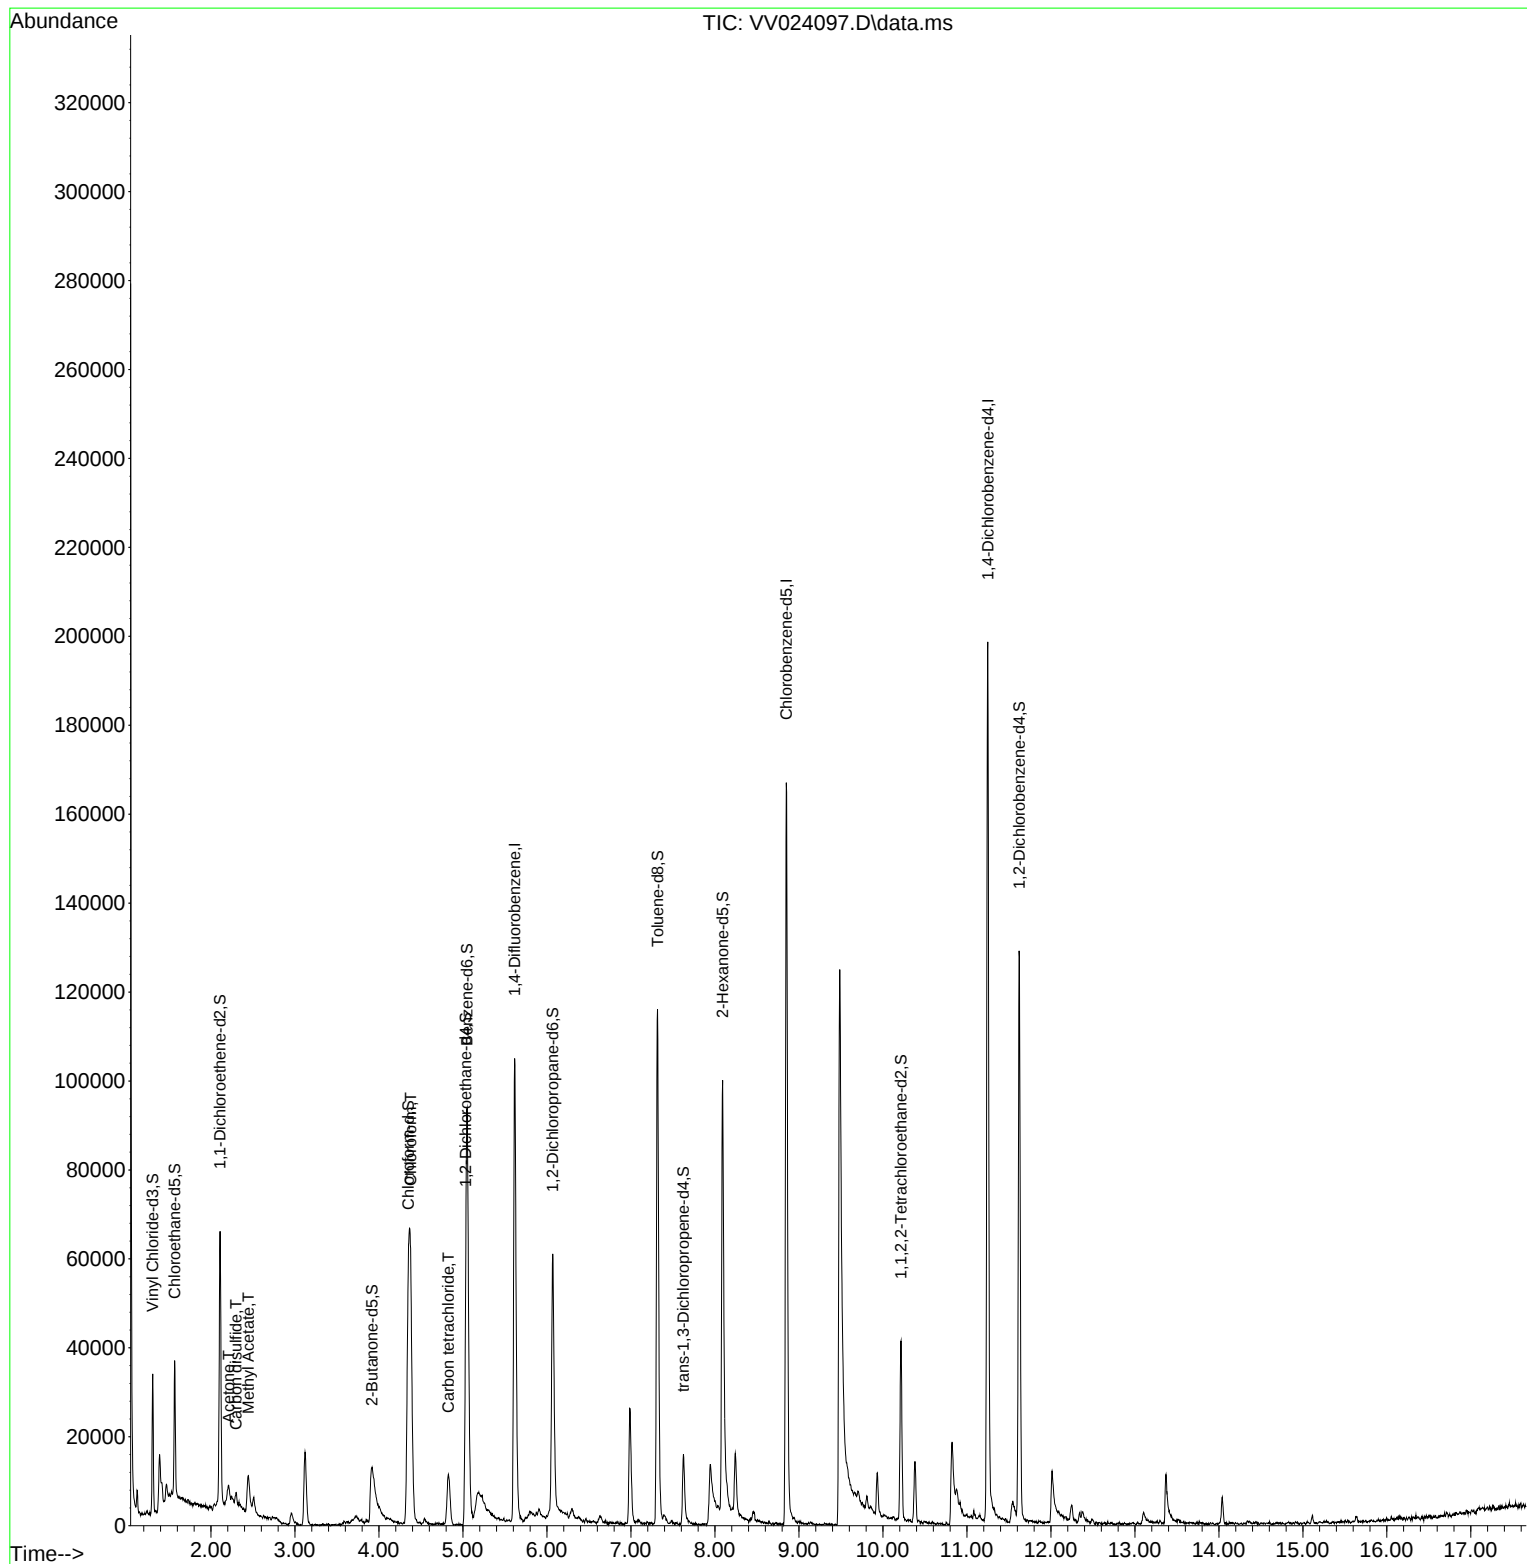

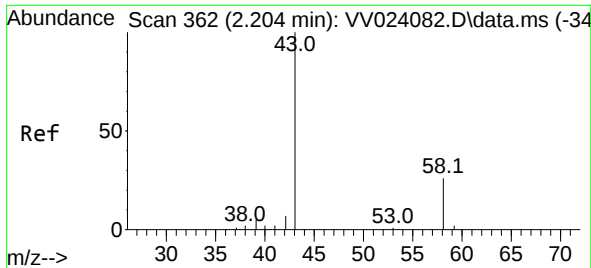

#13

Acetone

Concen: 15.645 ug/L m

RT: 2.211 min Scan# 3

Delta R.T. 0.007 min

Lab File: VV024097.D

Acq: 19 Dec 2021 18:38

Instrument :

MSVOA_V

ClientSampleId :

GBBL0

Tgt Ion: 43 Resp: 1213

Ion Ratio Lower Upper

43 100





58 14.1 0.0 41.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/20/2021

Supervised By :Mahesh Dadoda 12/22/2021

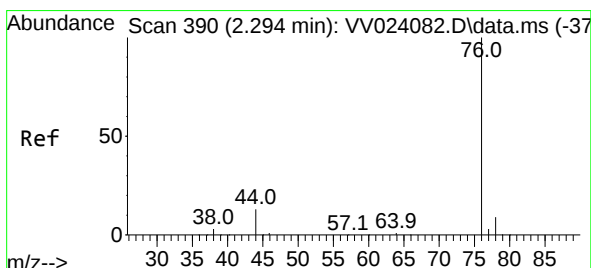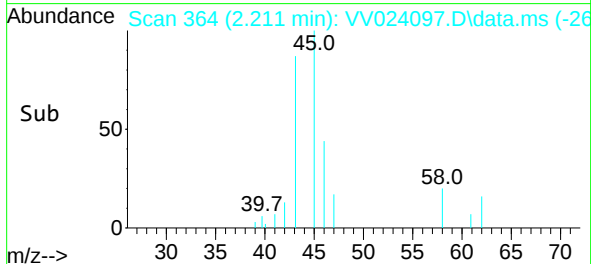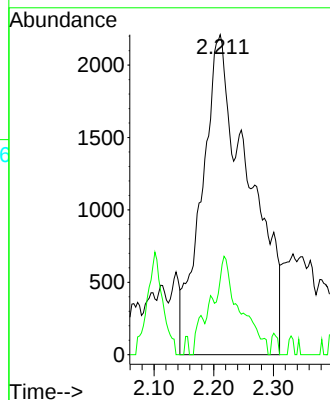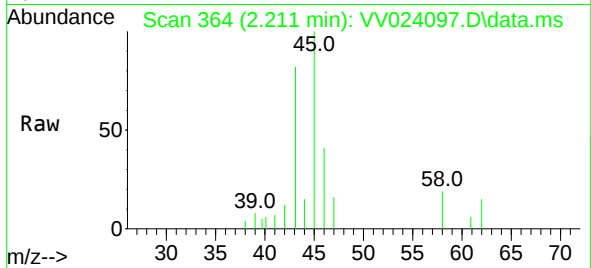

#14

Carbon disulfide

Concen: 0.162 ug/L

RT: 2.298 min Scan# 391

Delta R.T. 0.003 min

Lab File: VV024097.D




Acq: 19 Dec 2021 18:38


Tgt Ion: 76 Resp: 2917

Ion Ratio Lower Upper

76 100

78 11.7 7.5 11.3#

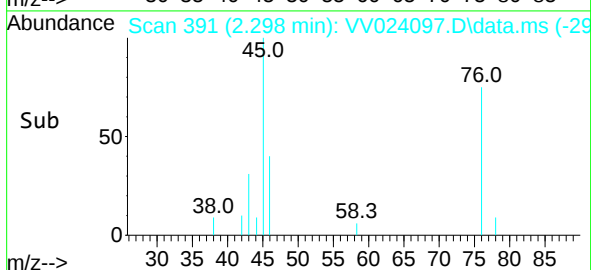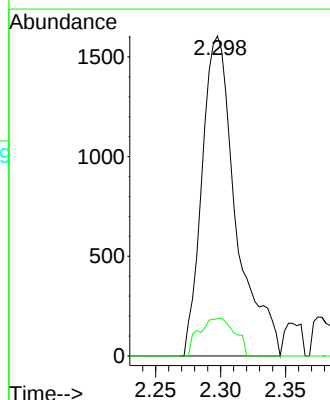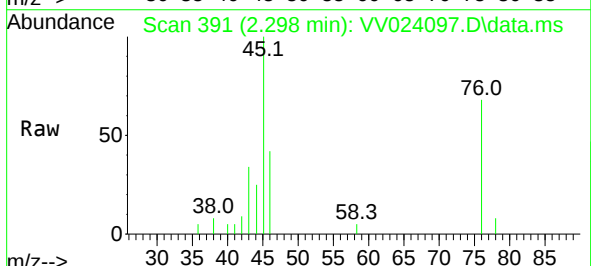

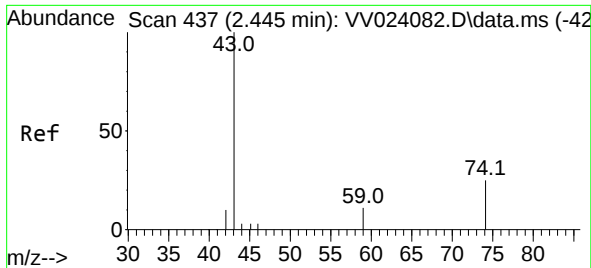





#15
Methyl Acetate
Concen: 6.840 ug/L
RT: 2.446 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV024097.D
Acq: 19 Dec 2021 18:38

Instrument :
MSVOA_V
ClientSampleId :
GBBL0

Tgt Ion: 43 Resp: 1286
Ion Ratio Lower Upper
43 100
74 25.9 20.2 30.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

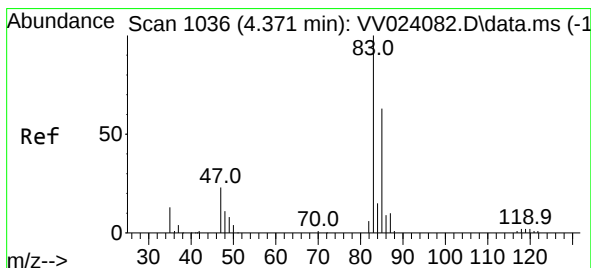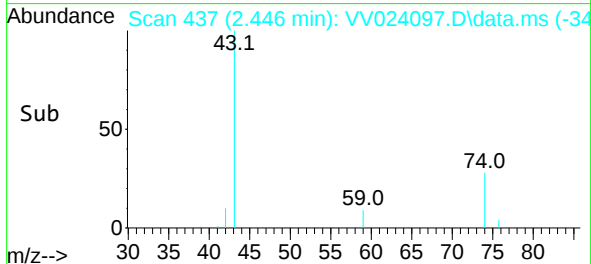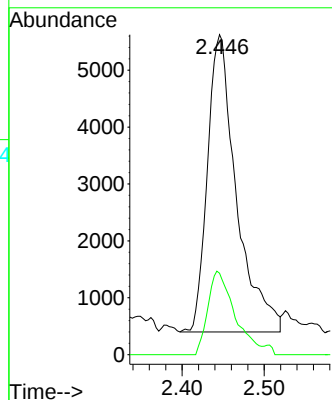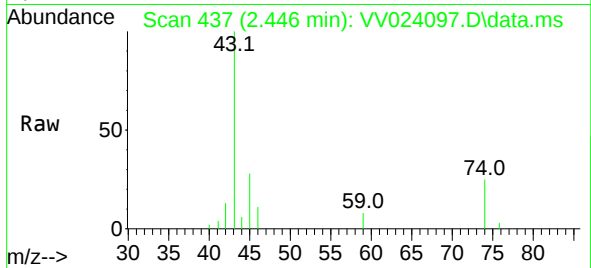

#25
Chloroform
Concen: 3.580 ug/L
RT: 4.378 min Scan# 1038
Delta R.T. 0.007 min
Lab File: VV024097.D
Acq: 19 Dec 2021 18:38


Tgt Ion: 83 Resp: 48975
Ion Ratio Lower Upper
83 100
85 67.0 45.2 84.0

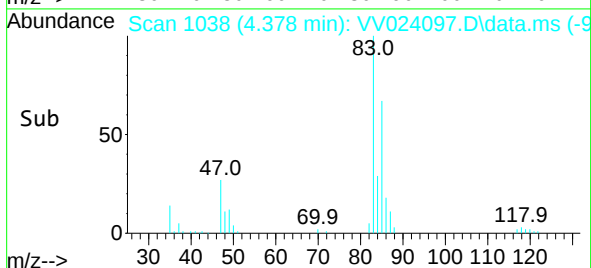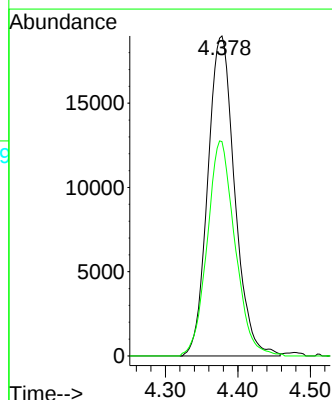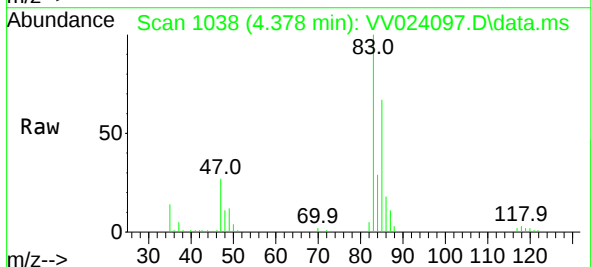

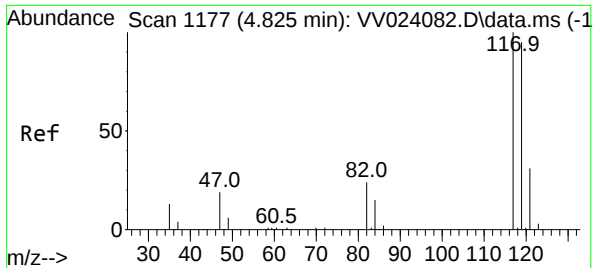

#31
Carbon tetrachloride
Concen: 0.799 ug/L
RT: 4.825 min Scan# 1177
Delta R.T. 0.000 min
Lab File: VV024097.D
Acq: 19 Dec 2021 18:38

Instrument :
MSVOA_V
ClientSampleId :
GBBL0

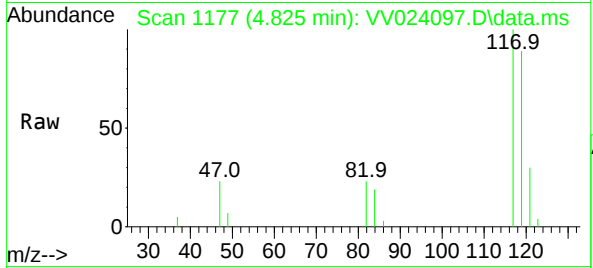

Tgt Ion:117 Resp: 922
Ion Ratio Lower Upper
117 100
119 94.9 76.6 114.8

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/22/2021

