

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024083.D
 Acq On : 19 Dec 2021 11:31
 Operator : SY/MD
 Sample : VV1219WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK282

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024083.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rBV	40867	42398	14.88%	1.738%
2	1.568	156	164	178	rBV	35963	40461	14.20%	1.659%
3	2.108	317	332	349	rBV	71269	106394	37.34%	4.362%
4	2.500	448	454	469	rVB	6148	10714	3.76%	0.439%
5	3.908	881	892	911	rBV	13176	46252	16.23%	1.896%
6	4.346	1012	1028	1052	rVB	52391	134655	47.26%	5.520%
7	5.043	1229	1245	1266	rBV2	112938	282200	99.04%	11.569%
8	5.612	1409	1422	1448	rBV	104275	211340	74.17%	8.664%
9	5.905	1502	1513	1528	rVB9	3378	7758	2.72%	0.318%
10	6.066	1550	1563	1585	rBV2	62657	132946	46.66%	5.450%
11	6.985	1839	1849	1866	rBV2	29668	55303	19.41%	2.267%
12	7.313	1940	1951	1968	rBV	132461	232911	81.74%	9.548%
13	7.394	1972	1976	1992	rVB7	2396	4561	1.60%	0.187%
14	7.622	2038	2047	2067	rBV	18322	34057	11.95%	1.396%
15	8.088	2183	2192	2231	rBV	90497	231109	81.11%	9.475%
16	8.850	2417	2429	2452	rBV	171530	284687	99.91%	11.671%
17	10.214	2842	2853	2866	rBV2	41377	68960	24.20%	2.827%
18	11.249	3163	3175	3190	rBV	182364	284931	100.00%	11.681%
19	11.622	3278	3291	3310	rBV	136550	218005	76.51%	8.937%
20	12.252	3476	3487	3496	rBV2	4283	6498	2.28%	0.266%
21	13.750	3944	3953	3960	rVB5	2114	3115	1.09%	0.128%




Sum of corrected areas: 2439255

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024083.D
Acq On : 19 Dec 2021 11:31
Operator : SY/MD
Sample : VV1219WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK282

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

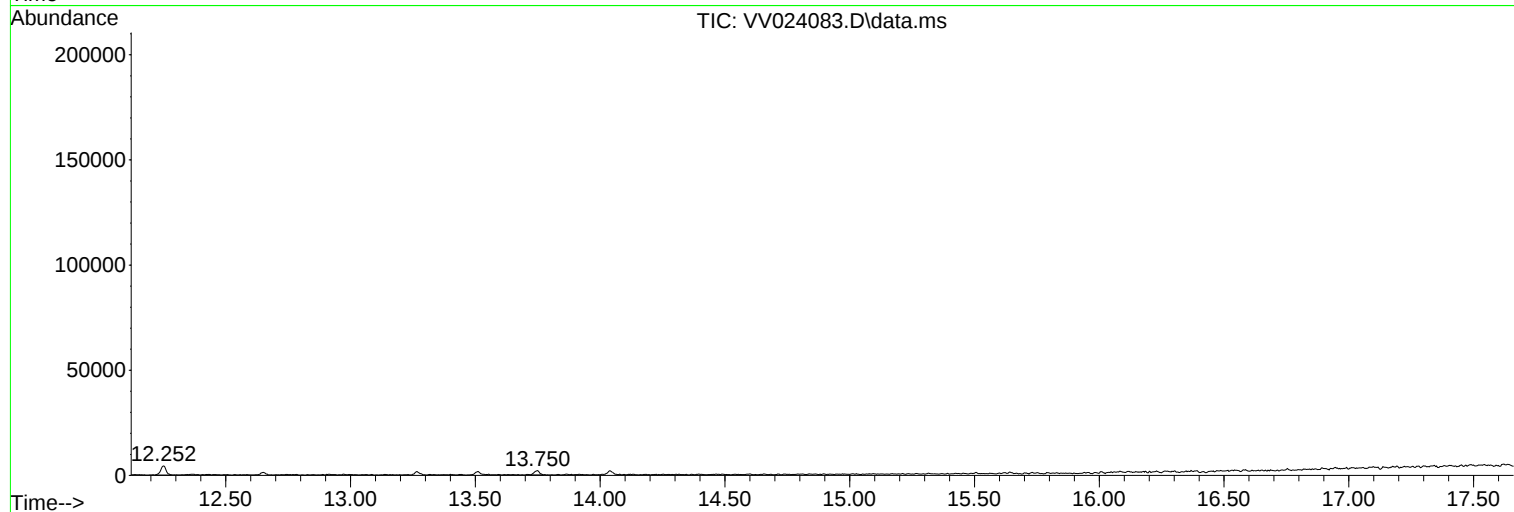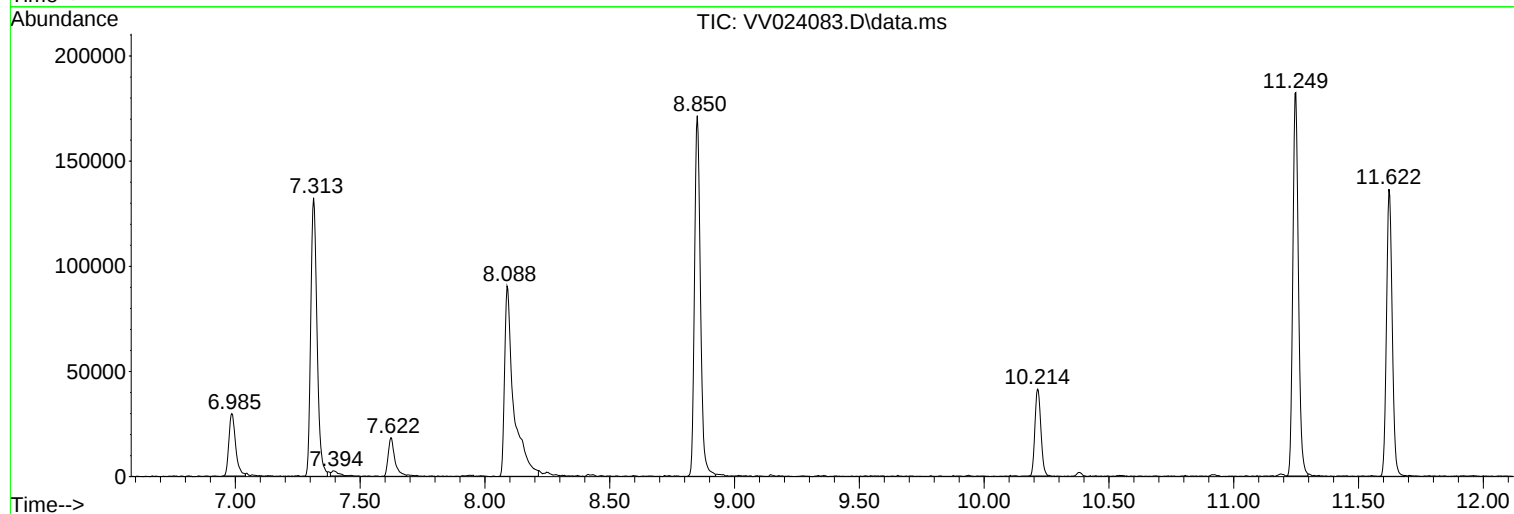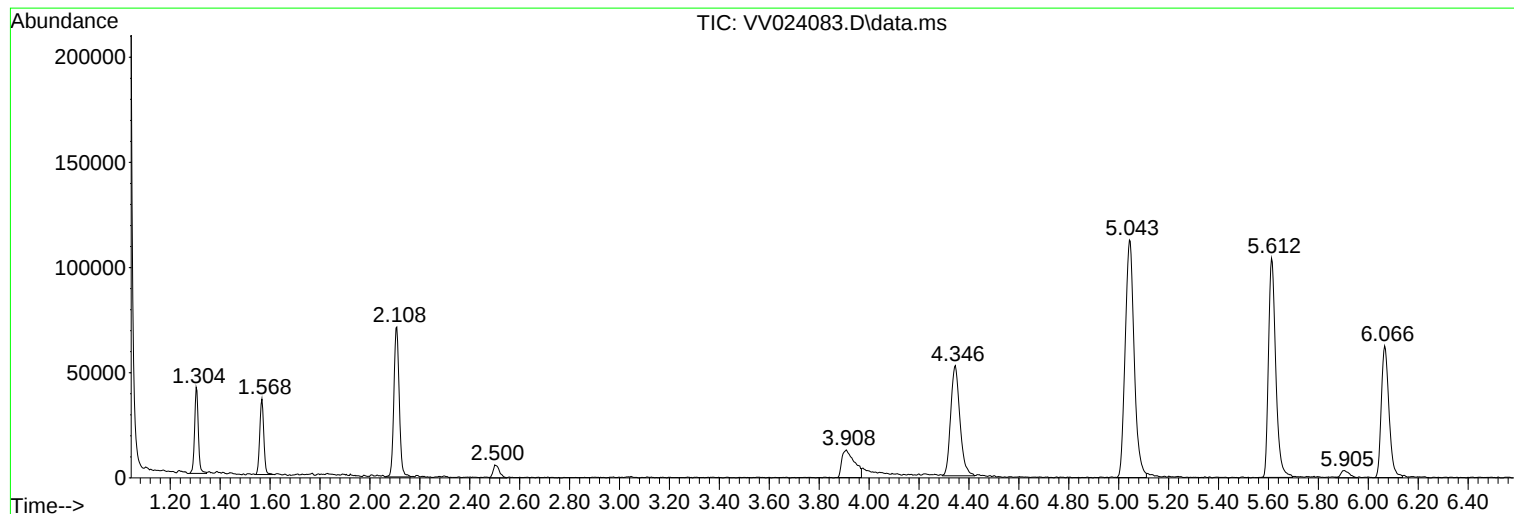

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024083.D
Acq On : 19 Dec 2021 11:31
Operator : SY/MD
Sample : VV1219WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK282

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
Data File : VV024083.D
Acq On : 19 Dec 2021 11:31
Operator : SY/MD
Sample : VV1219WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK282

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc