


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121921\
 Data File : VV024081.D
 Acq On : 19 Dec 2021 09:51
 Operator : SY/MD
 Sample : BFB255
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB255

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Dec 20 04:04:22 2021

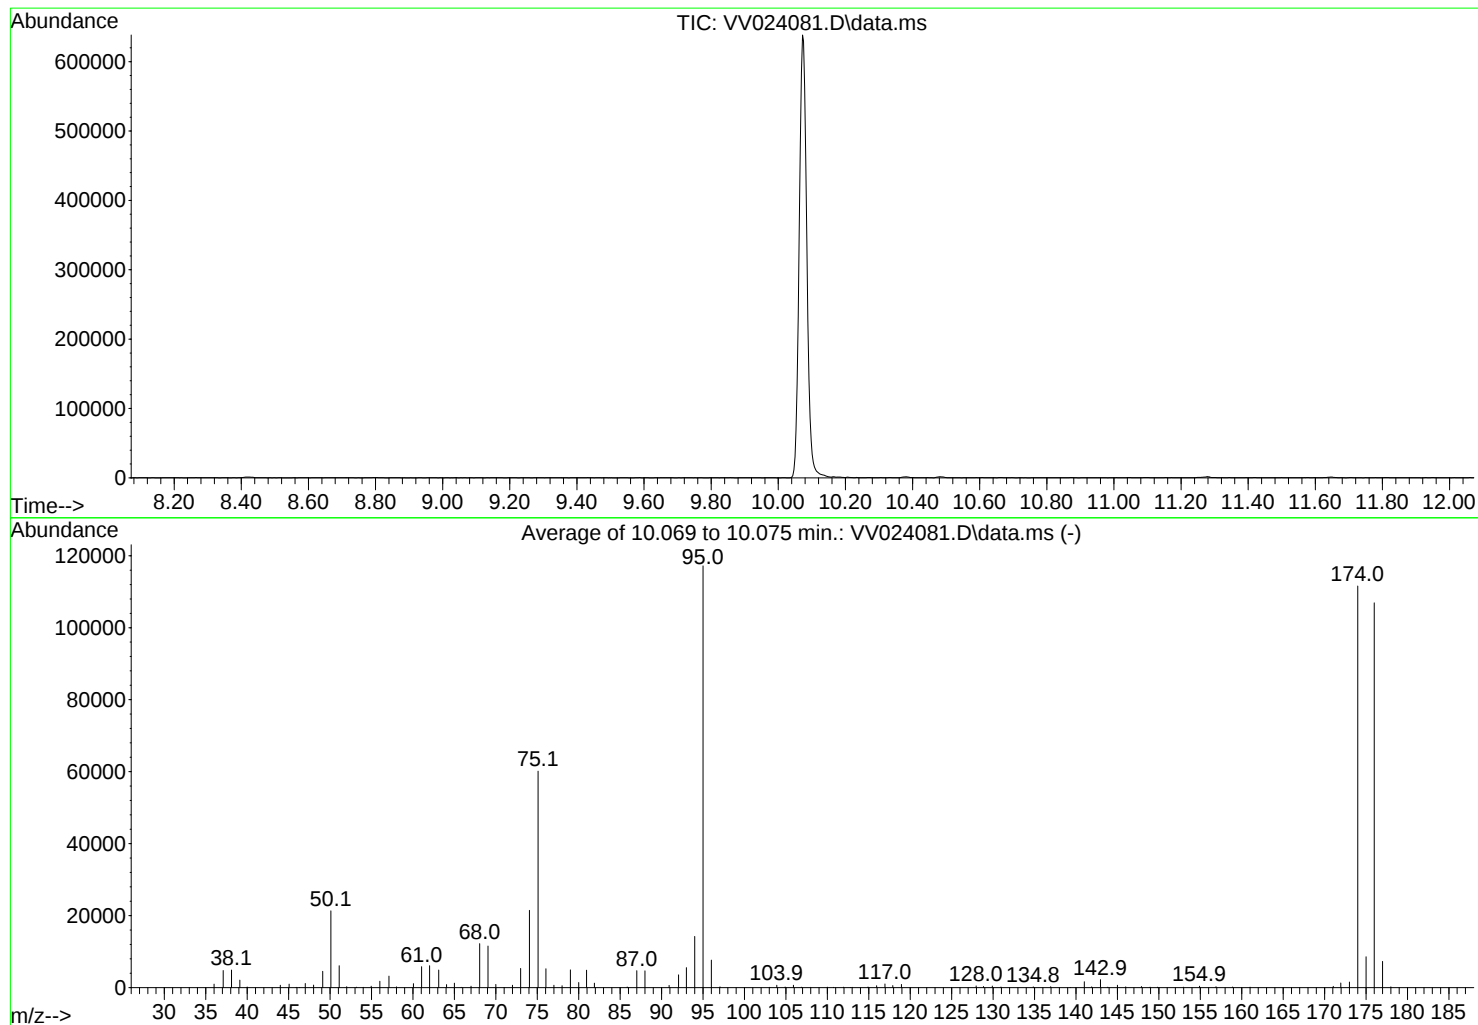

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	21344	PASS
75	95	30	80	51.3	60152	PASS
95	95	100	100	100.0	117189	PASS
96	95	5	9	6.5	7665	PASS
173	174	0.00	2	1.4	1566	PASS
174	95	50	120	95.2	111571	PASS
175	174	5	9	7.7	8562	PASS
176	174	95	105	95.8	106909	PASS
177	176	5	10	6.8	7283	PASS

m/z	Abundance
44.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
36.00	916.0
37.10	4636.0
38.10	4714.0
39.10	1991.0
40.00	122.0
44.00	715.0
45.10	939.0
45.90	156.0
47.00	975.0
48.00	658.0
49.10	4206.0
50.10	20144.0
51.10	6002.0
52.00	225.0
53.20	119.0
54.00	101.0
54.90	367.0
56.00	1645.0
57.10	2909.0
58.00	227.0
60.00	1081.0
61.10	5657.0
62.00	5801.0
63.10	4661.0
64.10	881.0
65.00	1273.0
65.80	153.0
67.00	419.0
68.00	11657.0
69.00	10967.0
70.00	890.0
72.00	576.0
73.00	5059.0
74.00	20152.0
75.10	57616.0
76.10	5106.0
77.00	623.0
78.00	525.0
79.00	4675.0
80.00	1333.0
80.90	4671.0
81.90	1141.0
85.90	174.0
87.00	4517.0
88.00	4308.0
90.90	524.0
92.00	3324.0
93.00	5234.0
94.00	13587.0
95.00	111800.0
96.00	7460.0
97.10	268.0
103.90	562.0
104.90	149.0
105.90	607.0
106.90	114.0
110.00	134.0
112.00	149.0
112.80	140.0
114.90	188.0
116.00	544.0
116.90	995.0
117.90	531.0
118.90	833.0
128.00	528.0
128.80	353.0
129.90	457.0
130.90	205.0
134.80	245.0
136.90	233.0
141.00	1542.0
141.90	239.0
142.90	2154.0
143.80	113.0
145.00	685.0
145.90	242.0
147.90	265.0
149.00	134.0
149.90	162.0
152.90	105.0
154.90	328.0
156.90	276.0
158.90	188.0
161.00	135.0
171.00	311.0
171.90	1228.0
173.00	1395.0
174.00	104360.0
175.00	8184.0
176.00	100424.0
177.00	6885.0
178.00	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
36.00	1021.0
37.10	4809.0
38.10	5145.0
39.10	2136.0
40.00	169.0
44.10	824.0
45.00	1006.0
45.90	112.0
47.00	1179.0
48.00	743.0
49.10	4650.0
50.10	22032.0
51.10	6312.0
52.00	261.0
53.20	160.0
54.00	129.0
54.90	437.0
56.00	1868.0
57.10	3378.0
58.00	243.0
60.10	1128.0
61.10	6020.0
62.00	6353.0
63.10	5066.0
64.10	902.0
65.00	1320.0
65.80	123.0
67.00	424.0
68.00	12724.0
69.10	11773.0
70.00	961.0
72.00	705.0
73.00	5448.0
74.00	22400.0
75.10	62192.0
76.10	5449.0
77.00	712.0
78.00	561.0
79.00	5075.0
80.00	1504.0
80.90	5021.0
81.90	1289.0
85.80	203.0
87.00	4892.0
88.00	4763.0
90.90	651.0
92.00	3685.0
93.00	5731.0
94.00	14679.0
95.00	121096.0
96.00	7898.0
97.10	228.0
103.10	122.0
103.90	677.0
104.90	179.0
105.90	675.0
106.80	134.0
108.00	105.0
110.00	135.0
110.70	107.0
111.90	146.0
113.00	168.0
114.90	194.0
115.90	561.0
116.90	1021.0
117.90	609.0
119.00	921.0
128.00	508.0
128.90	323.0
129.90	461.0
130.90	186.0
134.80	252.0
136.90	248.0
139.30	103.0
141.00	1732.0
141.90	226.0
142.90	2252.0
143.90	145.0
145.00	715.0
146.00	248.0
147.90	343.0
148.90	169.0
149.80	154.0
153.00	151.0
154.90	428.0
156.90	287.0
158.90	185.0
161.00	145.0
171.10	363.0
172.00	1376.0
173.00	1634.0
174.00	115384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

175.00	8820.0
176.00	110480.0
177.00	7527.0
178.00	239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
36.00	1035.0
37.10	4792.0
38.10	4886.0
39.10	2105.0
40.00	191.0
44.10	827.0
45.00	999.0
46.30	171.0
47.00	1280.0
48.00	771.0
49.10	4699.0
50.10	21856.0
51.10	5950.0
52.00	289.0
53.20	181.0
54.00	116.0
55.00	428.0
56.00	1892.0
57.10	3318.0
58.00	214.0
60.10	1120.0
61.00	5844.0
62.00	6150.0
63.10	5003.0
64.00	825.0
65.00	1155.0
67.00	333.0
68.10	12325.0
69.10	11938.0
70.00	878.0
71.00	128.0
72.00	720.0
73.00	5451.0
74.10	21928.0
75.10	60648.0
76.00	5166.0
77.00	686.0
78.00	550.0
79.00	5027.0
80.00	1409.0
81.00	4900.0
81.90	1357.0
85.80	190.0
87.00	4748.0
88.00	4887.0
90.90	655.0
92.10	3710.0
93.00	5742.0
94.00	14477.0
95.00	118672.0
96.00	7636.0
97.00	239.0
103.00	115.0
103.90	714.0
104.90	179.0
105.90	672.0
106.80	129.0
108.00	128.0
110.00	126.0
110.80	133.0
111.90	166.0
113.00	170.0
114.90	177.0
115.90	504.0
117.00	997.0
117.90	613.0
119.00	919.0
127.90	452.0
128.90	272.0
129.90	468.0
131.00	197.0
134.90	240.0
137.00	263.0
141.00	1698.0
141.90	193.0
143.00	2224.0
143.90	150.0
145.00	619.0
146.10	234.0
147.90	338.0
148.90	170.0
149.80	140.0
153.00	169.0
154.90	483.0
156.90	263.0
158.90	162.0
161.00	148.0
171.10	378.0
172.00	1315.0
173.00	1668.0
174.00	114968.0
175.00	8683.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

176.00	109824.0
177.00	7438.0
178.00	241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255