

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW121922\  
 Data File : VW029712.D  
 Acq On : 19 Dec 2022 11:32  
 Operator : SY/MD  
 Sample : N6075-01 10X  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BGSL8

Quant Time: Dec 20 00:51:54 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM120722WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Dec 20 00:50:16 2022  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|---------|-------|----------|----------|--------|----------|
| -----                         |         |       |          |          |        |          |
| Internal Standards            |         |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.609   | 114   | 488733   | 50.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.844   | 117   | 460232   | 50.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.239  | 152   | 239484   | 50.000   | ug/L   | 0.00     |
|                               |         |       |          |          |        |          |
| System Monitoring Compounds   |         |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.304   | 65    | 141053   | 47.131   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 135 | Recovery | =      | 94.260%  |
| 7) Chloroethane-d5            | 1.561   | 69    | 117917   | 51.670   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 130 | Recovery | =      | 103.340% |
| 11) 1,1-Dichloroethene-d2     | 2.105   | 63    | 183936   | 39.404   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =      | 78.800%  |
| 21) 2-Butanone-d5             | 3.873   | 46    | 169120   | 92.634   | ug/L   | 0.00     |
| Spiked Amount                 | 100.000 | Range | 40 - 130 | Recovery | =      | 92.630%  |
| 24) Chloroform-d              | 4.339   | 84    | 252043   | 44.753   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 89.500%  |
| 26) 1,2-Dichloroethane-d4     | 5.024   | 65    | 148534   | 46.178   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 92.360%  |
| 32) Benzene-d6                | 5.043   | 84    | 546325   | 44.925   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 89.840%  |
| 36) 1,2-Dichloropropane-d6    | 6.063   | 67    | 169503   | 45.632   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 120 | Recovery | =      | 91.260%  |
| 41) Toluene-d8                | 7.307   | 98    | 495099   | 43.209   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =      | 86.420%  |
| 43) trans-1,3-Dichloroprop... | 7.613   | 79    | 71326    | 38.026   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =      | 76.060%  |
| 47) 2-Hexanone-d5             | 8.082   | 63    | 139965   | 88.238   | ug/L   | 0.00     |
| Spiked Amount                 | 100.000 | Range | 45 - 130 | Recovery | =      | 88.240%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.207  | 84    | 229575   | 43.250   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 65 - 120 | Recovery | =      | 86.500%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.612  | 152   | 190573   | 41.803   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =      | 83.600%  |
|                               |         |       |          |          |        |          |
| Target Compounds              |         |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.163   | 43    | 6663     | 5.602    | ug/L   | 99       |
| -----                         |         |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV121922\  
Data File : VV029712.D  
Acq On : 19 Dec 2022 11:32  
Operator : SY/MD  
Sample : N6075-01 10X  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BGSL8

Quant Time: Dec 20 00:51:54 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM120722WMA.M  
Quant Title : VOC Analysis  
QLast Update : Tue Dec 20 00:50:16 2022  
Response via : Initial Calibration

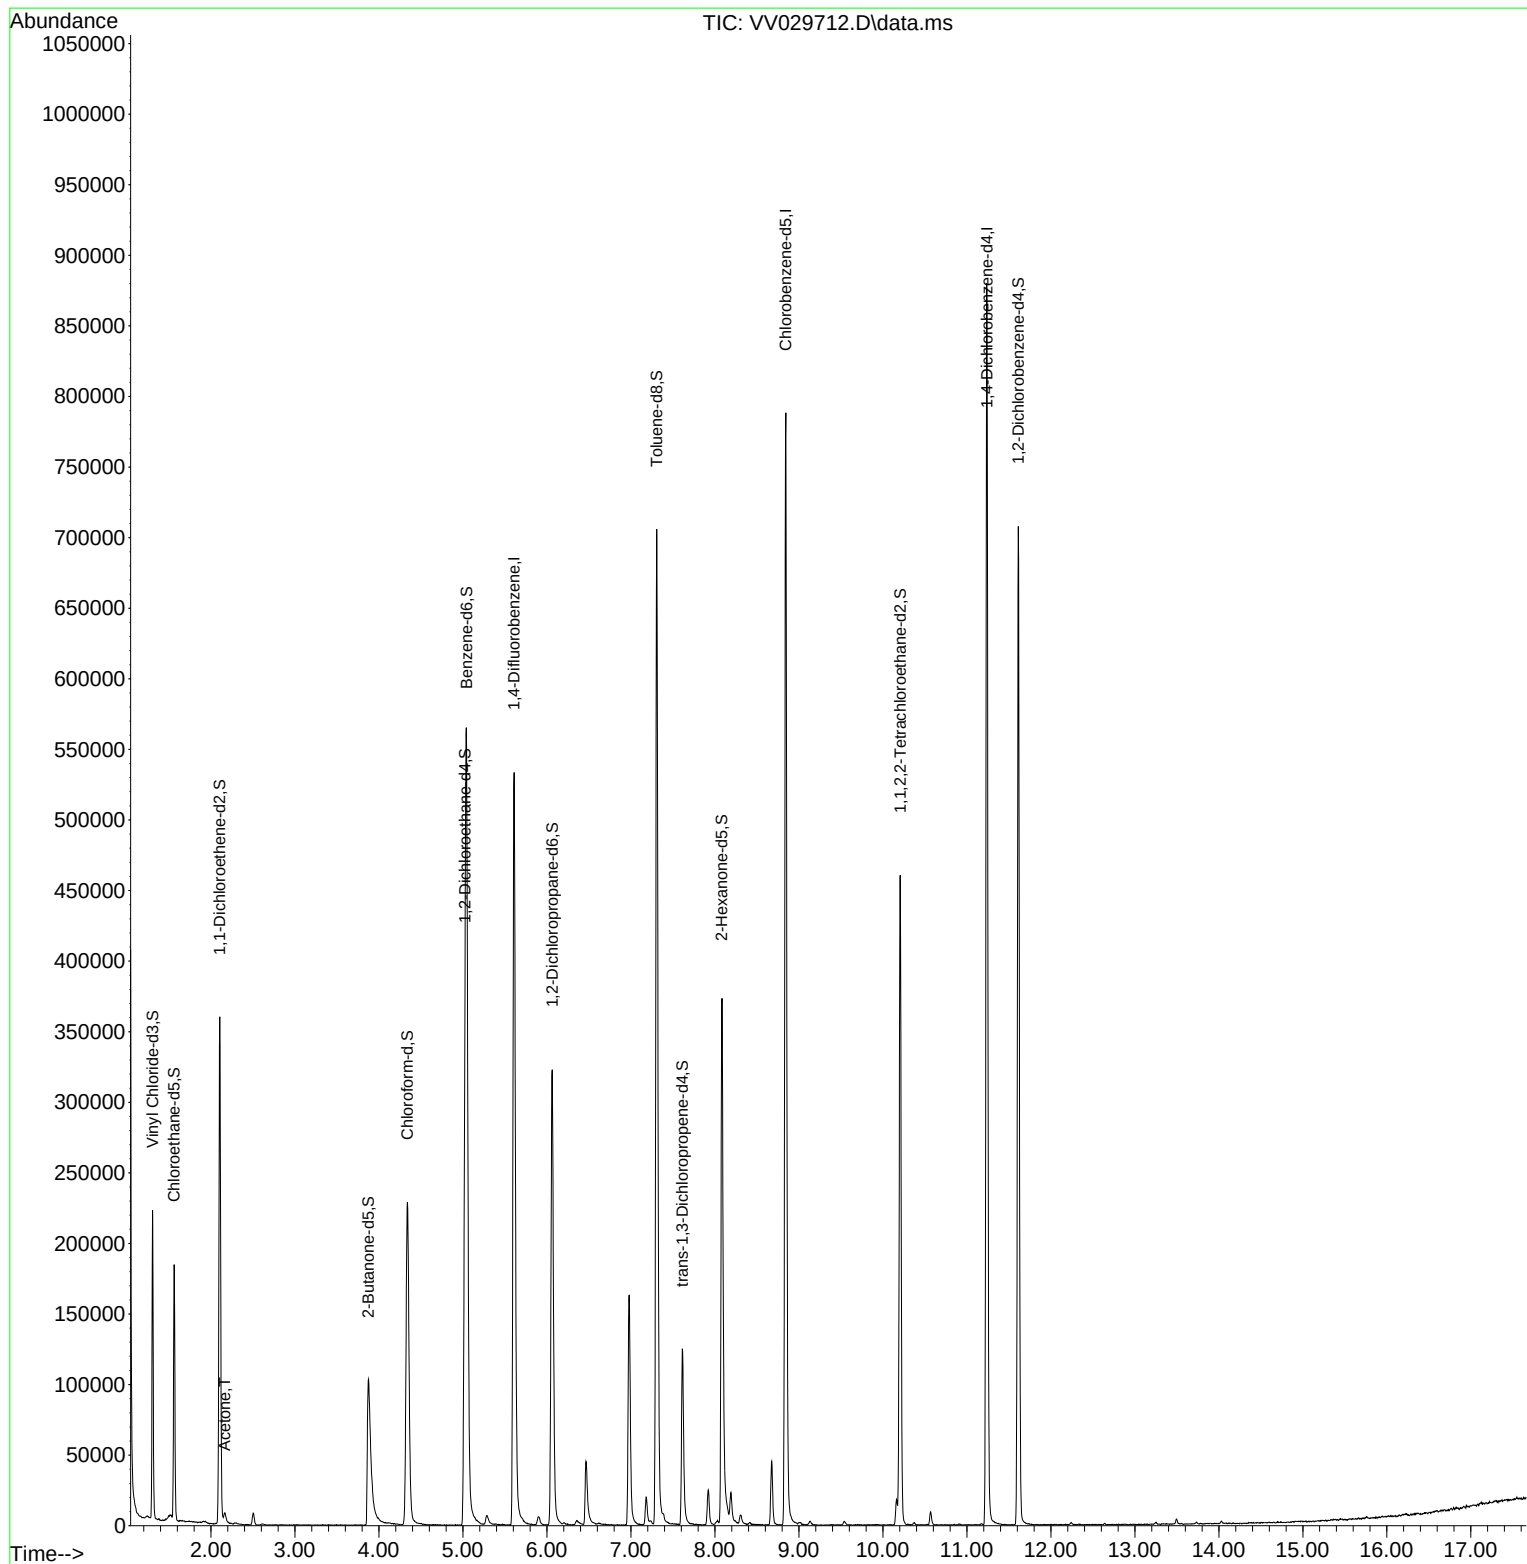

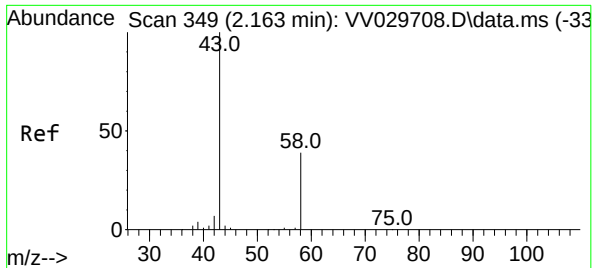

#13  
 Acetone  
 Concen: 5.602 ug/L  
 RT: 2.163 min Scan# 34  
 Delta R.T. -0.000 min  
 Lab File: VV029712.D  
 Acq: 19 Dec 2022 11:32

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BGSL8

Tgt Ion: 43 Resp: 6663  
 Ion Ratio Lower Upper  
 43 100  
 58 37.0 0.0 74.8

