

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029721.D
 Acq On : 19 Dec 2022 15:03
 Operator : SY/MD
 Sample : N6093-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN6

Quant Time: Dec 20 00:53:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 20 00:50:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	488916	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	456985	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	239553	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	134846	45.040	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.080%		
7) Chloroethane-d5	1.561	69	112990	49.493	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.980%		
11) 1,1-Dichloroethene-d2	2.105	63	179339	38.405	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.800%		
21) 2-Butanone-d5	3.873	46	169529	92.823	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.820%		
24) Chloroform-d	4.339	84	247398	43.912	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.820%		
26) 1,2-Dichloroethane-d4	5.024	65	146643	45.573	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.140%		
32) Benzene-d6	5.043	84	532878	44.130	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.260%		
36) 1,2-Dichloropropane-d6	6.063	67	168044	45.560	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.120%		
41) Toluene-d8	7.307	98	476612	41.891	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.780%		
43) trans-1,3-Dichloroprop...	7.612	79	69704	37.425	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.860%		
47) 2-Hexanone-d5	8.082	63	139084	88.306	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.310%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	231554	43.932	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.860%		
66) 1,2-Dichlorobenzene-d4	11.612	152	197644	43.341	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.680%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.105	101	1739	0.681	ug/L	# 20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029721.D
Acq On : 19 Dec 2022 15:03
Operator : SY/MD
Sample : N6093-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN6

Quant Time: Dec 20 00:53:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 20 00:50:16 2022
Response via : Initial Calibration

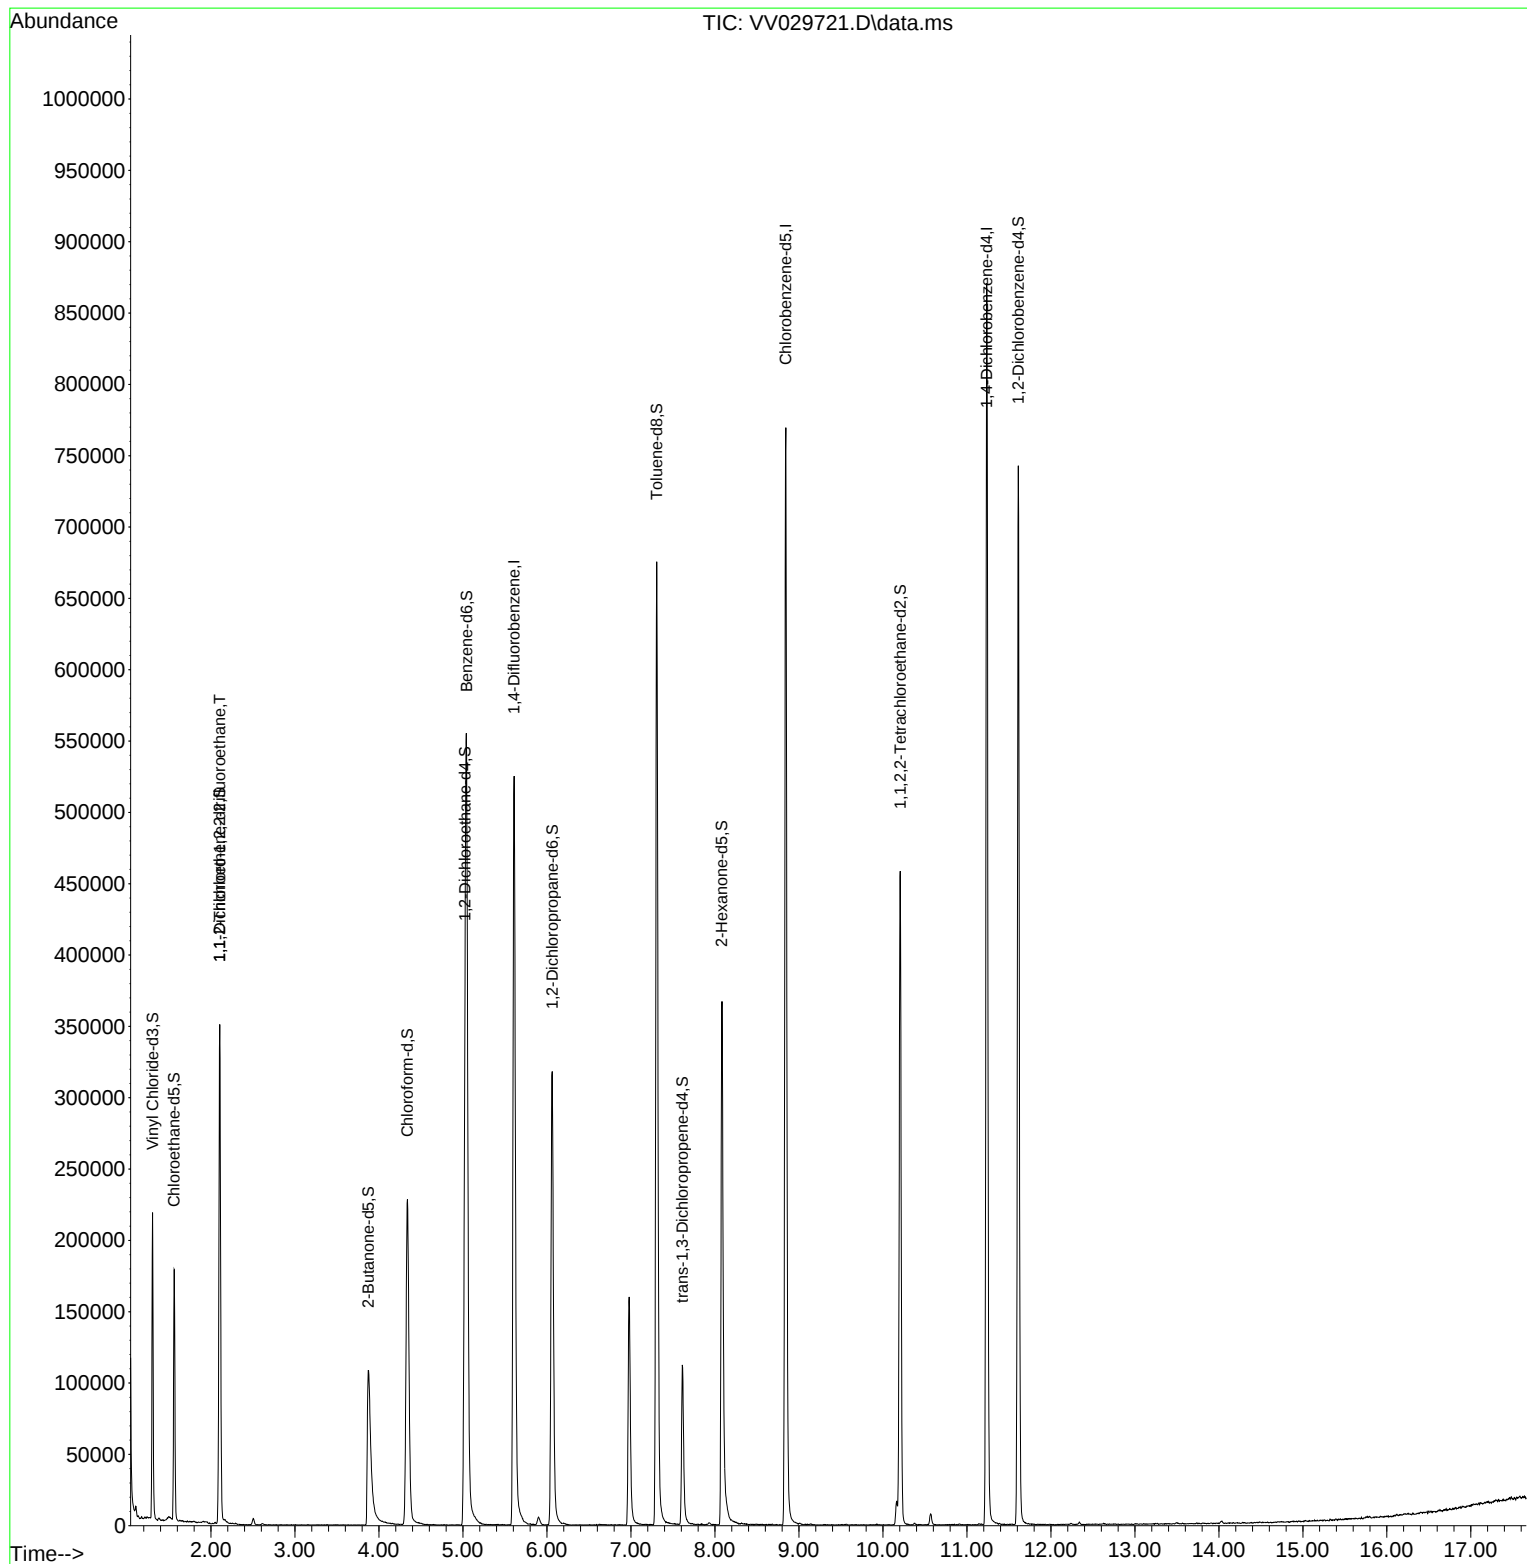

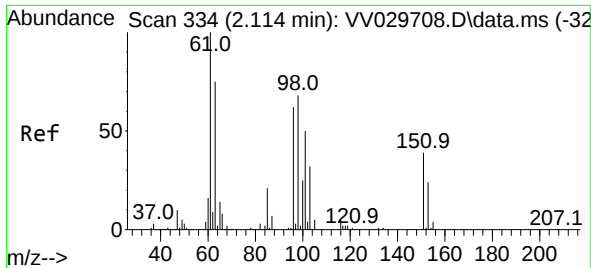

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.681 ug/L
 RT: 2.105 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV029721.D
 Acq: 19 Dec 2022 15:03

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN6

Tgt Ion:101 Resp: 1739
 Ion Ratio Lower Upper
 101 100
 85 4.0 33.6 50.4#
 151 0.0 63.5 95.3#

